
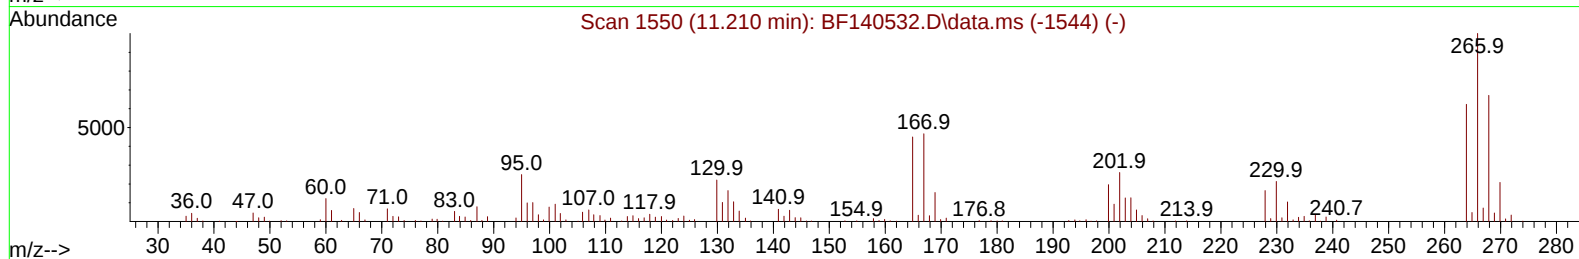
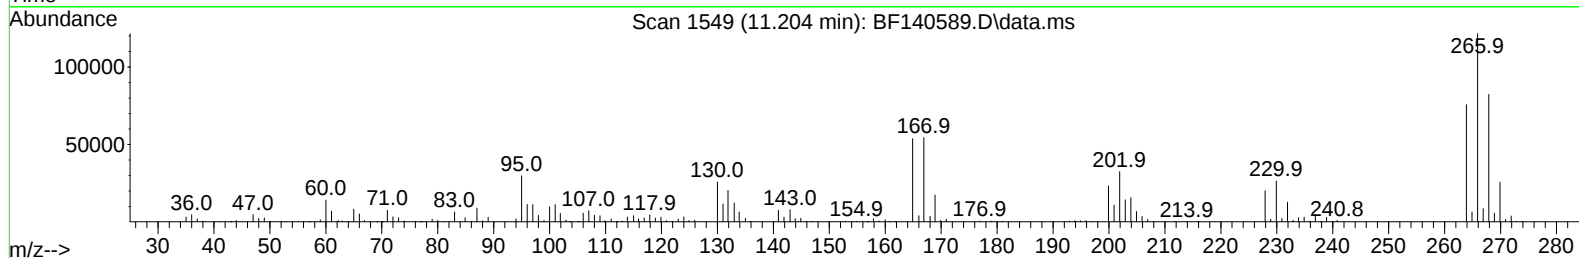


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140589.D
Acq On : 25 Nov 2024 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 10:32:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

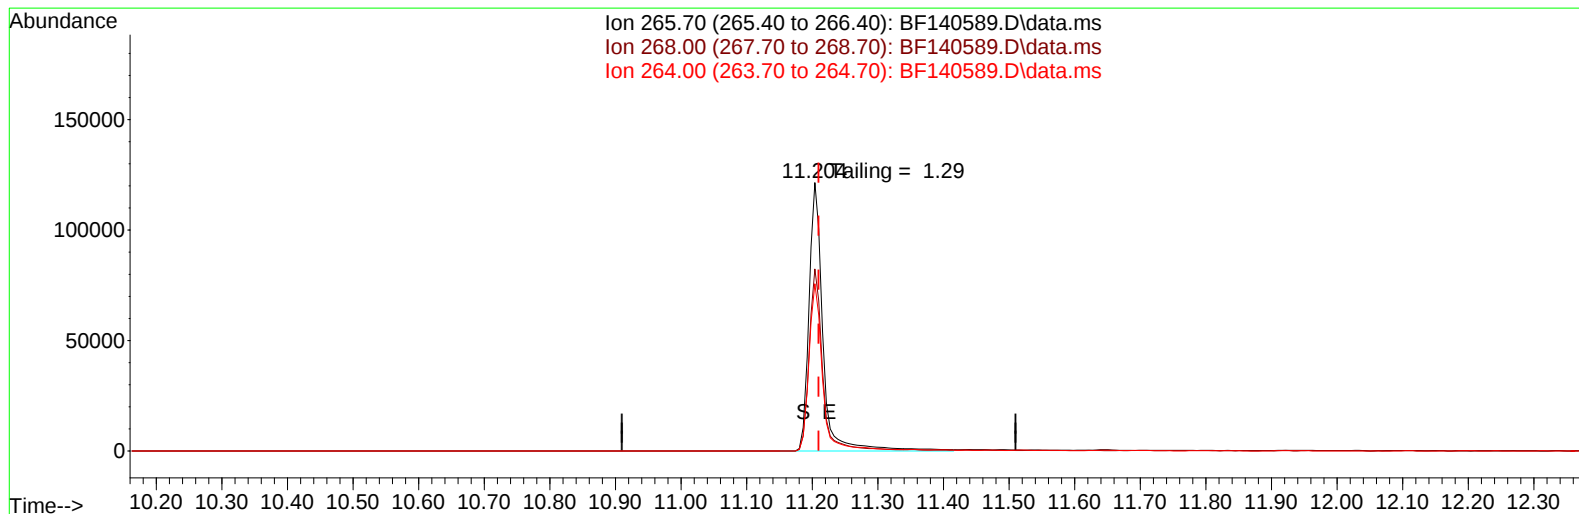

TIC: BF140589.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.006) 31422.92 ng

response 179265

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	67.82
264.00	62.30	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140589.D
Acq On : 25 Nov 2024 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 10:32:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

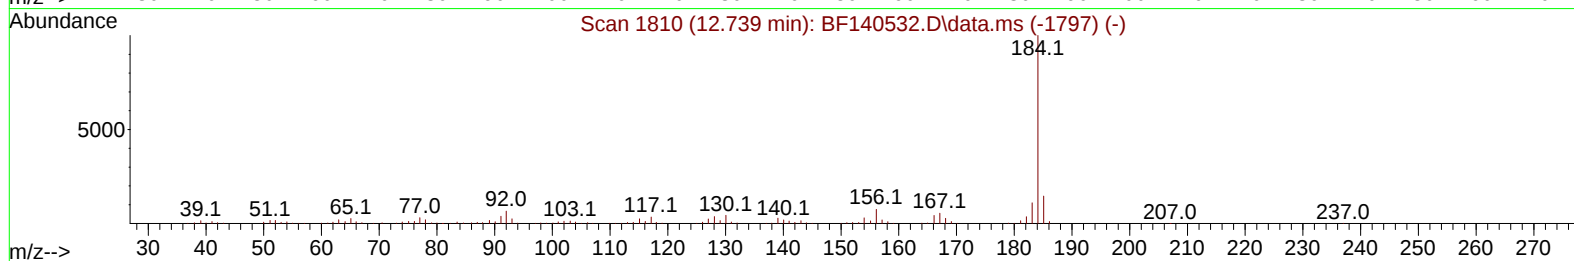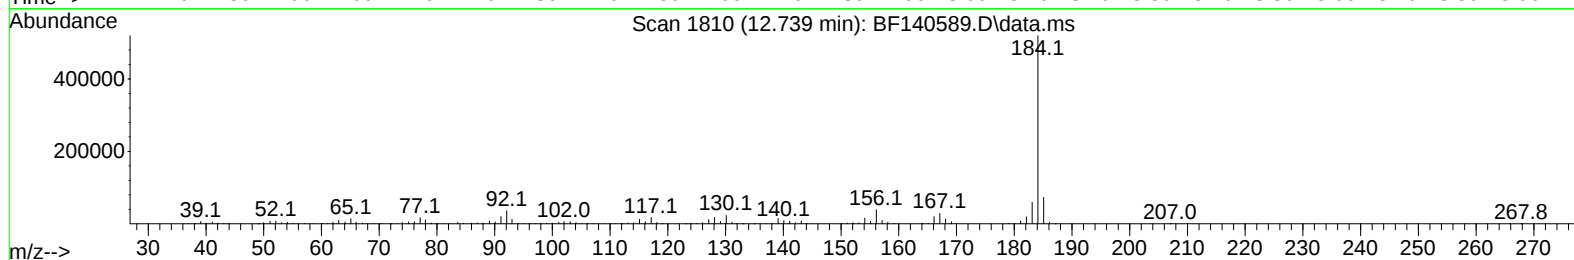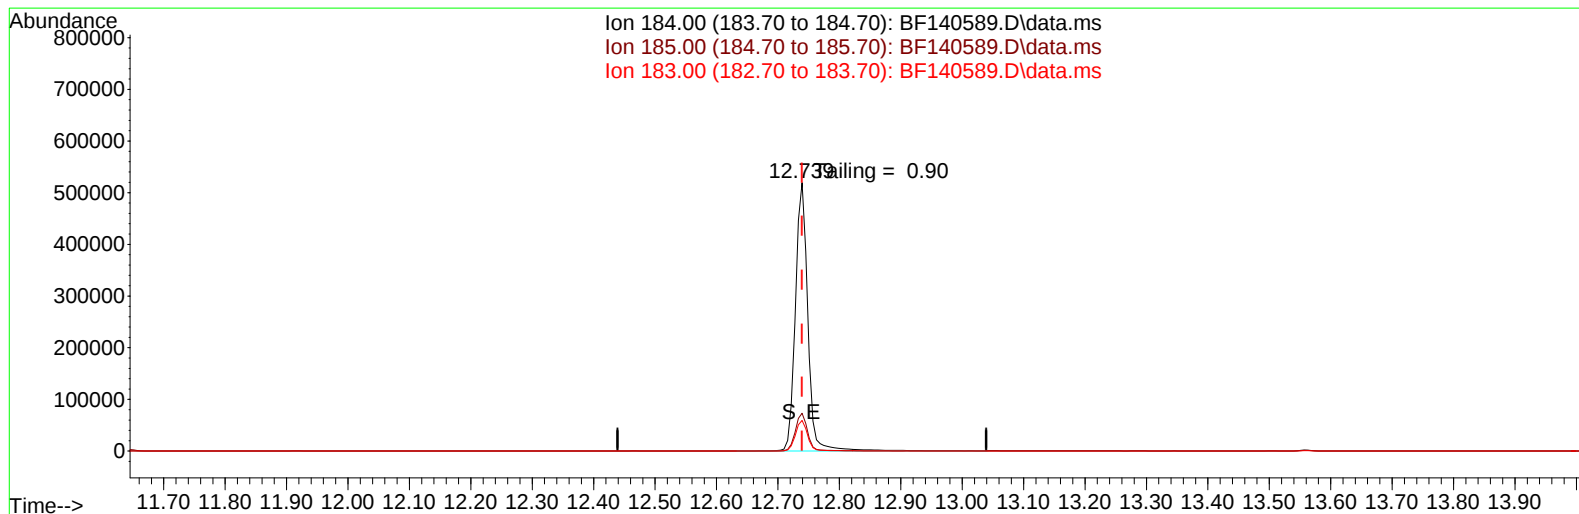

TIC: BF140589.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 27658.53 ng

response 736607

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.07
183.00	11.00	11.40
0.00	0.00	0.00