
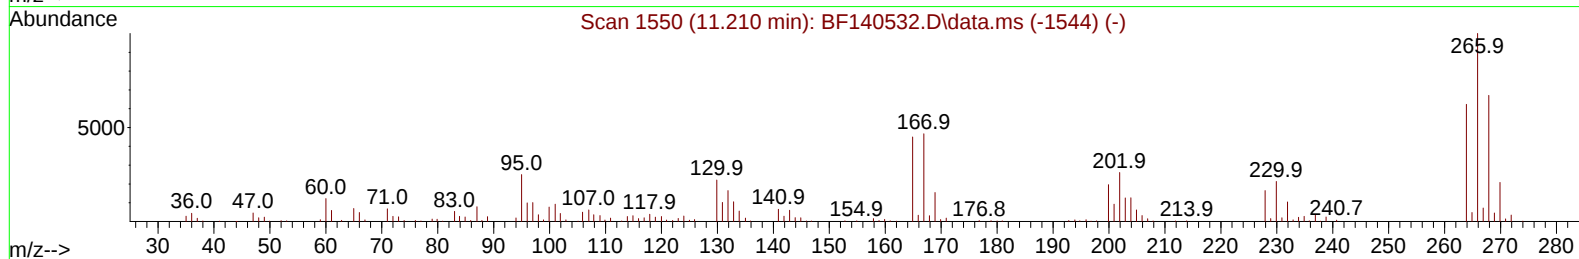
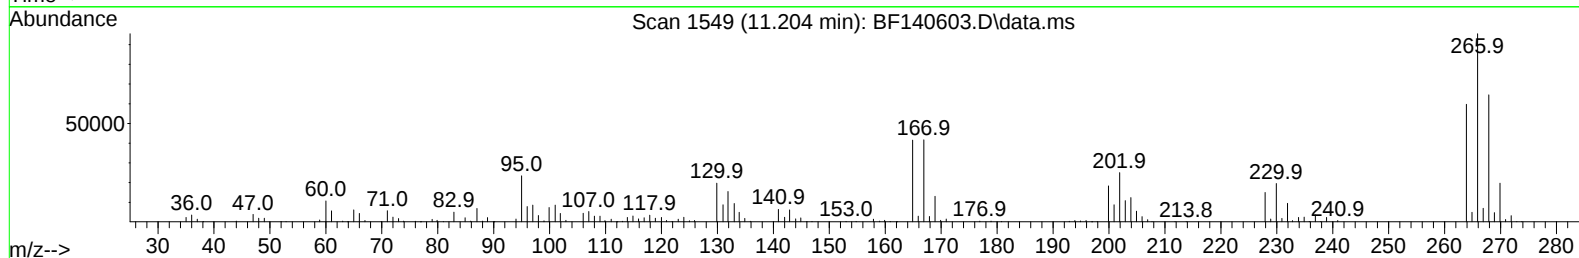


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140603.D
Acq On : 25 Nov 2024 15:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 15:47:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

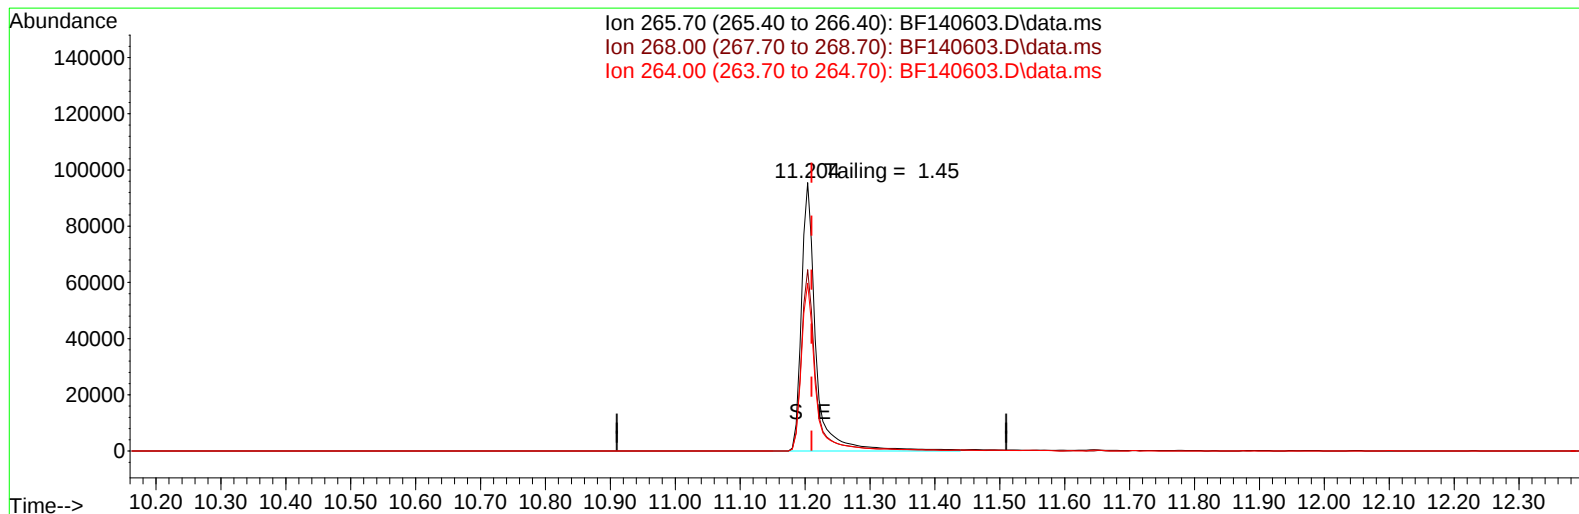

TIC: BF140603.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.006) 19738.30 ng

response 147516

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	67.54
264.00	62.30	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140603.D
Acq On : 25 Nov 2024 15:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 15:47:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

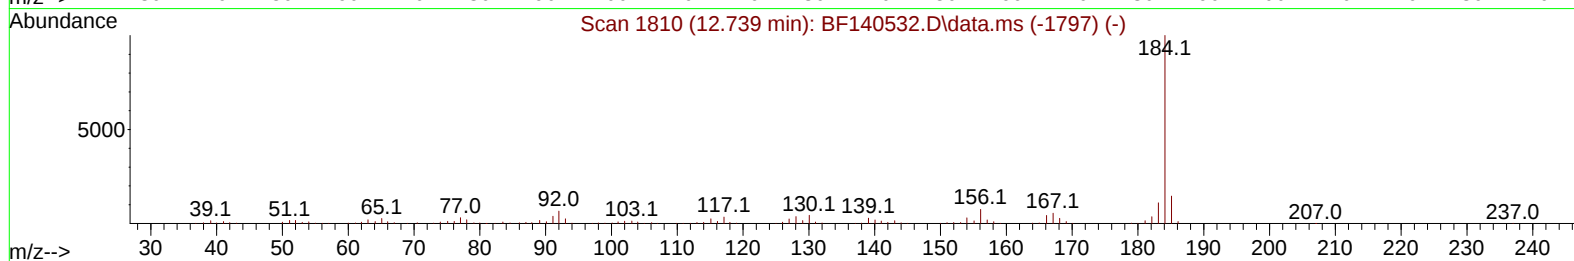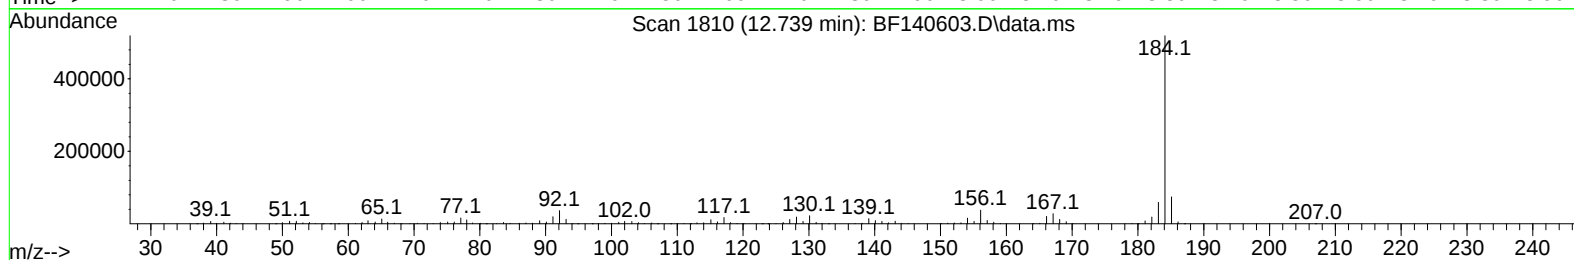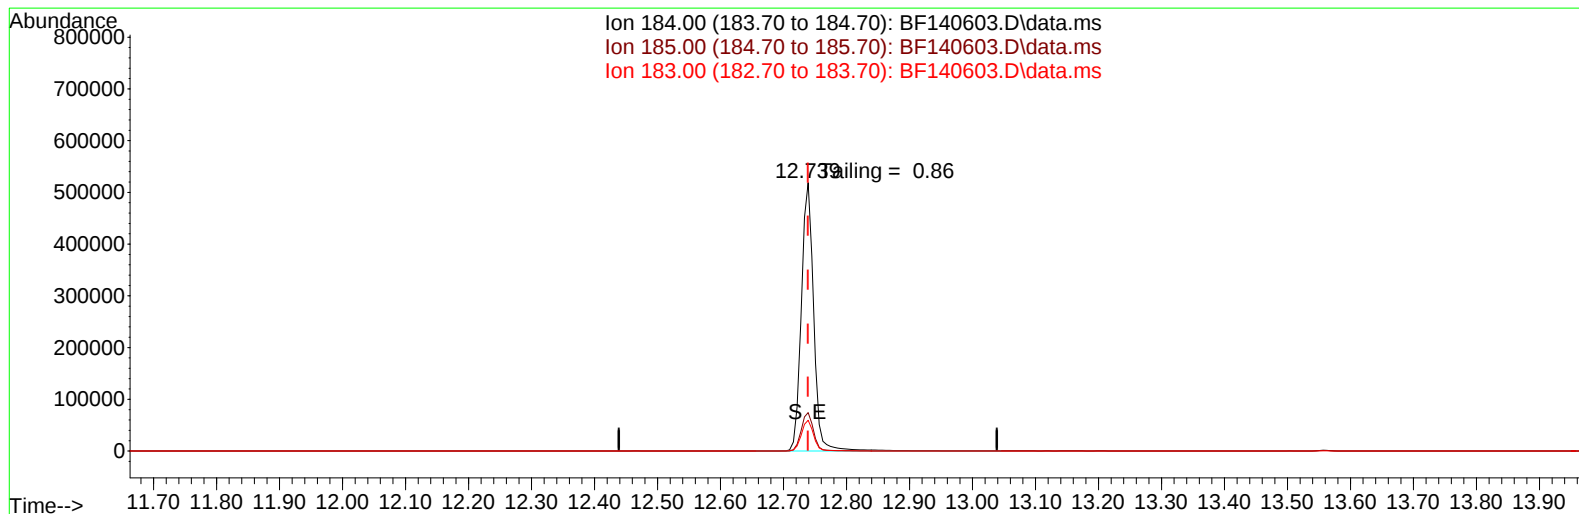

TIC: BF140603.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 26793.97 ng

response 714361

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.33
183.00	11.00	11.43
0.00	0.00	0.00