

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140601.D
Acq On : 25 Nov 2024 14:28
Operator : RC/JU
Sample : PB165152BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165152BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	11	25	32	rVB	34244	63804	1.61%	0.281%
2	5.510	575	581	586	rBV	2204989	2961294	74.74%	13.054%
3	6.504	744	750	770	rBV	2011018	3003080	75.80%	13.238%
4	6.869	807	812	817	rBV	490276	604561	15.26%	2.665%
5	7.428	901	907	924	rBV	1381583	2003501	50.57%	8.832%
6	8.145	1023	1029	1042	rBV	561255	784132	19.79%	3.457%
7	9.222	1205	1212	1243	rBV	2797087	3961932	100.00%	17.465%
8	9.904	1321	1328	1348	rVB	684222	919029	23.20%	4.051%
9	10.698	1457	1463	1488	rBV	1696800	2327294	58.74%	10.259%
10	11.398	1576	1582	1605	rVB	734623	989235	24.97%	4.361%
11	12.986	1846	1852	1857	rBV	2953701	3917606	98.88%	17.270%
12	14.057	2029	2034	2049	rBV	457806	634355	16.01%	2.796%
13	15.580	2286	2293	2313	rBV	290609	514817	12.99%	2.269%




Sum of corrected areas: 22684640

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140601.D
Acq On : 25 Nov 2024 14:28
Operator : RC/JU
Sample : PB165152BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165152BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

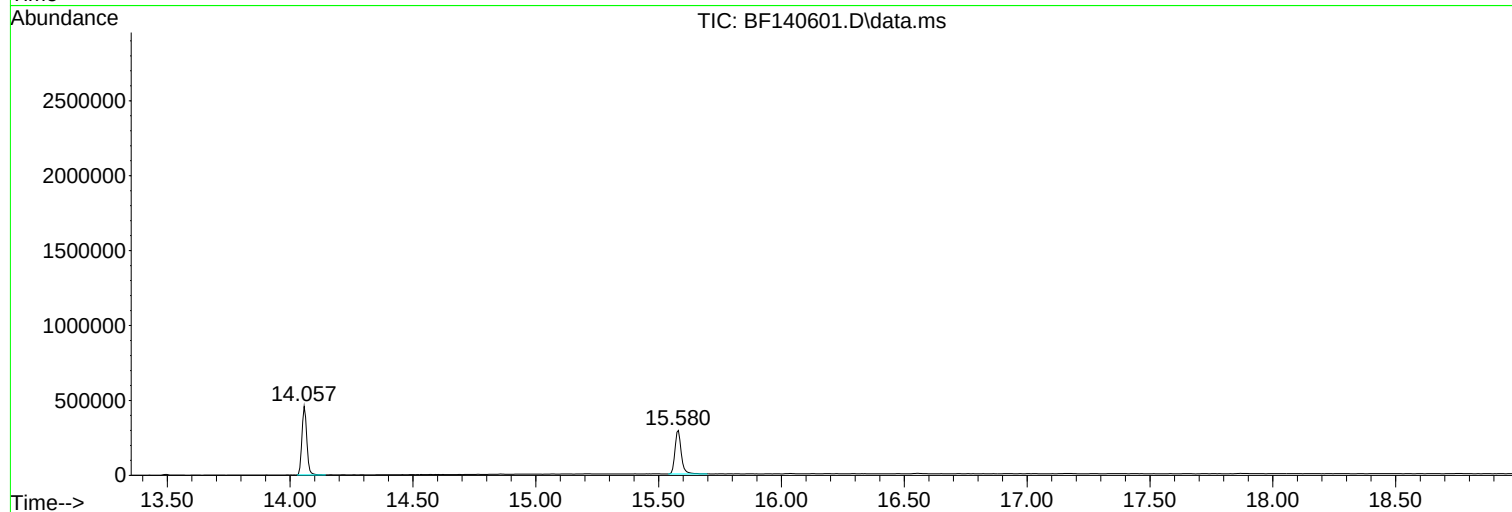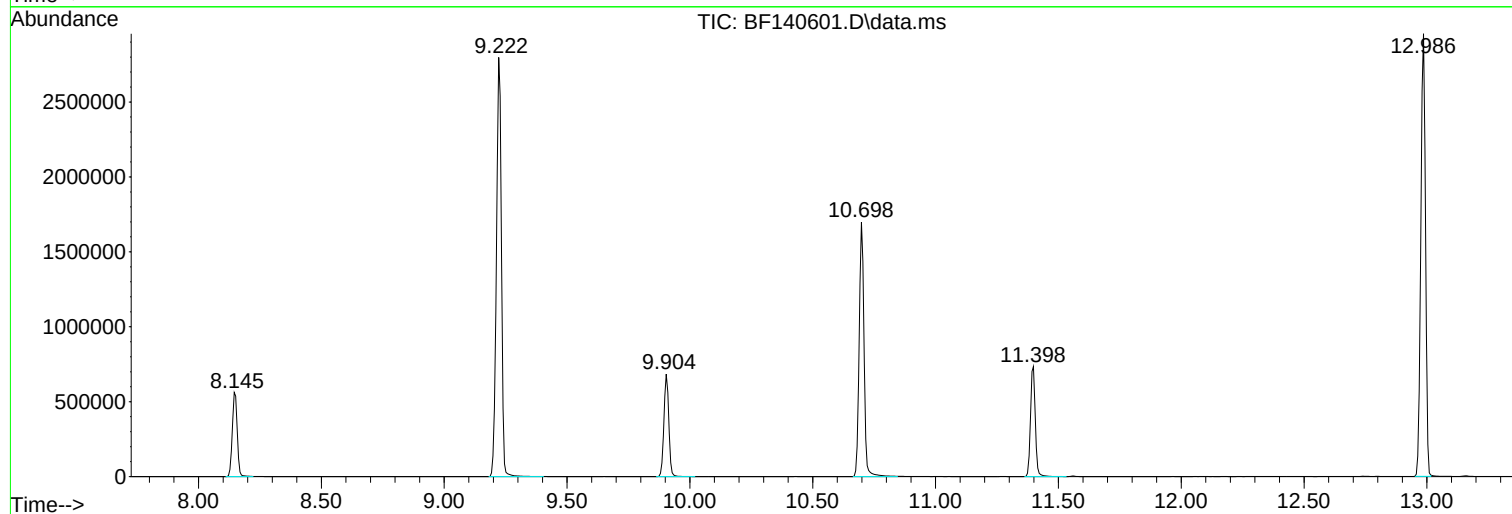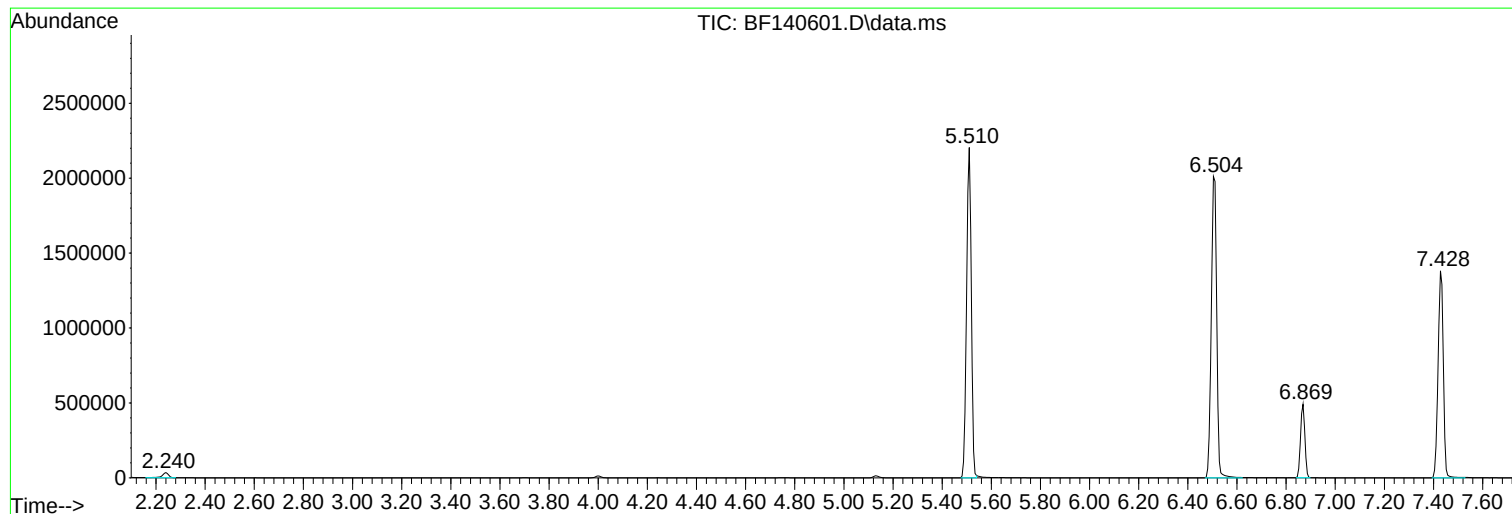

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140601.D
Acq On : 25 Nov 2024 14:28
Operator : RC/JU
Sample : PB165152BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165152BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.240	2.11 ng	63804	1,4-Dichlorobenzene-d4	6.869

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	10

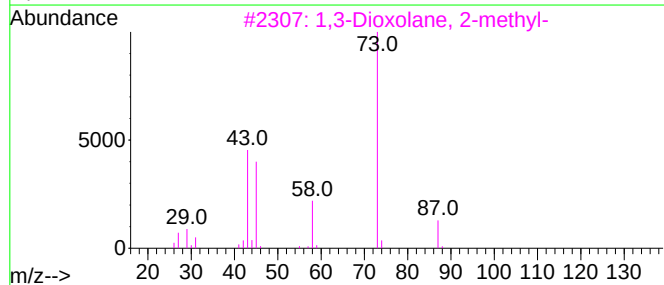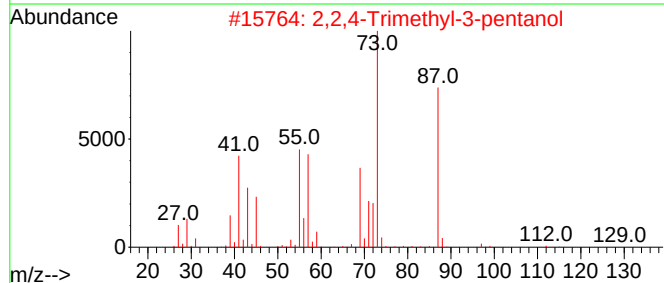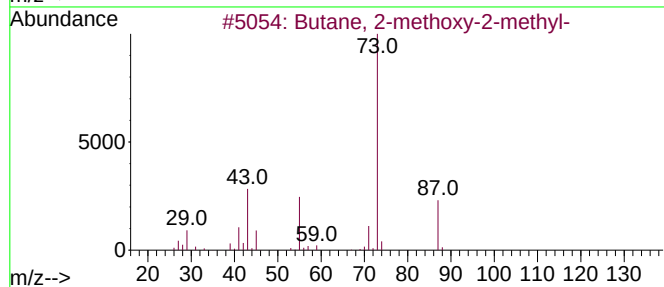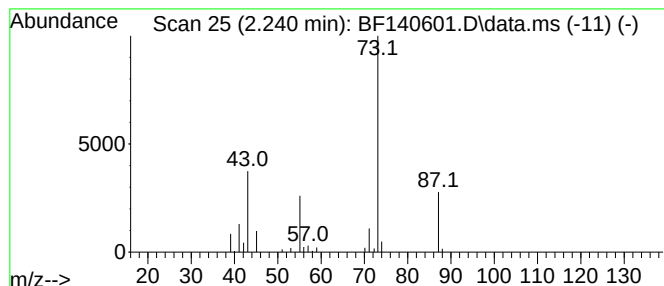

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112524\
Data File : BF140601.D
Acq On : 25 Nov 2024 14:28
Operator : RC/JU
Sample : PB165152BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165152BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.240	2.1	ng	63804	1	6.869	604561	20.0