
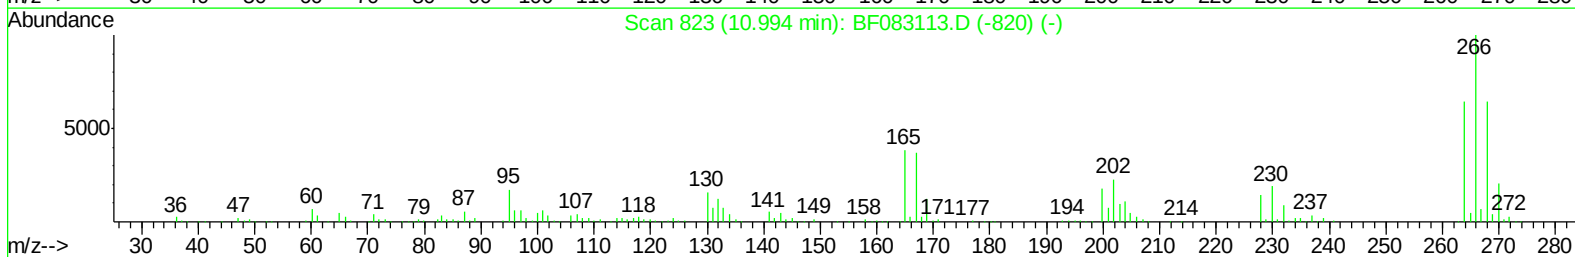
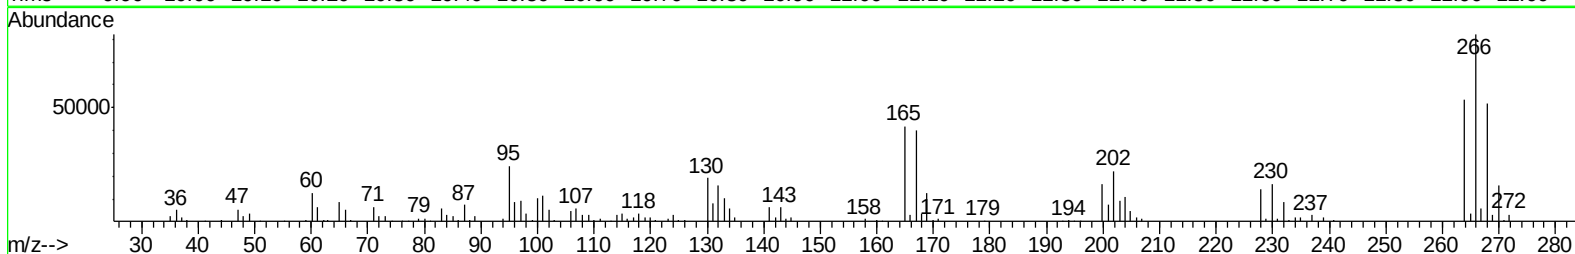


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112615\
Data File : BF083322.D
Acq On : 26 Nov 2015 16:28
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 00:29:35 2015
Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

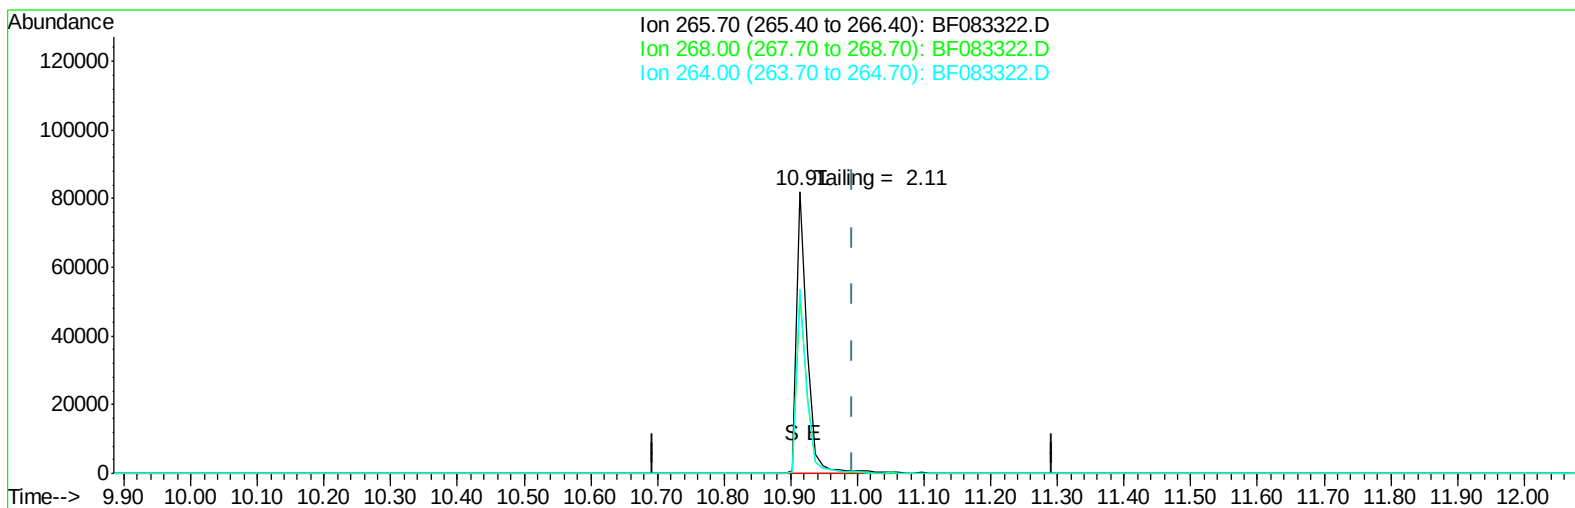

TIC: BF083322.D

(69) Pentachlorophenol (C)




10.913min (-0.080) 31022.76ng

response 91117

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	62.95
264.00	64.60	65.43
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112615\
Data File : BF083322.D
Acq On : 26 Nov 2015 16:28
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 00:29:35 2015
Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

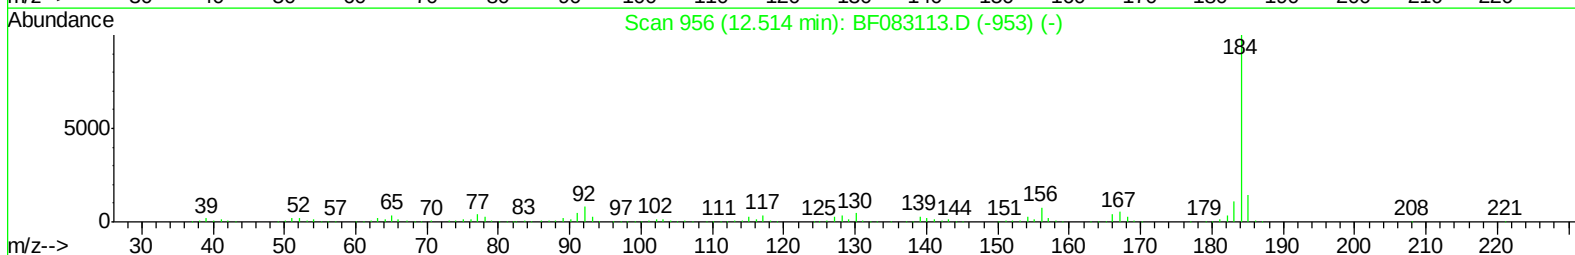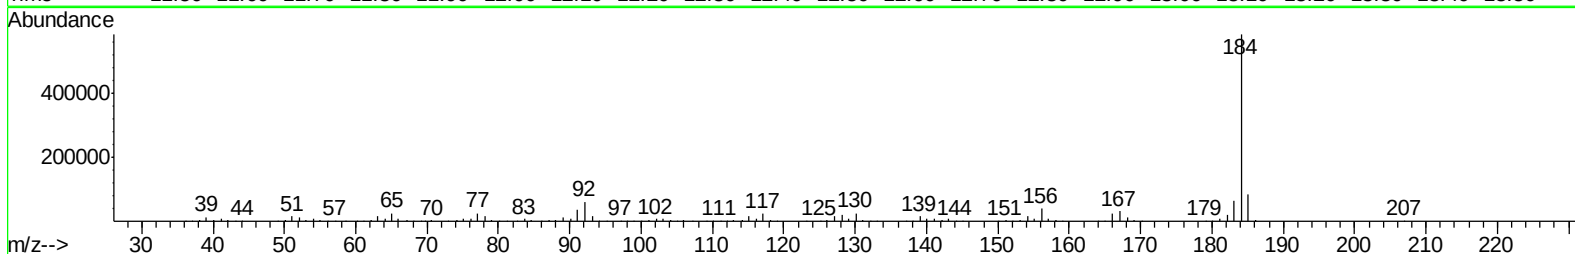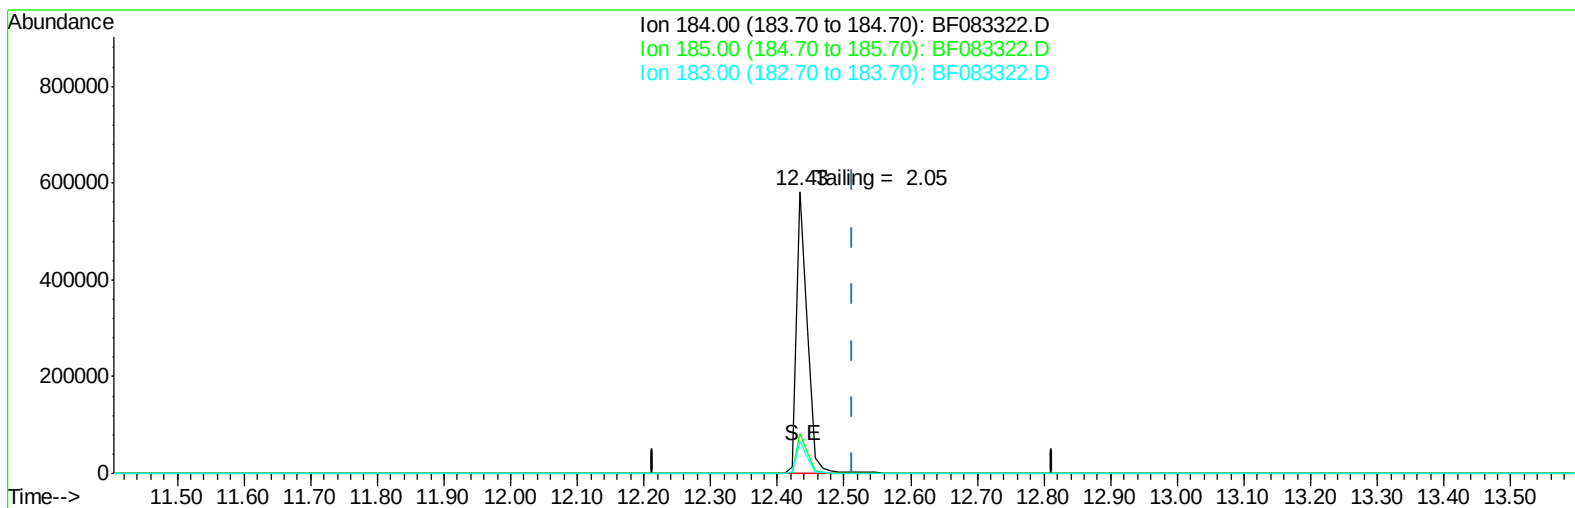

TIC: BF083322.D

(76) Benzidine

12.433min (-0.080) 16555.86ng

response 657391

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	14.24
183.00	11.00	11.16
0.00	0.00	0.00