
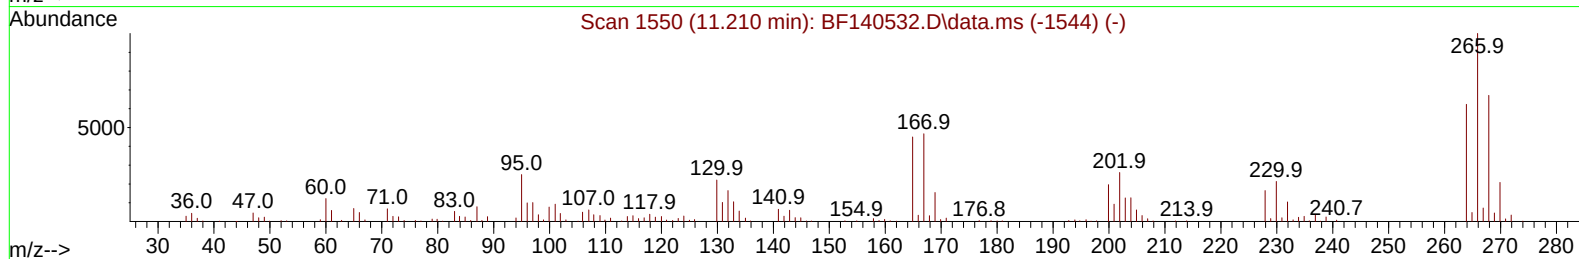
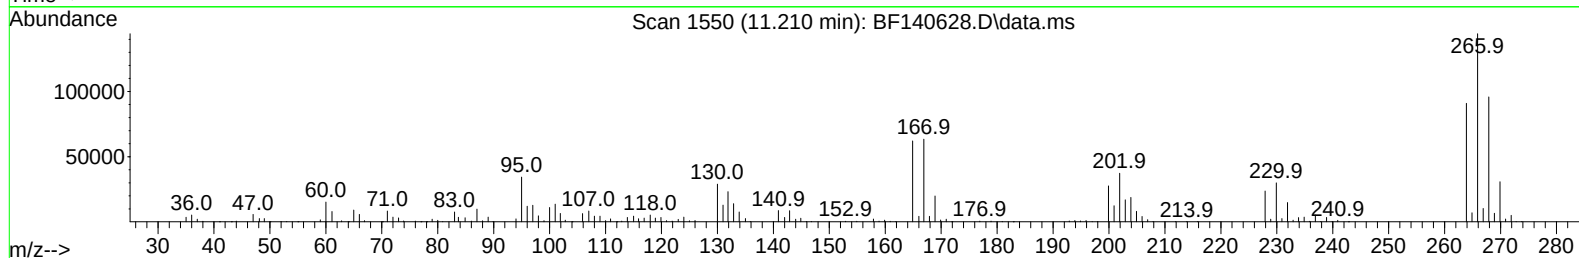


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112624\
Data File : BF140628.D
Acq On : 26 Nov 2024 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 10:51:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

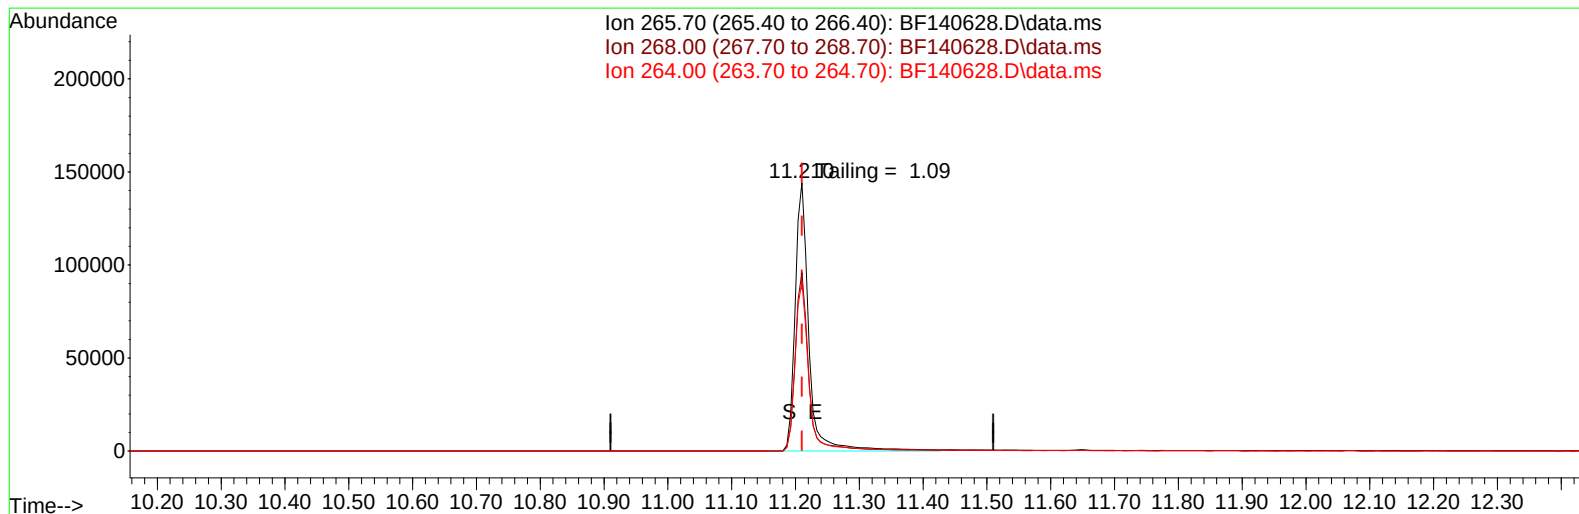

TIC: BF140628.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 21857.61 ng

response 216927

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	66.44
264.00	62.30	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112624\
 Data File : BF140628.D
 Acq On : 26 Nov 2024 09:09
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 10:51:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 15:23:48 2024
 Response via : Initial Calibration

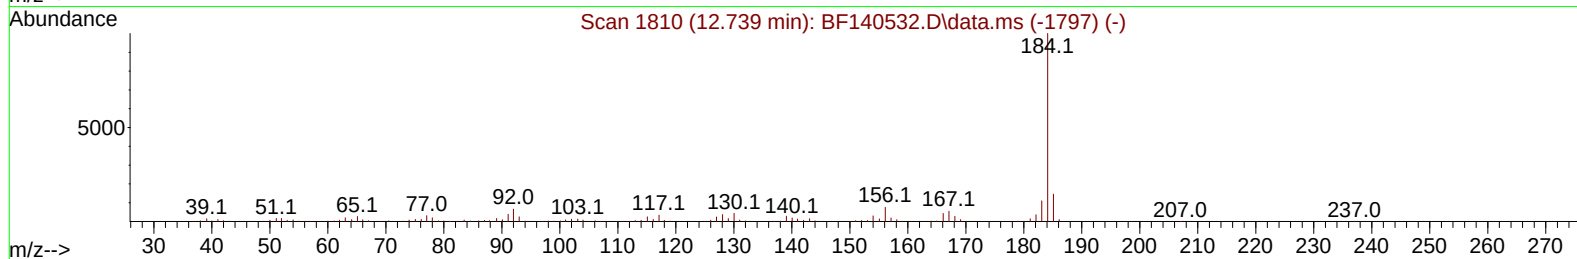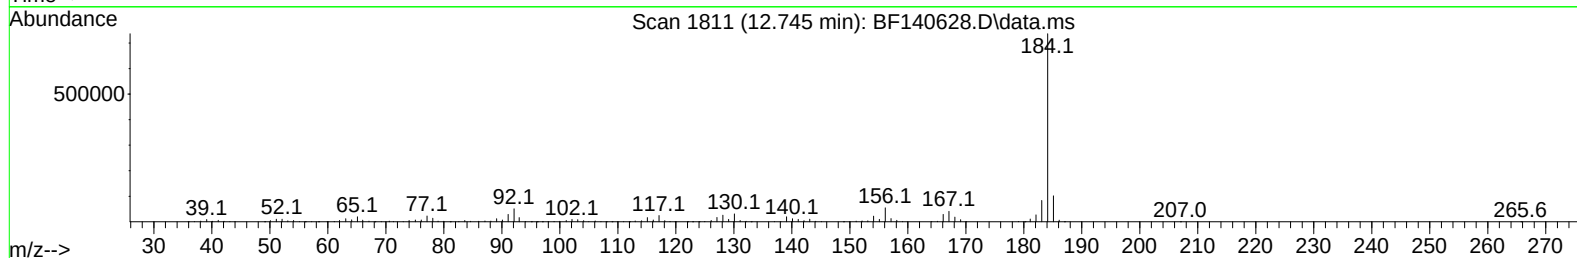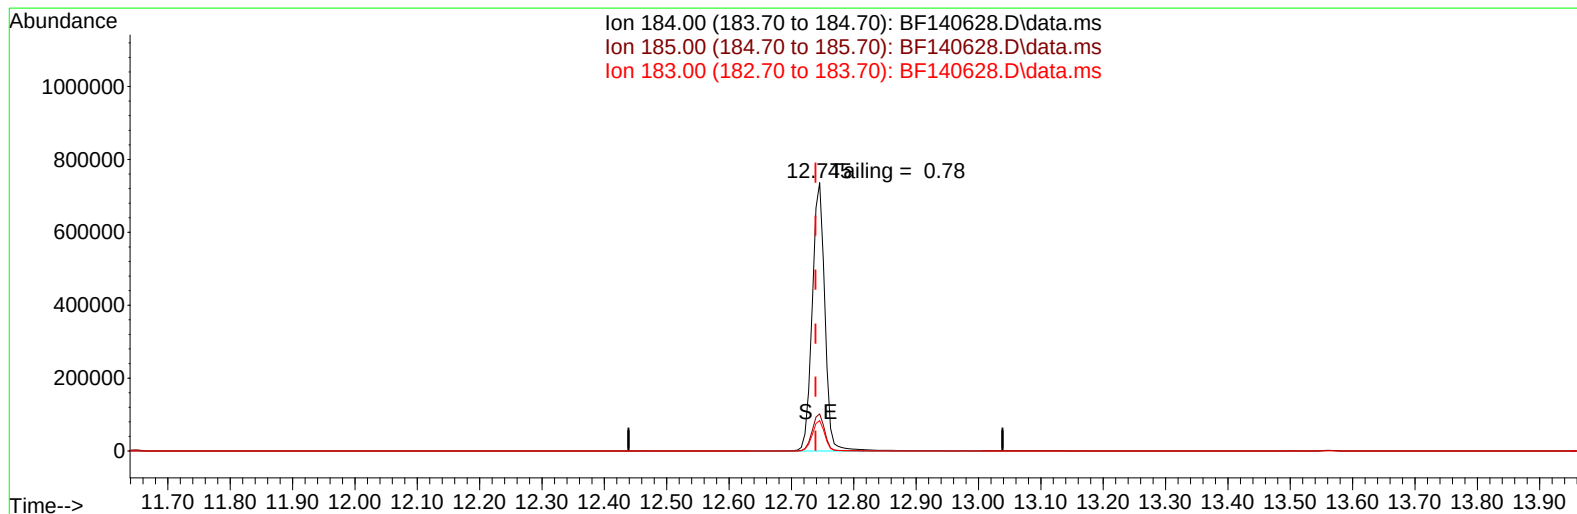

TIC: BF140628.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 20800.75 ng

response 1043833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.84
183.00	11.00	11.34
0.00	0.00	0.00