

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112624\  
 Data File : BF140630.D  
 Acq On : 26 Nov 2024 10:01  
 Operator : RC/JU  
 Sample : PB165203BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB165203BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140630.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.251       | 15            | 27          | 33           | rVB      | 28730          | 52560         | 1.21%           | 0.216%        |
| 2         | 4.010       | 318           | 326         | 338          | rBV      | 93096          | 148760        | 3.42%           | 0.611%        |
| 3         | 5.510       | 575           | 581         | 601          | rBV      | 2189870        | 3031832       | 69.71%          | 12.458%       |
| 4         | 6.510       | 744           | 751         | 756          | rBV      | 2201692        | 3128608       | 71.93%          | 12.856%       |
| 5         | 6.869       | 807           | 812         | 823          | rVB      | 522784         | 639443        | 14.70%          | 2.628%        |
| 6         | 7.433       | 901           | 908         | 922          | rBV      | 1448547        | 2089454       | 48.04%          | 8.586%        |
| 7         | 8.151       | 1024          | 1030        | 1050         | rBV      | 608557         | 837571        | 19.26%          | 3.442%        |
| 8         | 9.227       | 1205          | 1213        | 1242         | rBV      | 2883957        | 4101199       | 94.29%          | 16.852%       |
| 9         | 9.904       | 1322          | 1328        | 1349         | rVB      | 707715         | 990834        | 22.78%          | 4.071%        |
| 10        | 10.704      | 1457          | 1464        | 1485         | rBV      | 1756474        | 2495547       | 57.38%          | 10.255%       |
| 11        | 11.398      | 1576          | 1582        | 1601         | rBV      | 827341         | 1083869       | 24.92%          | 4.454%        |
| 12        | 12.986      | 1846          | 1852        | 1857         | rBV      | 3282977        | 4349402       | 100.00%         | 17.872%       |
| 13        | 14.045      | 2027          | 2032        | 2045         | rVB      | 560132         | 798133        | 18.35%          | 3.280%        |
| 14        | 15.545      | 2281          | 2287        | 2299         | rBV      | 330089         | 588789        | 13.54%          | 2.419%        |




Sum of corrected areas: 24336001

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112624\  
Data File : BF140630.D  
Acq On : 26 Nov 2024 10:01  
Operator : RC/JU  
Sample : PB165203BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB165203BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

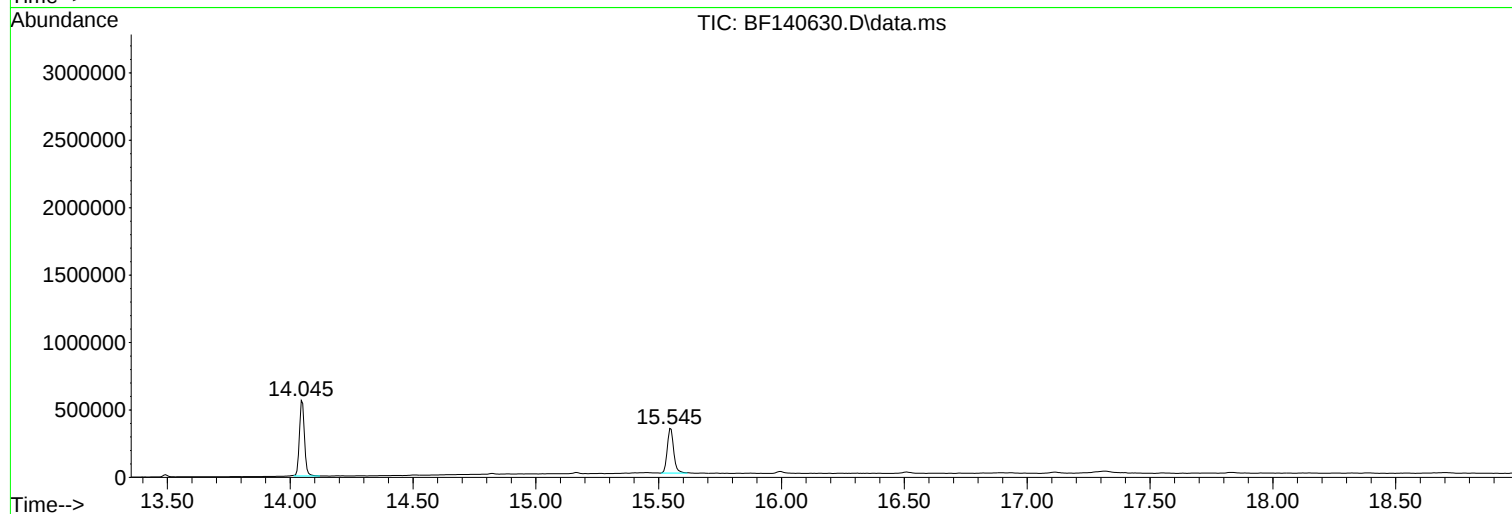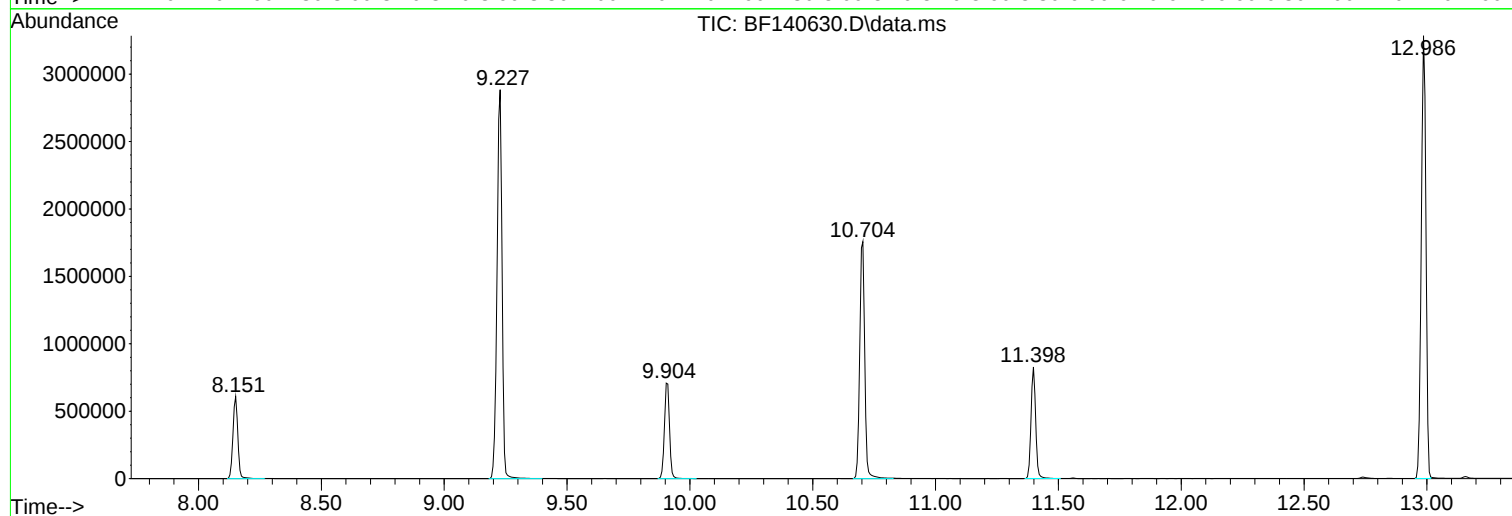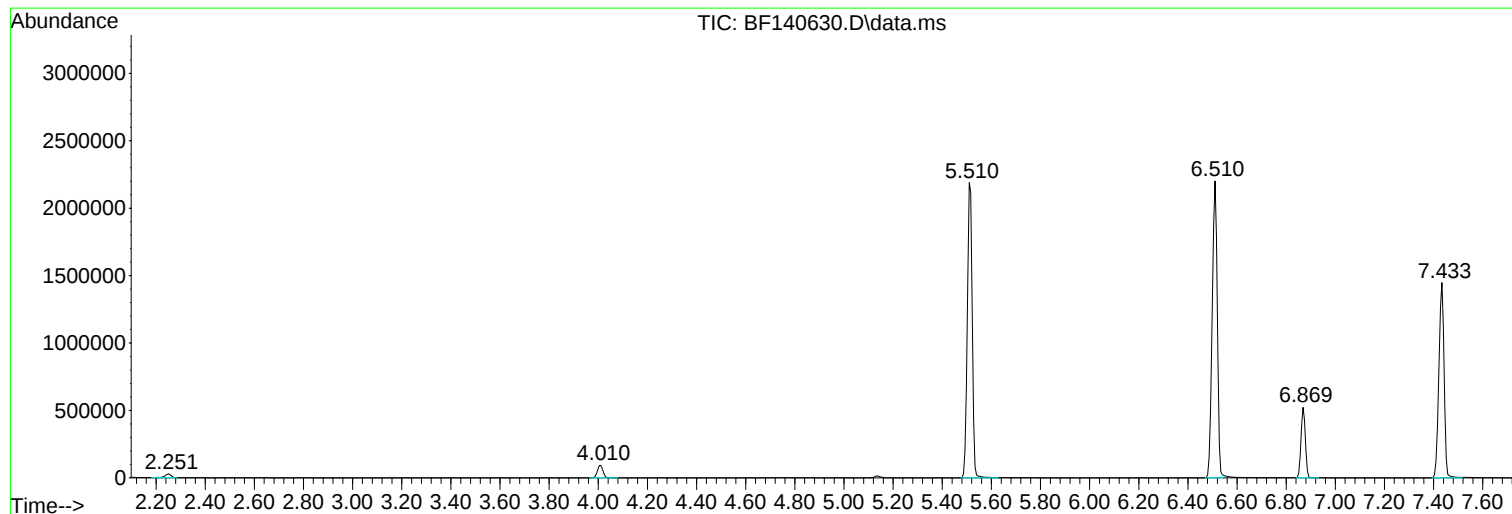

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112624\  
Data File : BF140630.D  
Acq On : 26 Nov 2024 10:01  
Operator : RC/JU  
Sample : PB165203BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB165203BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112624\  
Data File : BF140630.D  
Acq On : 26 Nov 2024 10:01  
Operator : RC/JU  
Sample : PB165203BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB165203BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|