


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112624\
Data File : BF140628.D
Acq On : 26 Nov 2024 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

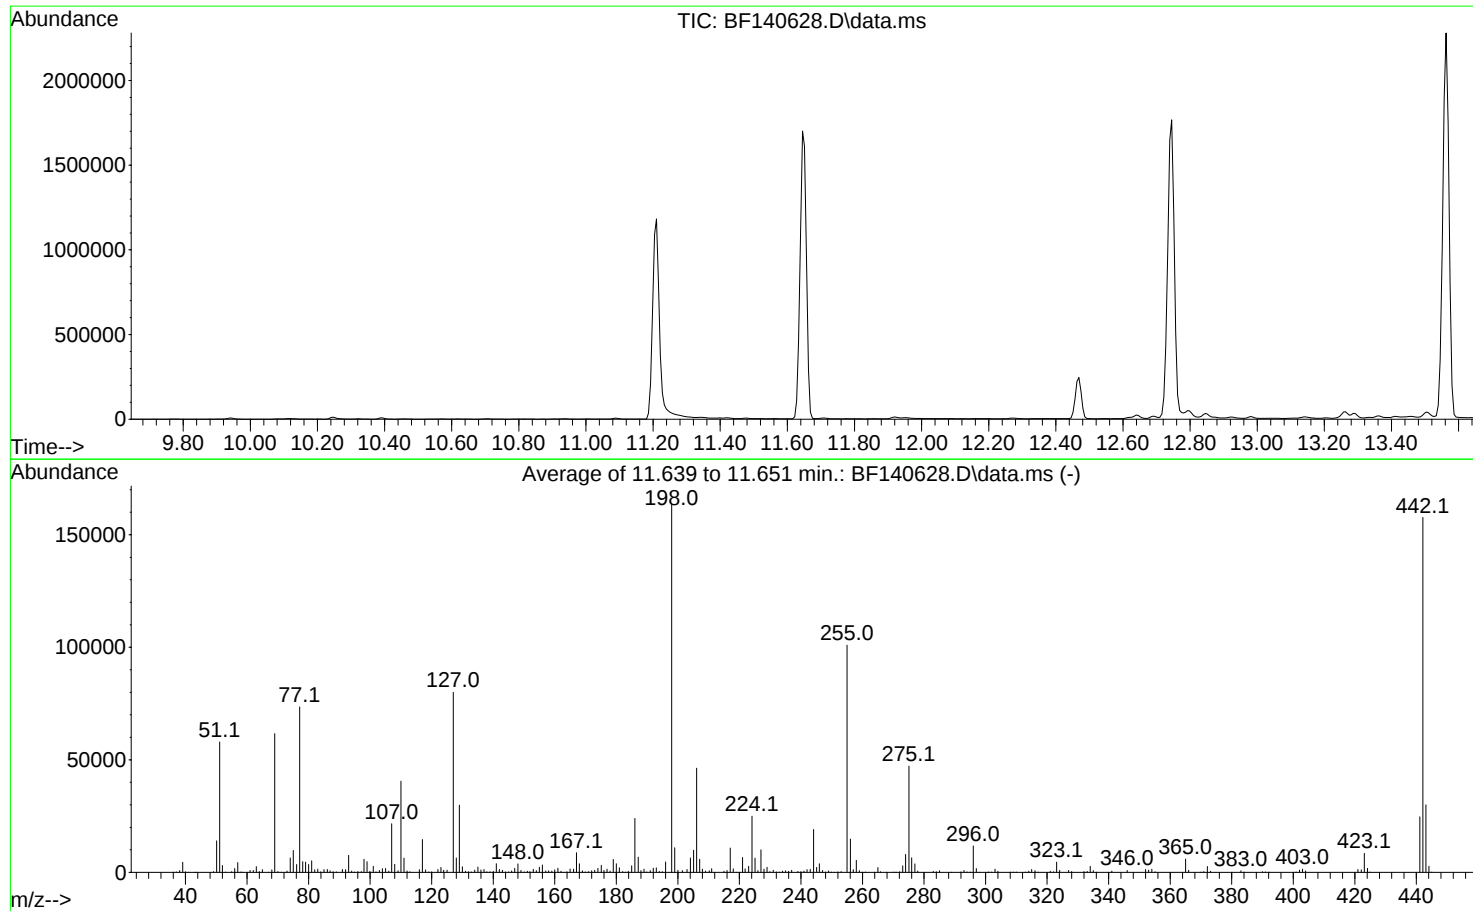

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	57963	PASS
68	69	0.00	2	1.9	1165	PASS
69	198	0.00	100	37.7	61659	PASS
70	69	0.00	2	0.6	363	PASS
127	198	10	80	48.9	79981	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	163443	PASS
199	198	5	9	6.7	10921	PASS
275	198	10	60	28.9	47219	PASS
365	198	1	100	3.6	5879	PASS
441	198	0.01	100	15.1	24700	PASS
442	442	50	100	100.0	157699	PASS
443	442	15	24	19.0	29968	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/26/2024	BNA_F	<u>BF140628.D</u>
Compound Name	Response	Retention Time
DDT	583893	13.563
DDD	16620	13.263
DDE	2795	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19415	603308	3.22

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112624\
Data File : BF140628.D
Acq On : 26 Nov 2024 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 26 10:51:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

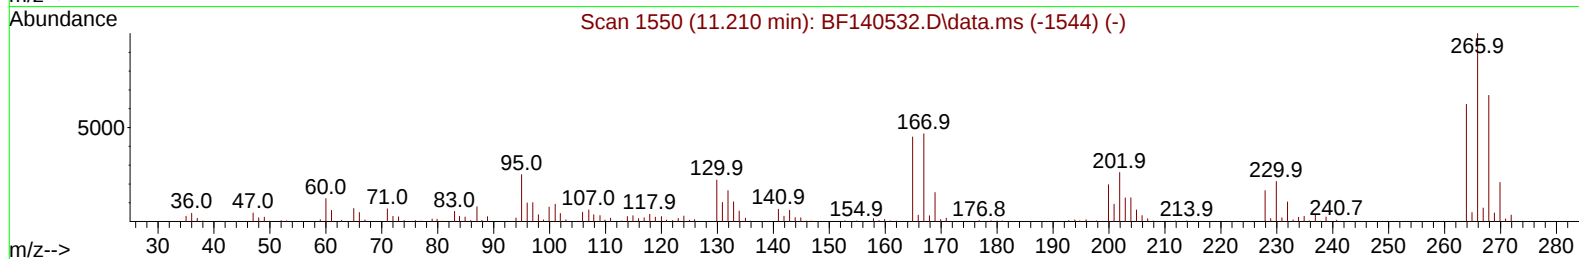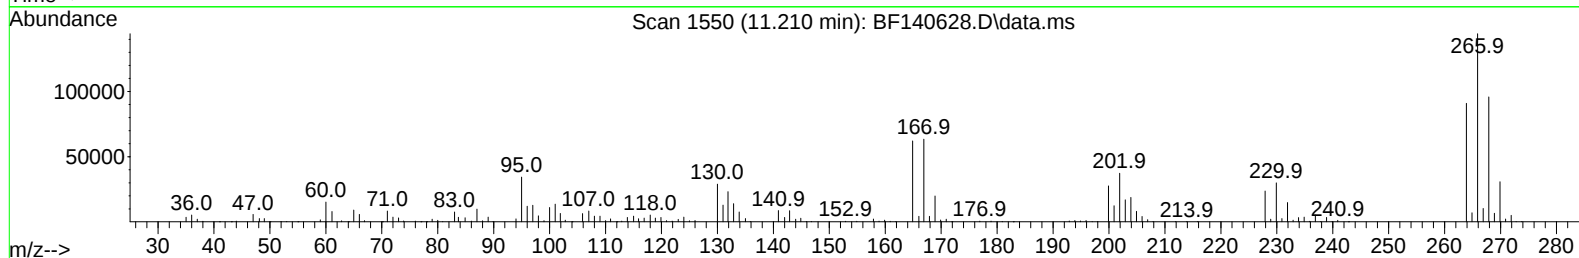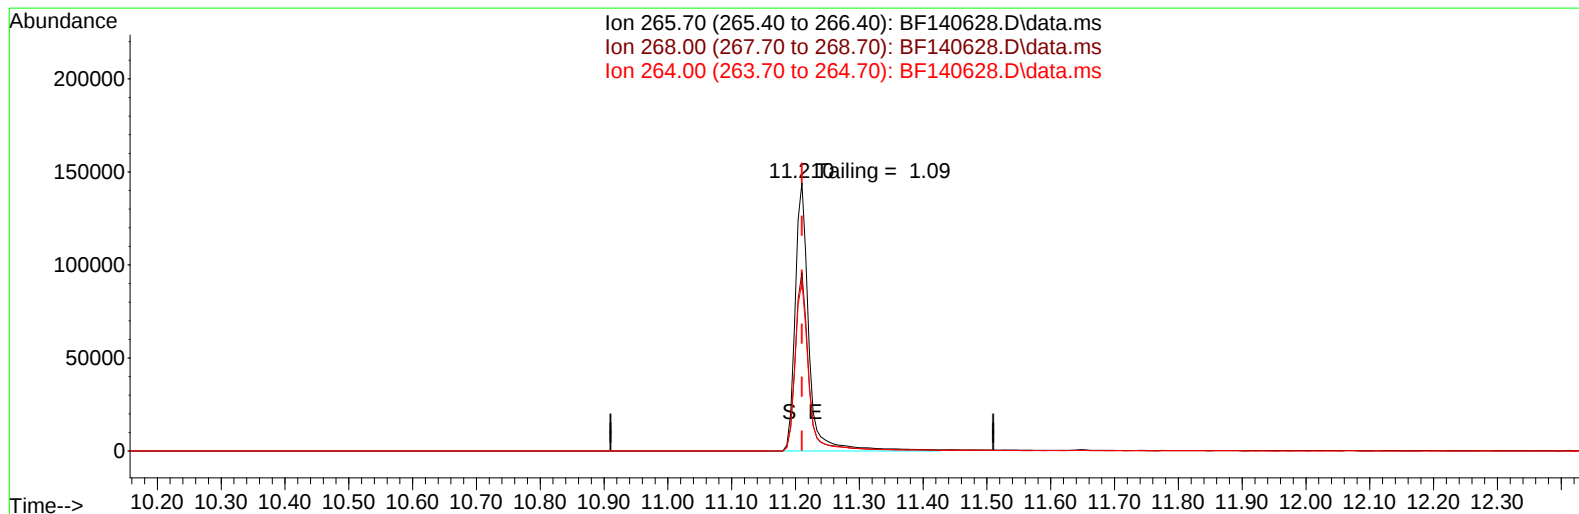

TIC: BF140628.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 21857.61 ng




response 216927

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	66.44
264.00	62.30	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112624\
Data File : BF140628.D
Acq On : 26 Nov 2024 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 26 10:51:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

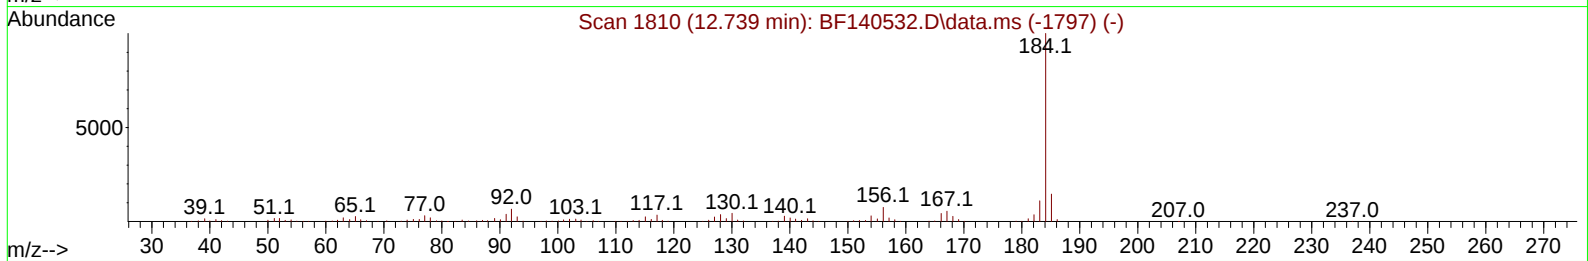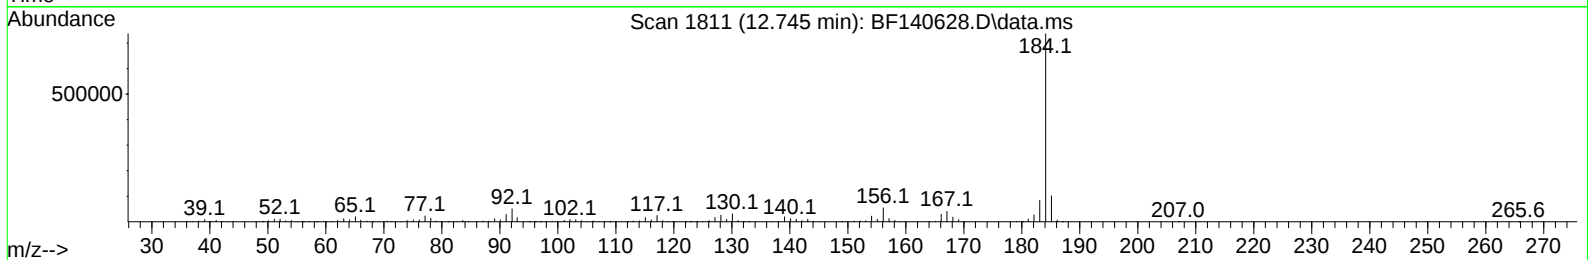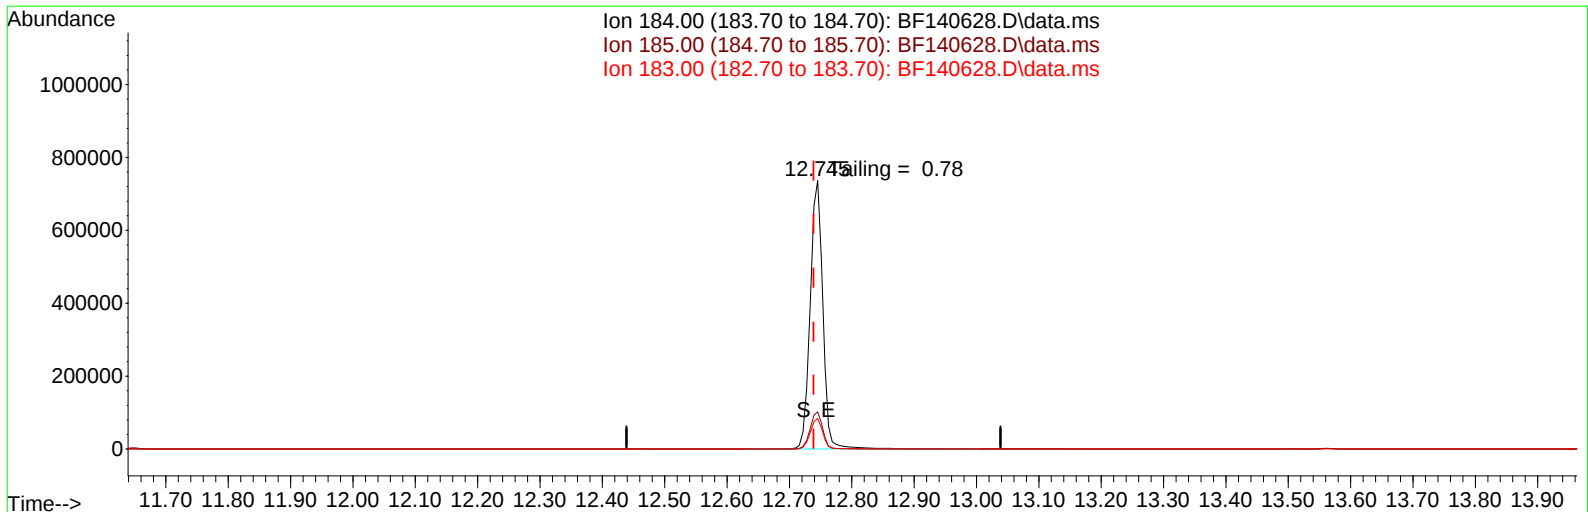

TIC: BF140628.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 20800.75 ng

response 1043833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.84
183.00	11.00	11.34
0.00	0.00	0.00