


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF112715\  
Data File : BF083327.D  
Acq On : 27 Nov 2015 11:11  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF112715.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Nov 27 19:11:49 2015

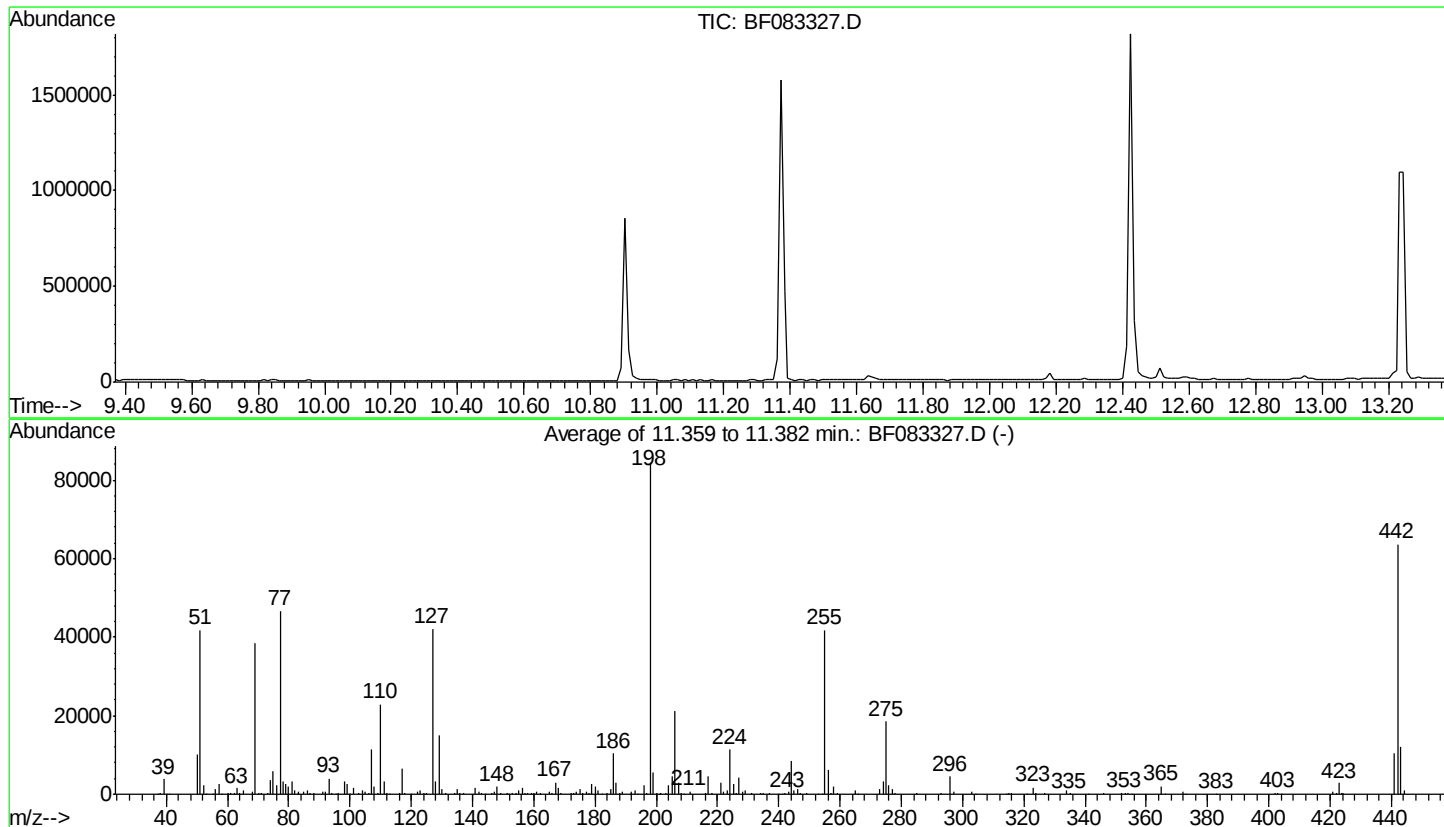

AutoFind: Scans 820, 821, 822; Background Corrected with Scan 817

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 49.5      | 41855   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 684     | PASS             |
| 69          | 198          | 0.00         | 100          | 45.6      | 38483   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 188     | PASS             |
| 127         | 198          | 10           | 80           | 50.0      | 42218   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 409     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 84474   | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 5497    | PASS             |
| 275         | 198          | 10           | 60           | 22.0      | 18579   | PASS             |
| 365         | 198          | 1            | 100          | 2.5       | 2098    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.6      | 10565   | PASS             |
| 442         | 198          | 50           | 100          | 75.4      | 63653   | PASS             |
| 443         | 442          | 15           | 24           | 18.9      | 12026   | PASS             |