

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112717\
 Data File : BF100891.D
 Acq On : 27 Nov 2017 14:52
 Operator : SJ/JU
 Sample : I6570-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Nov 27 21:57:22 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 14:11:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	72443	20.00	ng	0.00
21) Naphthalene-d8	8.14	136	289914	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	134396	20.00	ng	0.00
63) Phenanthrene-d10	11.38	188	252859	20.00	ng	0.00
75) Chrysene-d12	14.02	240	152337	20.00	ng	-0.01
86) Perylene-d12	15.49	264	164148	20.00	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.47	112	368928	81.63	ng	0.00
7) Phenol-d6	6.49	99	448113	80.41	ng	0.00
23) Nitrobenzene-d5	7.42	82	277178	63.21	ng	0.00
41) 2,4,6-Tribromophenol	10.69	330	125560	91.68	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	510698	57.86	ng	0.00
78) Terphenyl-d14	12.96	244	445909	67.26	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Phenol	6.50	94	17577	3.004	ng	96
19) n-Nitroso-di-n-propylamine	7.42	70	35310	9.136	ng	# 78
25) Isophorone	7.42	82	277175	30.079	ng	# 64
47) 2-Nitroaniline	9.60	65	590	3.007	ng	# 1
49) Dimethylphthalate	9.60	163	69888	6.811	ng	100
56) 2,4-Dinitrotoluene	9.89	165	16646	6.496	ng	# 21
64) 4,6-Dinitro-2-methylphenol	10.69	198	131	8.654	ng	# 41
66) 4-Bromophenyl-phenylether	10.68	248	8168	3.013	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112717\
Data File : BF100891.D
Acq On : 27 Nov 2017 14:52
Operator : SJ/JU
Sample : I6570-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Nov 27 21:57:22 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 14:11:25 2017
Response via : Initial Calibration

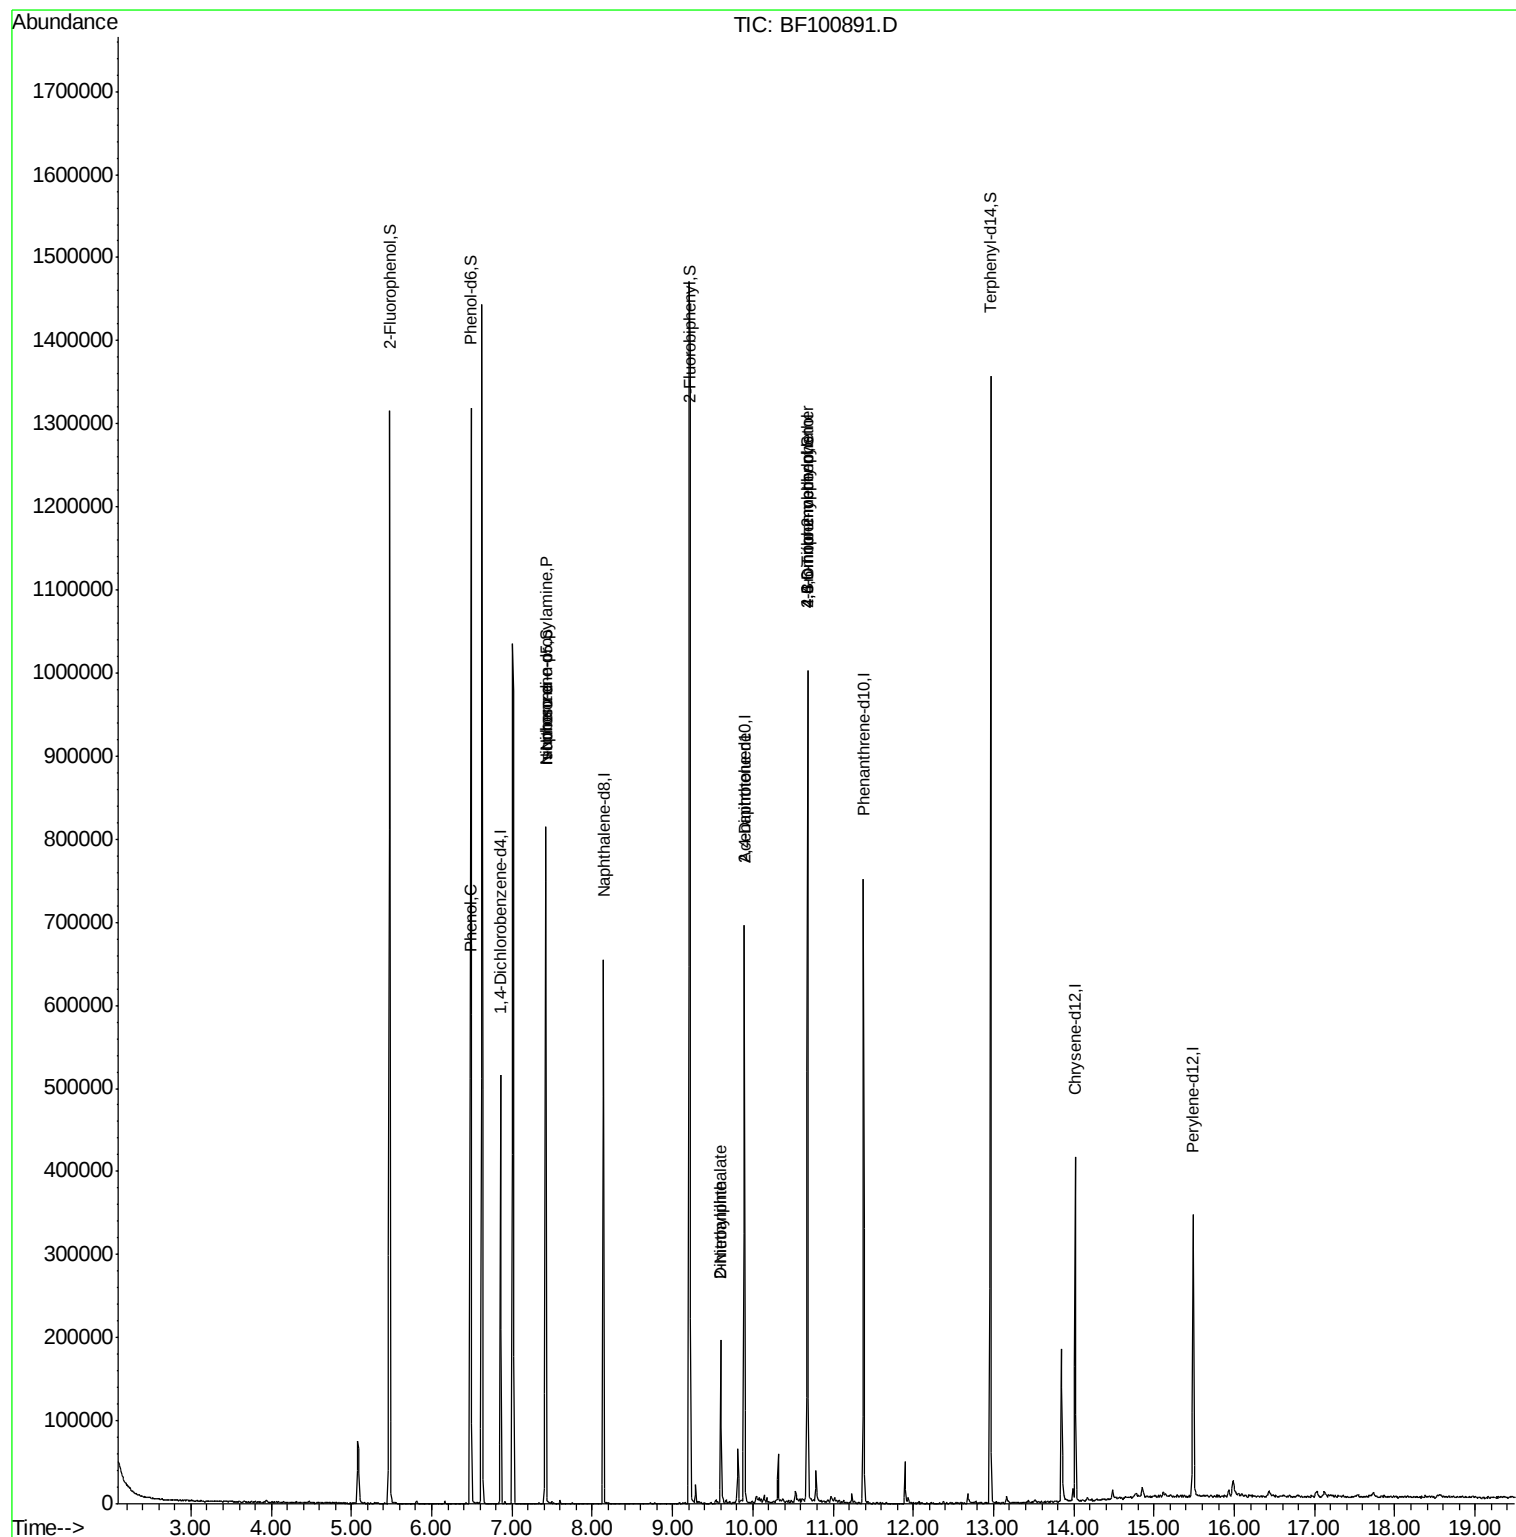

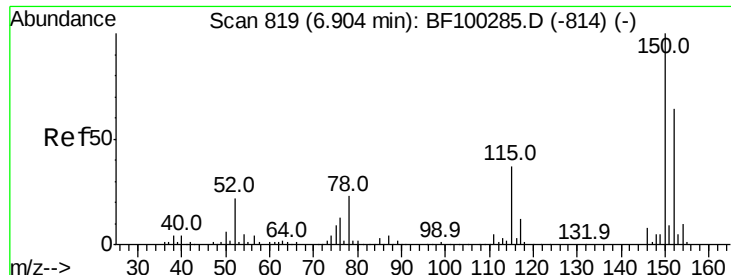


#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.86 min Scan# 811
 Delta R.T. 0.00 min
 Lab File: BF100891.D
 Acq: 27 Nov 2017 14:52

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:152 Resp: 72443
 Ion Ratio Lower Upper
 152 100
 150 156.2 124.6 186.8
 115 56.6 50.1 75.1

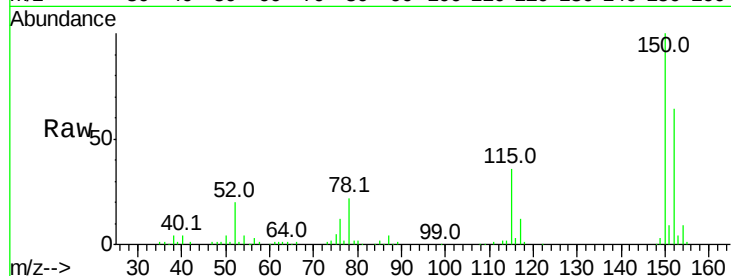


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

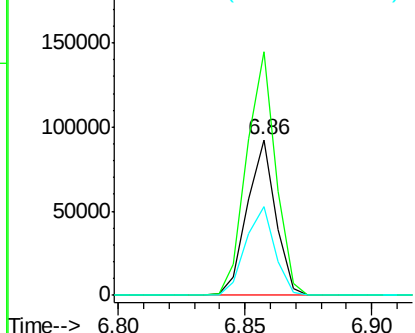



#5



2-Fluorophenol
 Concen: 81.635 ng
 RT: 5.47 min Scan# 576
 Delta R.T. 0.00 min
 Lab File: BF100891.D
 Acq: 27 Nov 2017 14:52

Tgt Ion:112 Resp: 368928
 Ion Ratio Lower Upper
 112 100
 64 60.7 47.9 71.9
 63 31.6 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

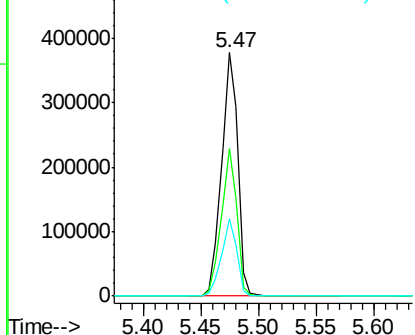

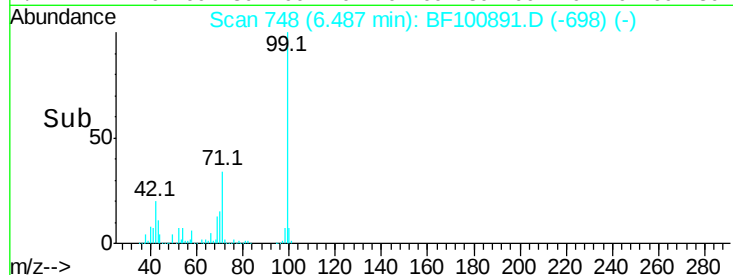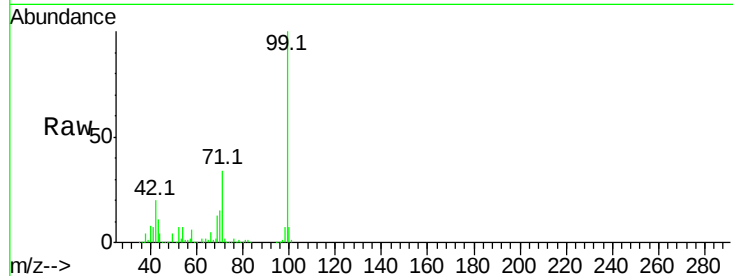

#7

Phenol-d6

Concen: 80.410 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF100891.D

Acq: 27 Nov 2017 14:52

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 448113

Ion Ratio Lower Upper

99 100

42 19.7 14.5 21.7

71 34.1 25.4 38.0

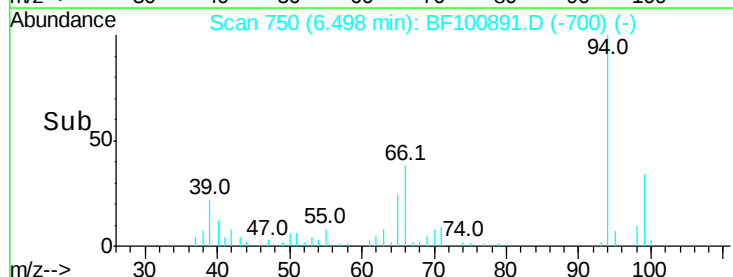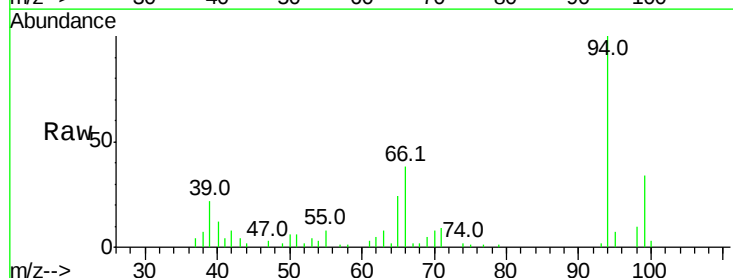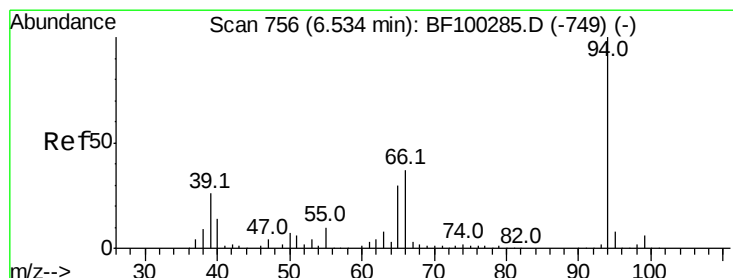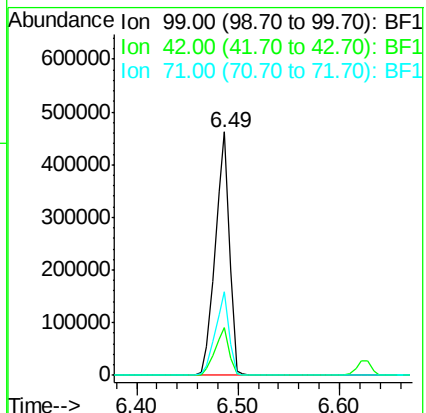

#10

Phenol

Concen: 3.004 ng

RT: 6.50 min Scan# 750

Delta R.T. -0.01 min

Lab File: BF100891.D

Acq: 27 Nov 2017 14:52


Tgt Ion: 94 Resp: 17577


Ion Ratio Lower Upper

94 100

65 24.2 7.9 47.9

66 37.5 16.2 56.2




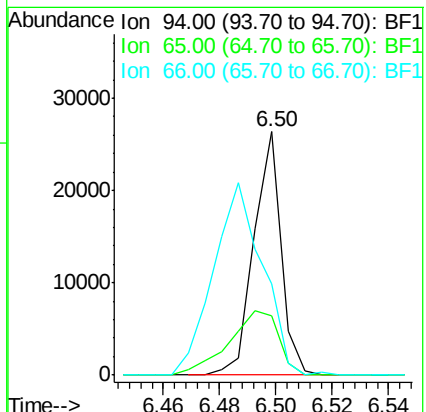




#19
n-Nitroso-di-n-propylamine
Concen: 9.136 ng
RT: 7.42 min Scan# 907
Delta R.T. 0.15 min
Lab File: BF100891.D
Acq: 27 Nov 2017 14:52




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 70 Resp: 35310
Ion Ratio Lower Upper
70 100
42 48.0 47.5 71.3
101 0.0 7.4 11.2#
130 2.1 16.6 25.0#

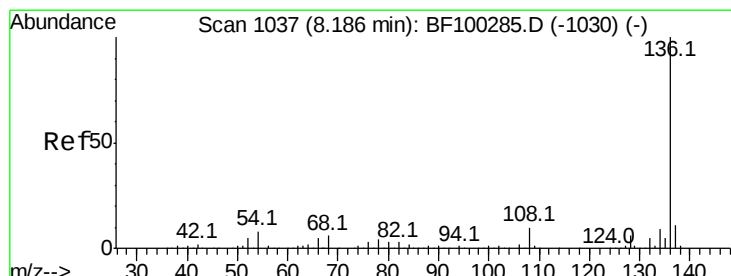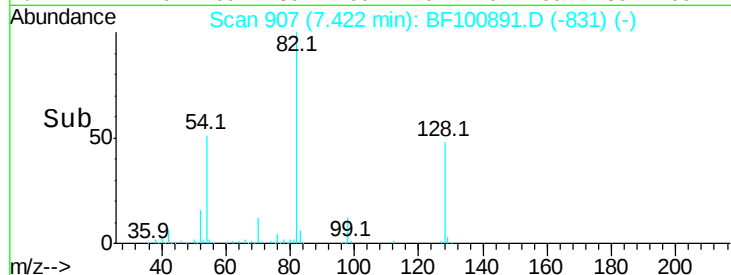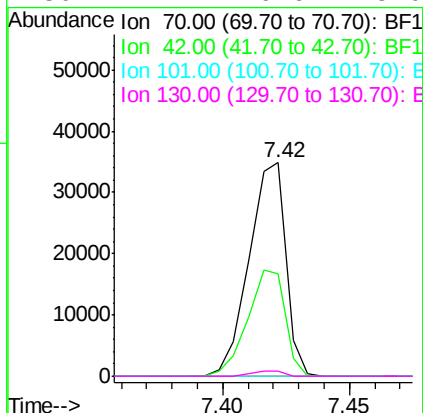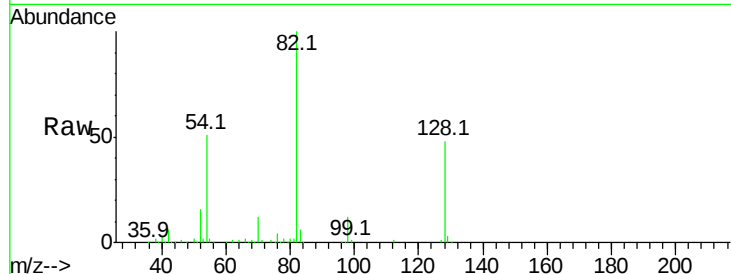

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.14 min Scan# 1029
Delta R.T. -0.01 min
Lab File: BF100891.D
Acq: 27 Nov 2017 14:52

Tgt Ion:136 Resp: 289914
Ion Ratio Lower Upper
136 100
137 10.8 8.9 13.3
54 7.3 6.6 9.8
68 4.5 5.0 7.4#

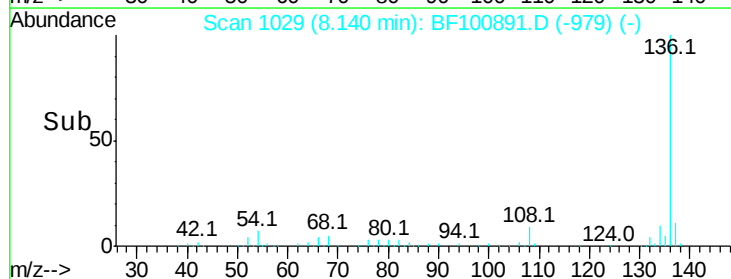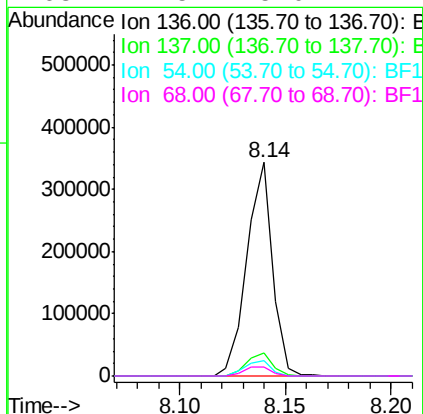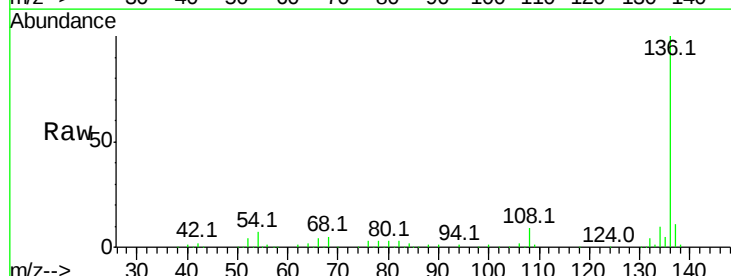


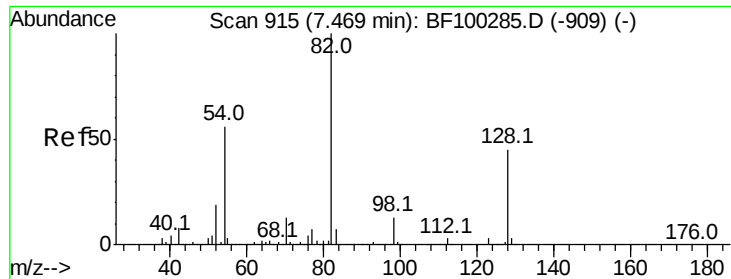




#23
Nitrobenzene-d5
Concen: 63.209 ng
RT: 7.42 min Scan# 907
Delta R.T. -0.01 min
Lab File: BF100891.D
Acq: 27 Nov 2017 14:52

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 82 Resp: 277178
Ion Ratio Lower Upper
82 100
128 47.7 36.1 54.1
54 50.9 41.4 62.2




Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

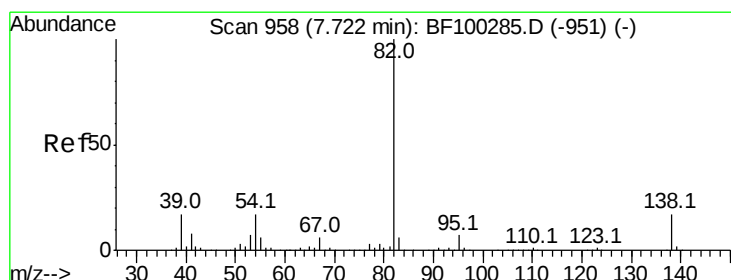
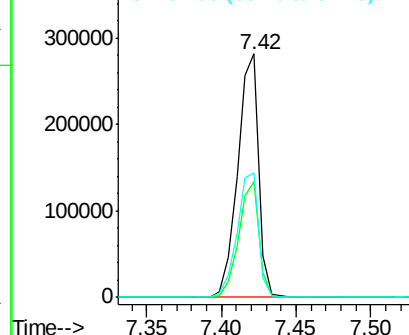



#25
Isophorone
Concen: 30.079 ng
RT: 7.42 min Scan# 907
Delta R.T. -0.26 min
Lab File: BF100891.D
Acq: 27 Nov 2017 14:52

Tgt Ion: 82 Resp: 277175
Ion Ratio Lower Upper
82 100
95 0.0 5.2 7.8#
138 0.0 14.9 22.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1



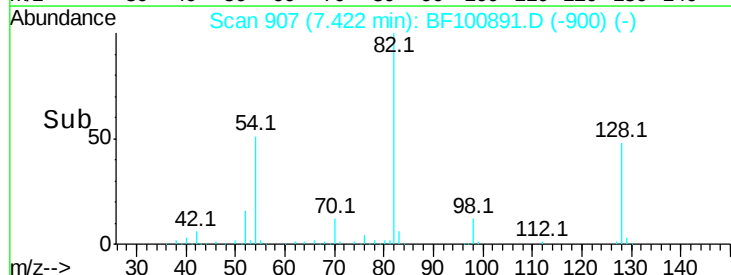
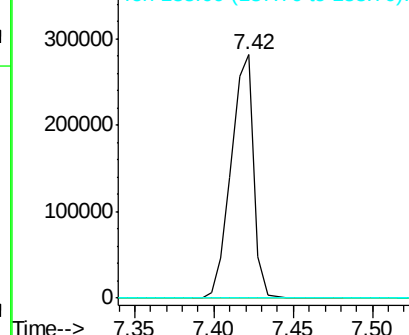


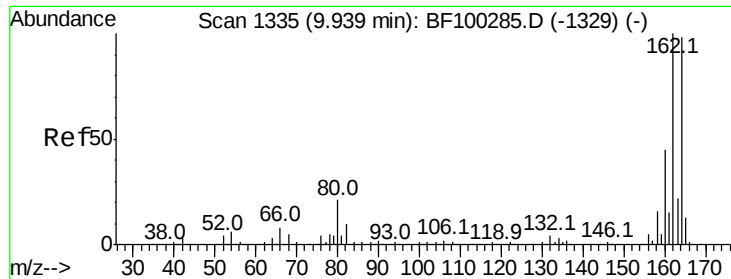

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.89 min Scan# 1327
 Delta R.T. -0.01 min
 Lab File: BF100891.D
 Acq: 27 Nov 2017 14:52




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:164 Resp: 134396
 Ion Ratio Lower Upper
 164 100
 162 104.8 86.1 129.1
 160 45.7 38.3 57.5

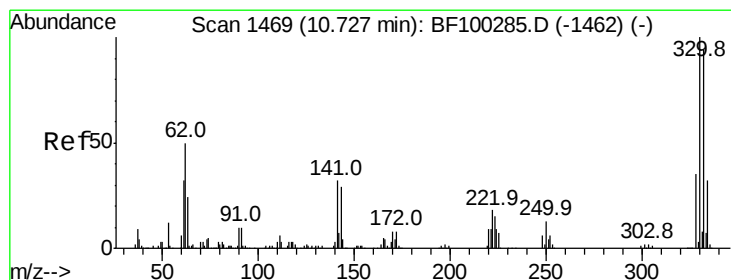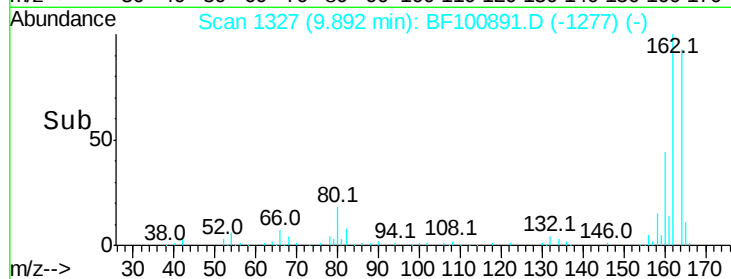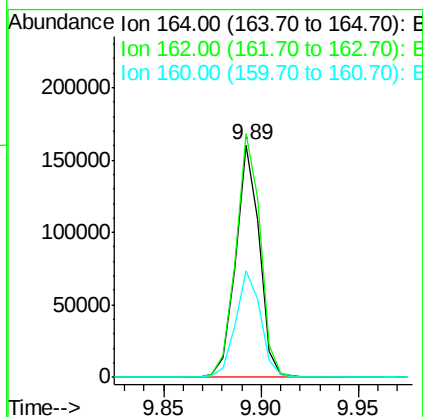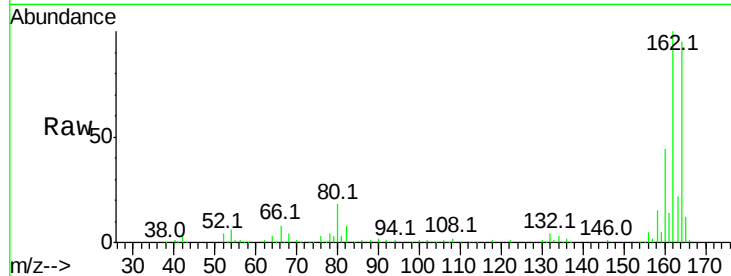

#41
 2,4,6-Tribromophenol
 Concen: 91.683 ng
 RT: 10.69 min Scan# 1462
 Delta R.T. -0.01 min
 Lab File: BF100891.D
 Acq: 27 Nov 2017 14:52

Tgt Ion:330 Resp: 125560
 Ion Ratio Lower Upper
 330 100
 332 98.8 77.0 115.6
 141 29.4 29.9 44.9#



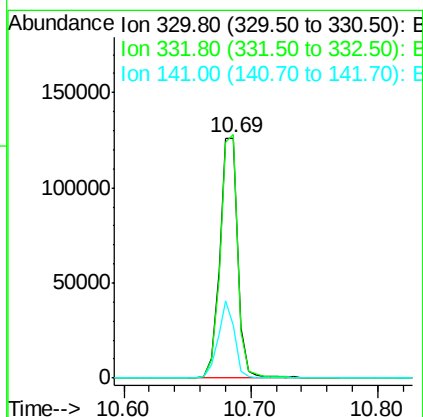





#44
 2-Fluorobiphenyl
 Concen: 57.862 ng
 RT: 9.22 min Scan# 1212
 Delta R.T. -0.01 min
 Lab File: BF100891.D
 Acq: 27 Nov 2017 14:52




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:172 Resp: 510698
 Ion Ratio Lower Upper
 172 100
 171 35.8 29.7 44.5
 170 24.3 19.6 29.4

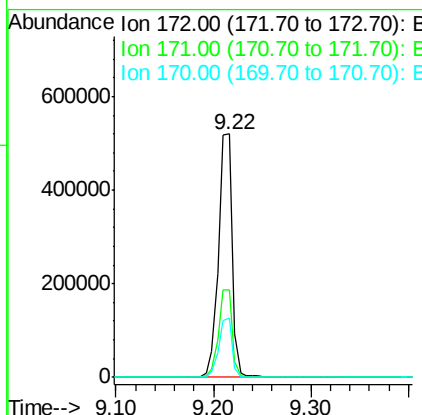

#47
 2-Nitroaniline
 Concen: 3.007 ng
 RT: 9.60 min Scan# 1278
 Delta R.T. 0.16 min
 Lab File: BF100891.D
 Acq: 27 Nov 2017 14:52

Tgt Ion: 65 Resp: 590
 Ion Ratio Lower Upper
 65 100
 92 1011.8 55.8 83.6#
 138 0.0 91.2 136.8#



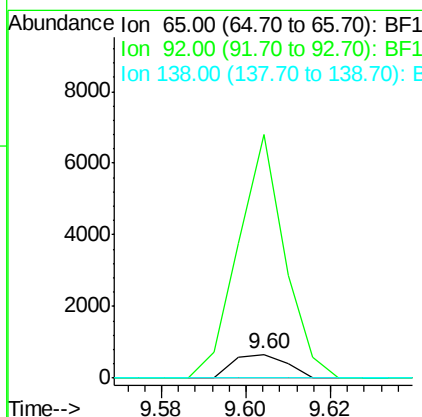



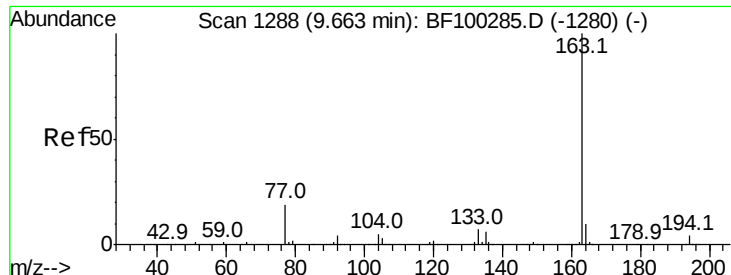

#49
Dimethylphthalate
Concen: 6.811 ng
RT: 9.60 min Scan# 1278
Delta R.T. -0.02 min
Lab File: BF100891.D
Acq: 27 Nov 2017 14:52




Instrument :
BNA_F
ClientSampleId :


Tot Ion:163 Resp: 69888
Ion Ratio Lower Upper
163 100
194 3.6 2.7 4.1
164 10.2 8.2 12.2

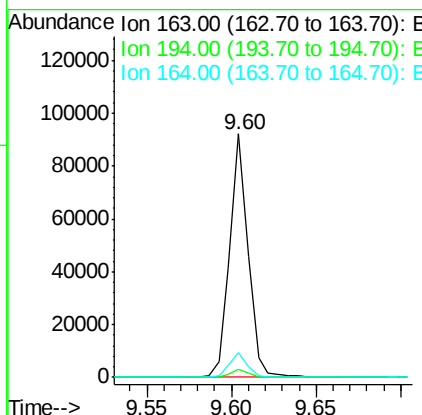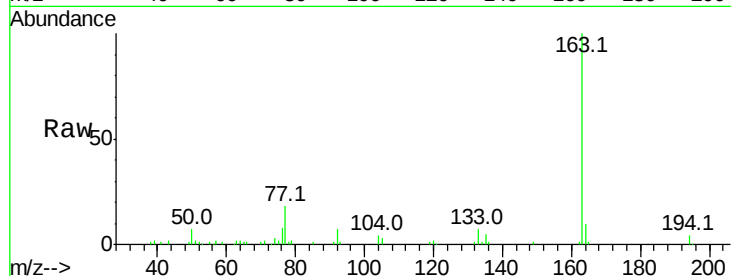

#56
2,4-Dinitrotoluene
Concen: 6.496 ng
RT: 9.89 min Scan# 1327
Delta R.T. -0.19 min
Lab File: BF100891.D
Acq: 27 Nov 2017 14:52

Tgt Ion:165 Resp: 16646
Ion Ratio Lower Upper
165 100
63 0.0 36.4 54.6#
89 0.0 57.8 86.6#
182 0.0 1.6 2.4#



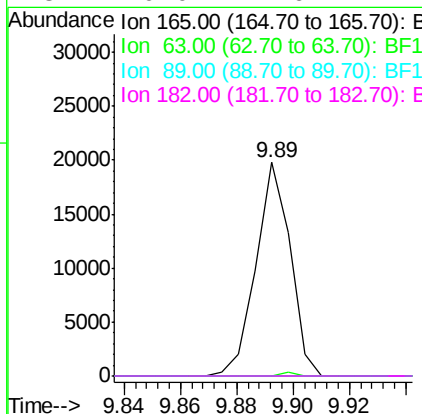





#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.38 min Scan# 1580
 Delta R.T. -0.01 min
 Lab File: BF100891.D
 Acq: 27 Nov 2017 14:52




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:188 Resp: 252859
 Ion Ratio Lower Upper
 188 100
 94 8.5 8.5 12.7#
 80 9.0 9.2 13.8#

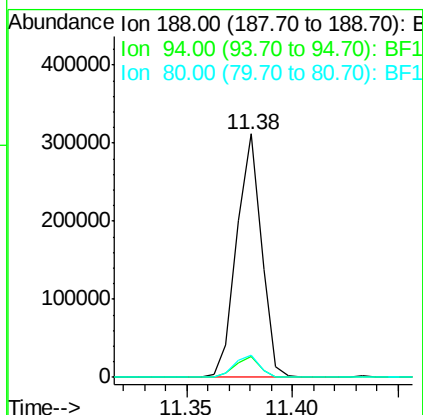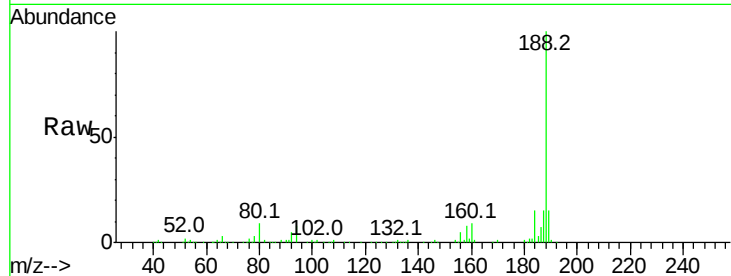

#64
 4,6-Dinitro-2-methylphenol
 Concen: 8.654 ng
 RT: 10.69 min Scan# 1462
 Delta R.T. 0.19 min
 Lab File: BF100891.D
 Acq: 27 Nov 2017 14:52

Tgt Ion:198 Resp: 131
 Ion Ratio Lower Upper
 198 100
 51 88.9 37.7 77.7#
 105 0.0 36.3 76.3#

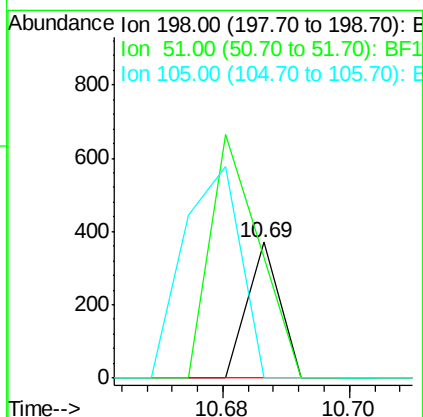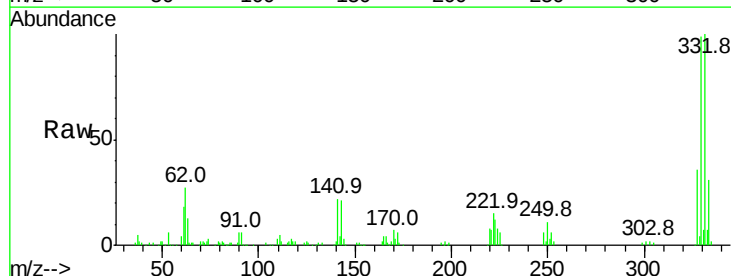


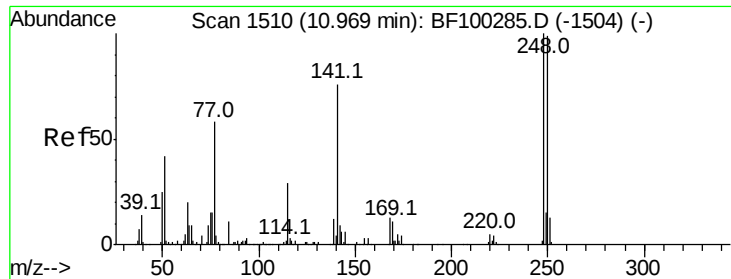




#66
4-Bromophenyl-phenylether
Concen: 3.013 ng
RT: 10.68 min Scan# 1461
Delta R.T. -0.25 min
Lab File: BF100891.D
Acq: 27 Nov 2017 14:52

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 8168
Ion Ratio Lower Upper
248 100
250 177.9 76.9 115.3#
141 439.5 74.4 111.6#




Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

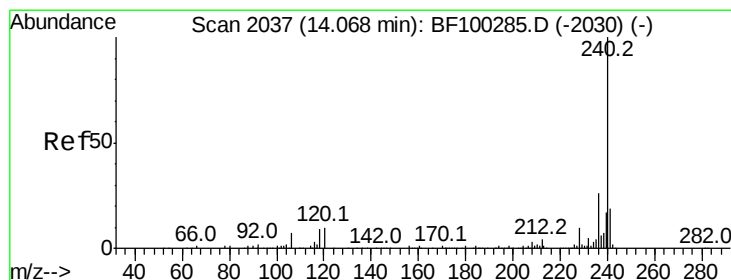
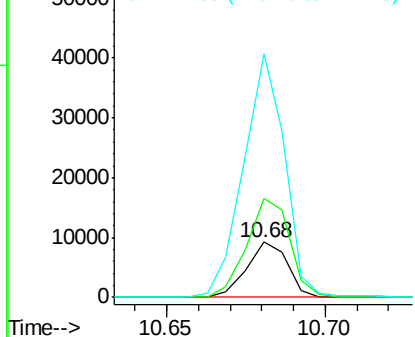



#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.02 min Scan# 2028
Delta R.T. -0.01 min
Lab File: BF100891.D
Acq: 27 Nov 2017 14:52

Tgt Ion:240 Resp: 152337
Ion Ratio Lower Upper
240 100
120 11.4 9.5 14.3
236 25.5 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



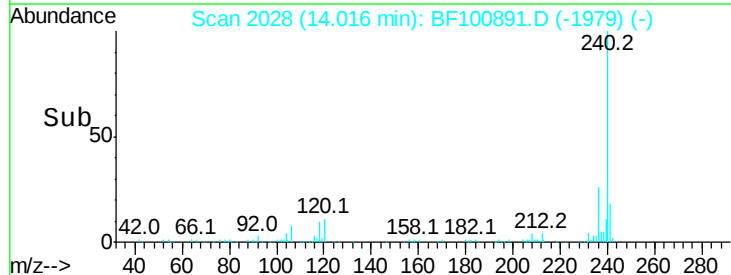
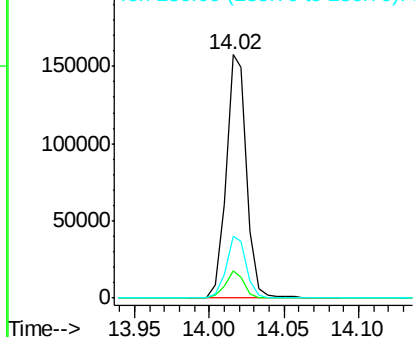




#78
 Terphenyl-d14
 Concen: 67.257 ng
 RT: 12.96 min Scan# 1849
 Delta R.T. -0.01 min
 Lab File: BF100891.D
 Acq: 27 Nov 2017 14:52

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:244 Resp: 445909
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.4 8.0
 122 10.4 11.0 16.4#

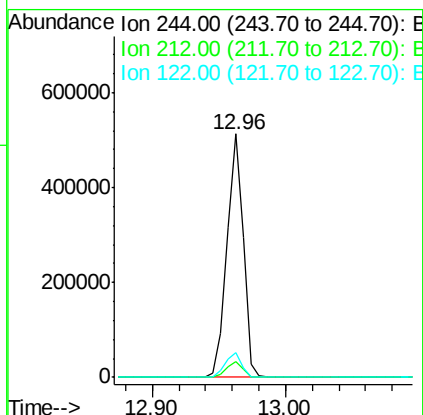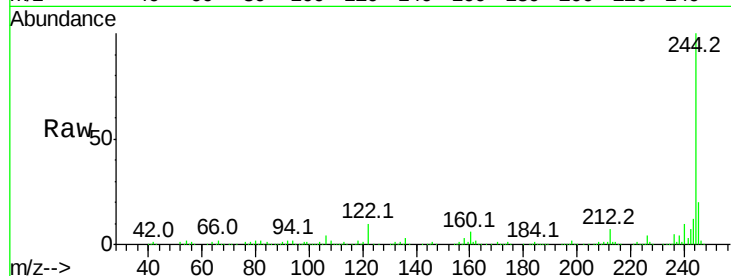

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.49 min Scan# 2278
 Delta R.T. -0.01 min
 Lab File: BF100891.D
 Acq: 27 Nov 2017 14:52

Tgt Ion:264 Resp: 164148
 Ion Ratio Lower Upper
 264 100
 260 22.8 19.2 28.8
 265 21.1 17.5 26.3

