

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112717\
 Data File : BF100892.D
 Acq On : 27 Nov 2017 15:19
 Operator : SJ/JU
 Sample : I6570-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Nov 27 21:57:47 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 14:11:25 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	79441	20.00	ng	0.00
21) Naphthalene-d8	8.14	136	314426	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	146026	20.00	ng	0.00
63) Phenanthrene-d10	11.38	188	270261	20.00	ng	0.00
75) Chrysene-d12	14.02	240	164025	20.00	ng	0.00
86) Perylene-d12	15.49	264	175085	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	375319	75.73	ng	0.00
7) Phenol-d6	6.49	99	455023	74.46	ng	0.00
23) Nitrobenzene-d5	7.42	82	281144	59.12	ng	0.00
41) 2,4,6-Tribromophenol	10.69	330	128800	86.56	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	539059	56.21	ng	0.00
78) Terphenyl-d14	12.96	244	457308	64.06	ng	0.00
Target Compounds						
10) Phenol	6.50	94	17360	2.706	ng	96
19) n-Nitroso-di-n-propylamine	7.42	70	36953	8.719	ng	# 77
25) Isophorone	7.42	82	281142	28.131	ng	# 64
47) 2-Nitroaniline	9.60	65	602	2.993	ng	# 1
49) Dimethylphthalate	9.60	163	73881	6.627	ng	99
56) 2,4-Dinitrotoluene	9.89	165	18622	6.689	ng	# 21
66) 4-Bromophenyl-phenylether	10.69	248	8268	2.854	ng	# 1
83) Bis(2-ethylhexyl)phthalate	13.99	149	19157	3.055	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112717\
Data File : BF100892.D
Acq On : 27 Nov 2017 15:19
Operator : SJ/JU
Sample : I6570-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Nov 27 21:57:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 14:11:25 2017
Response via : Initial Calibration

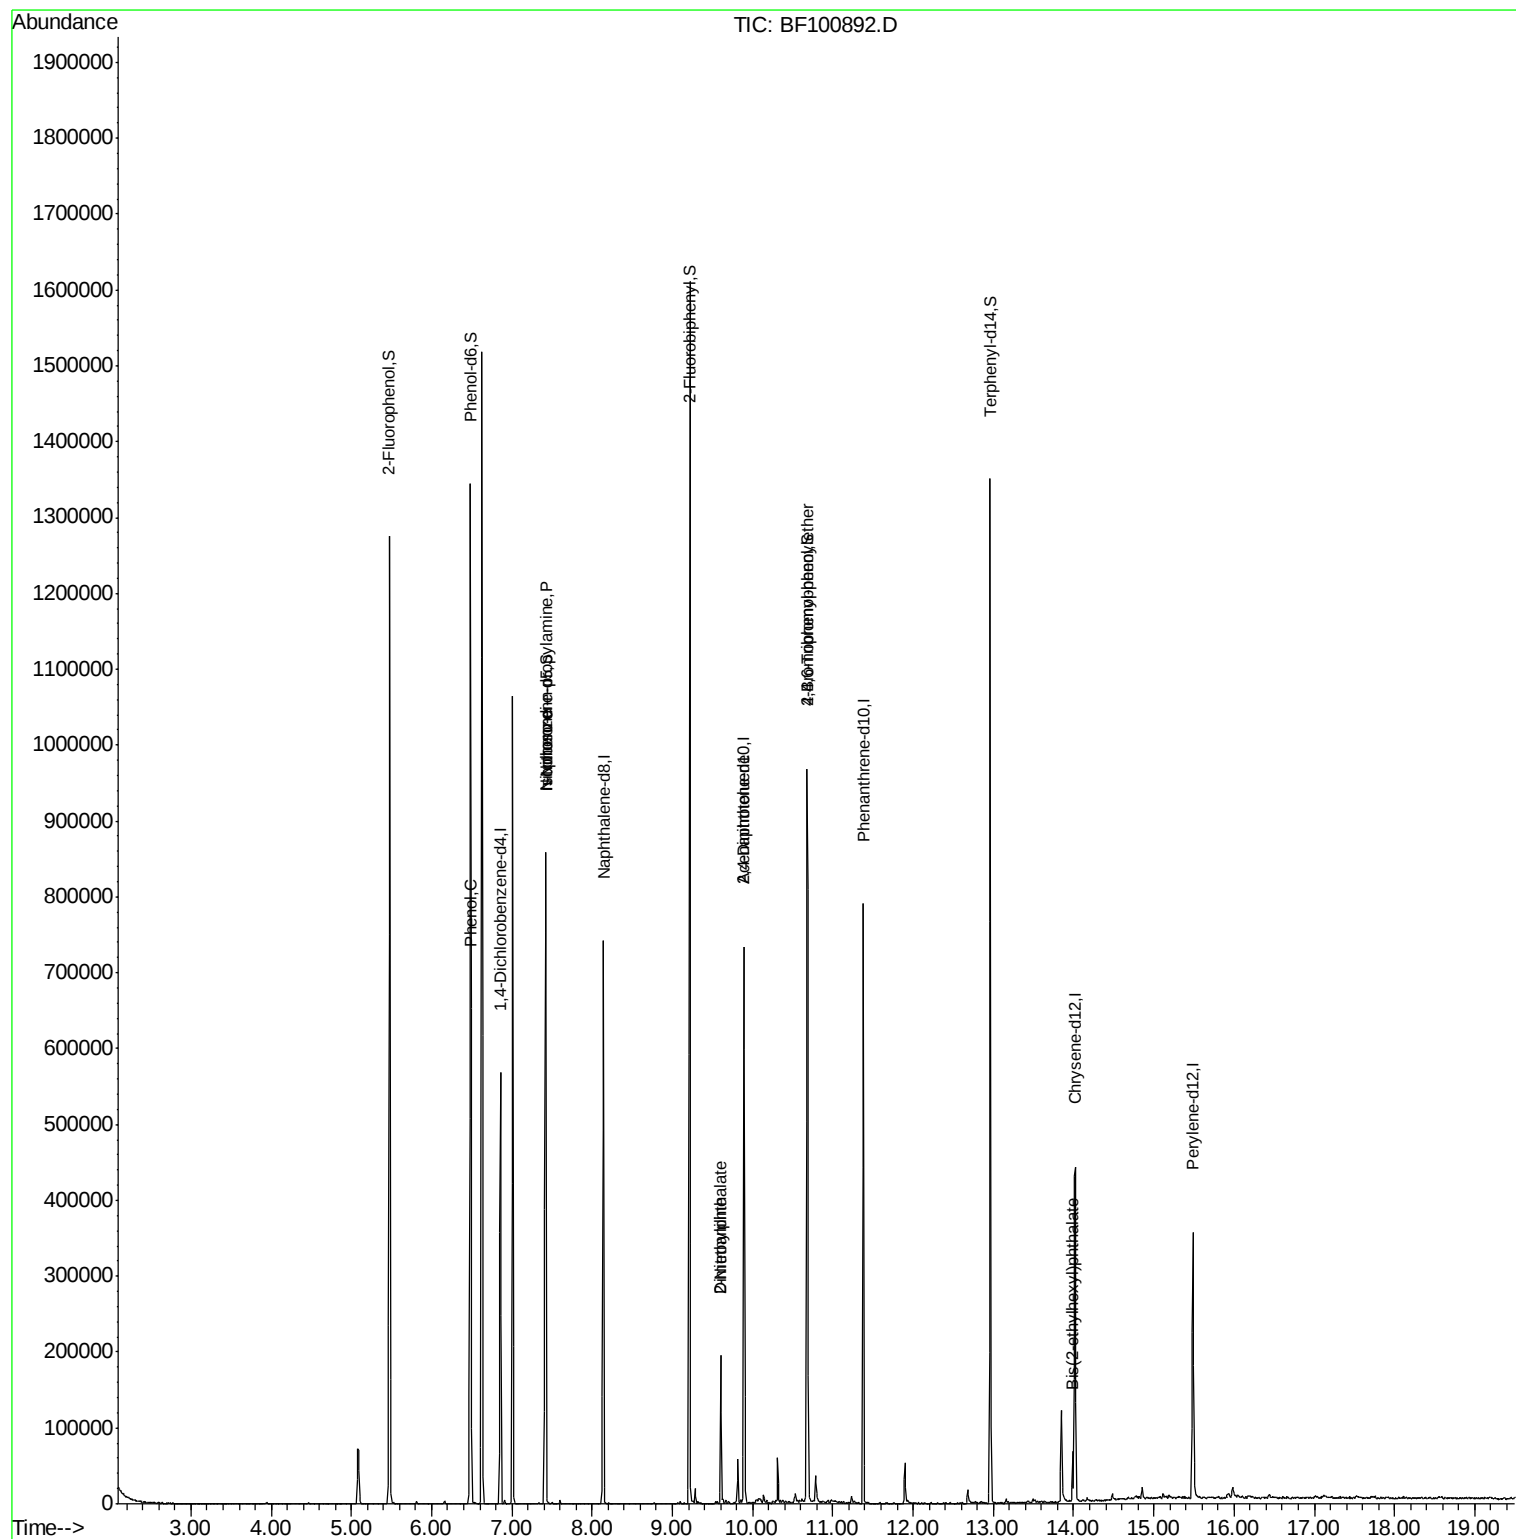

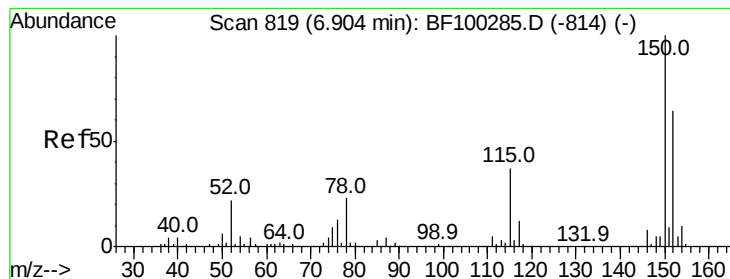


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.86 min Scan# 811
Delta R.T. -0.00 min
Lab File: BF100892.D
Acq: 27 Nov 2017 15:19

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 79441
Ion Ratio Lower Upper
152 100
150 153.9 124.6 186.8
115 59.5 50.1 75.1

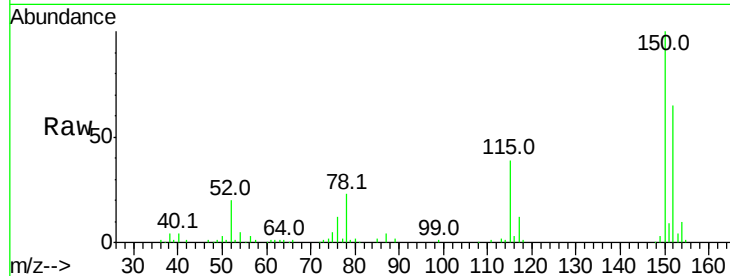


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

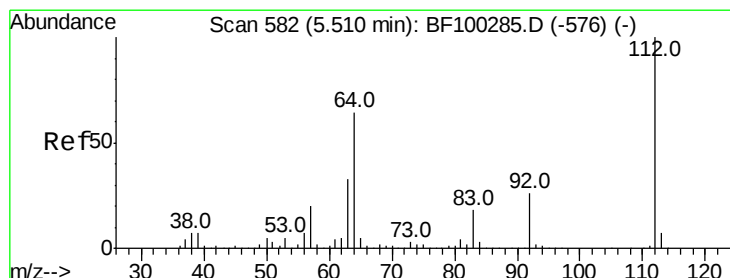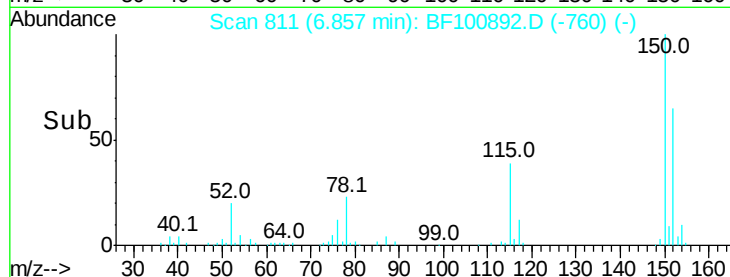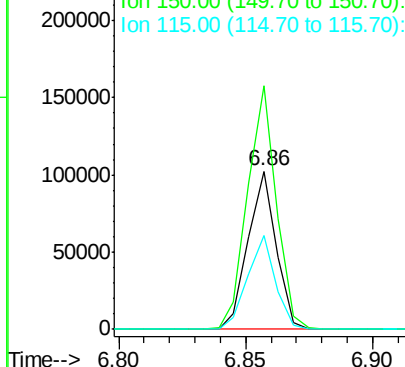



#5

2-Fluorophenol
Concen: 75.733 ng
RT: 5.47 min Scan# 576
Delta R.T. -0.00 min
Lab File: BF100892.D
Acq: 27 Nov 2017 15:19

Tgt Ion:112 Resp: 375319
Ion Ratio Lower Upper
112 100
64 60.2 47.9 71.9
63 31.5 23.7 35.5

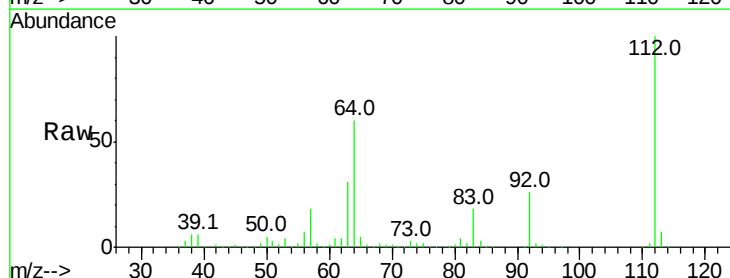

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

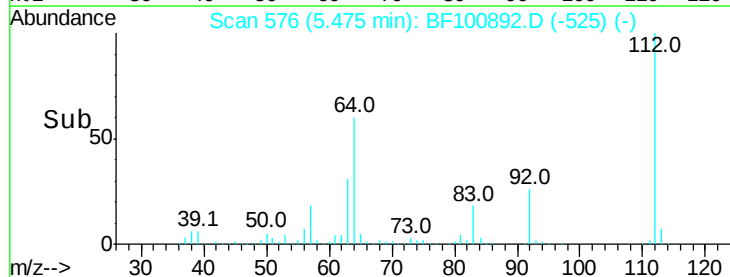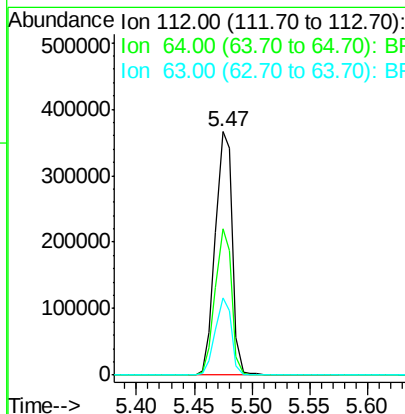



#7

Phenol-d6

Concen: 74.458 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF100892.D

Acq: 27 Nov 2017 15:19

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 455023

Ion Ratio Lower Upper

99 100

42 19.8 14.5 21.7

71 34.1 25.4 38.0

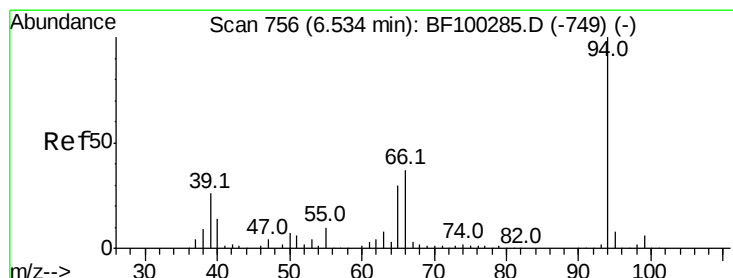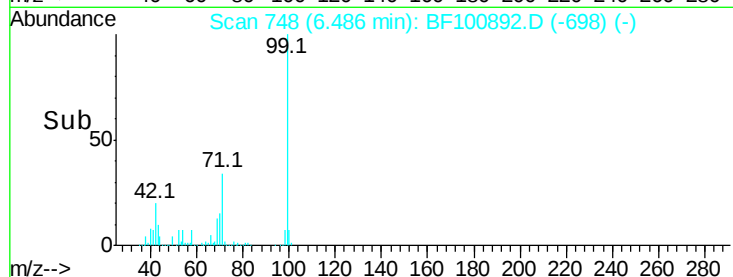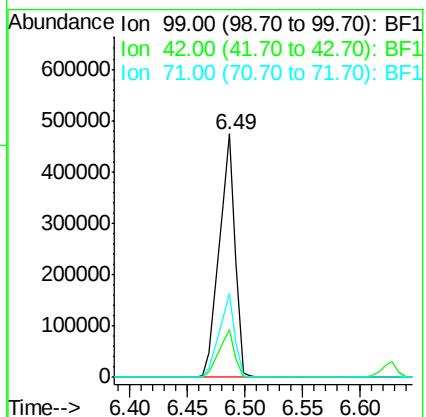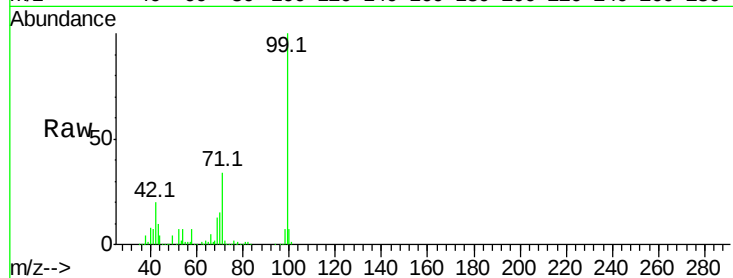

#10

Phenol

Concen: 2.706 ng

RT: 6.50 min Scan# 750

Delta R.T. -0.01 min

Lab File: BF100892.D

Acq: 27 Nov 2017 15:19




Tgt Ion: 94 Resp: 17360


Ion Ratio Lower Upper

94 100

65 28.2 7.9 47.9

66 32.6 16.2 56.2

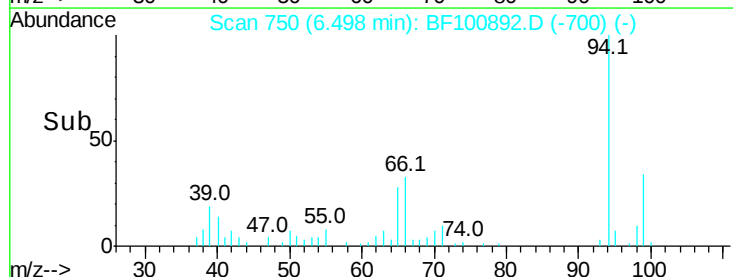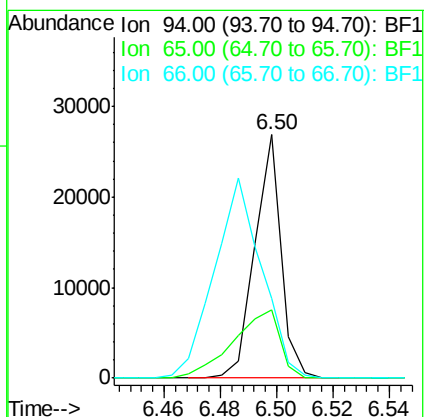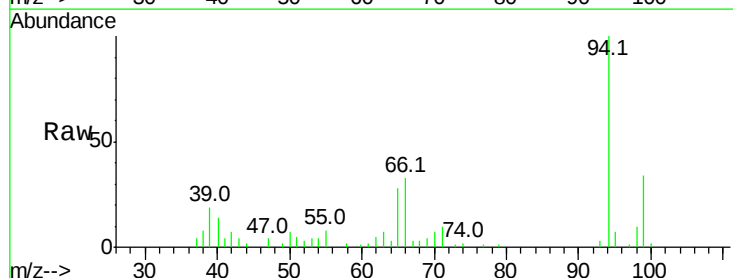

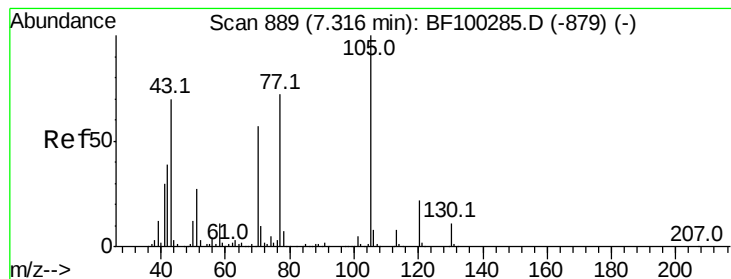

#19

n-Nitroso-di-n-propylamine

Concen: 8.719 ng

RT: 7.42 min Scan# 907

Delta R.T. 0.15 min

Lab File: BF100892.D

Acq: 27 Nov 2017 15:19

Instrument :

BNA_F

ClientSampled :

Tot Ion: 70 Resp: 36953


Ion Ratio Lower Upper

70 100

42 46.4 47.5 71.3#

101 0.0 7.4 11.2#

130 2.1 16.6 25.0#






Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

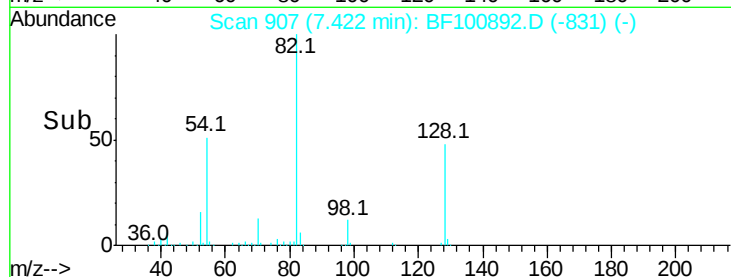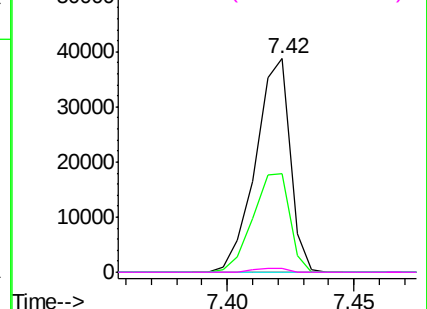

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.14 min Scan# 1029

Delta R.T. -0.01 min

Lab File: BF100892.D

Acq: 27 Nov 2017 15:19

Tgt Ion: 136 Resp: 314426


Ion Ratio Lower Upper

136 100

137 10.4 8.9 13.3

54 7.5 6.6 9.8

68 5.2 5.0 7.4






Abundance Ion 136.00 (135.70 to 136.70): BF1

Ion 137.00 (136.70 to 137.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



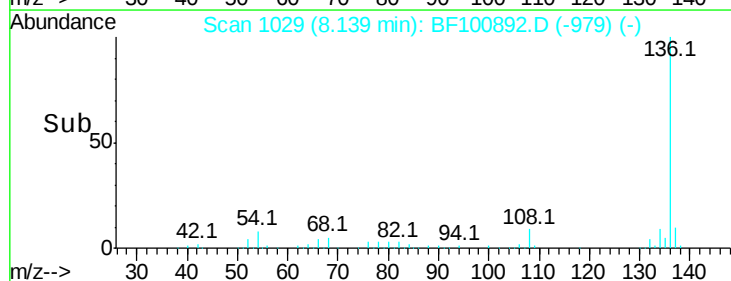
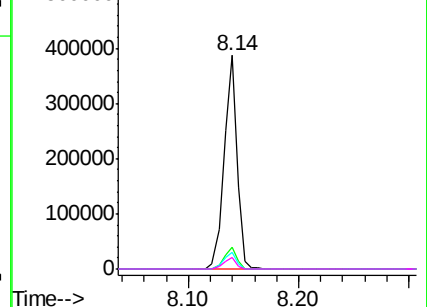


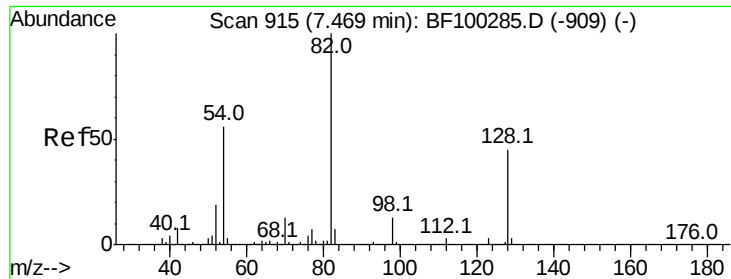

#23
 Nitrobenzene-d5
 Concen: 59.115 ng
 RT: 7.42 min Scan# 907
 Delta R.T. -0.01 min
 Lab File: BF100892.D
 Acq: 27 Nov 2017 15:19




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
82	100		
128	47.7	36.1	54.1
54	51.2	41.4	62.2

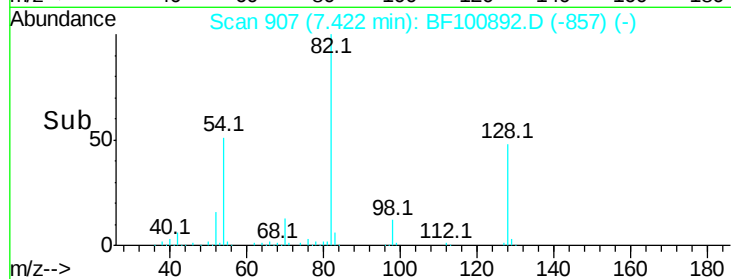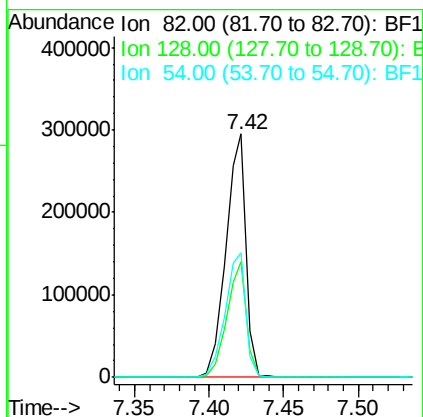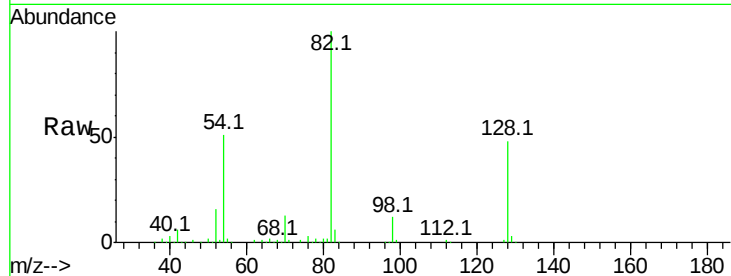

#25
 Isophorone
 Concen: 28.131 ng
 RT: 7.42 min Scan# 907
 Delta R.T. -0.26 min
 Lab File: BF100892.D
 Acq: 27 Nov 2017 15:19

Tgt Ion	Ratio	Lower	Upper
82	100		
95	0.0	5.2	7.8#
138	0.0	14.9	22.3#

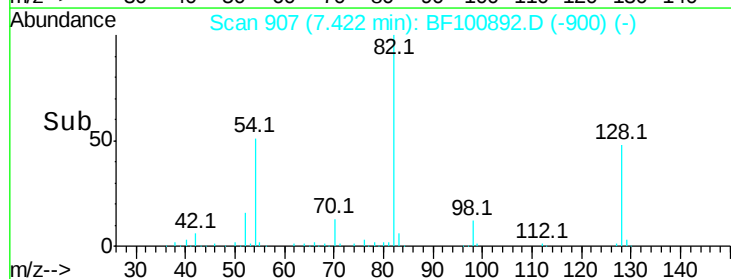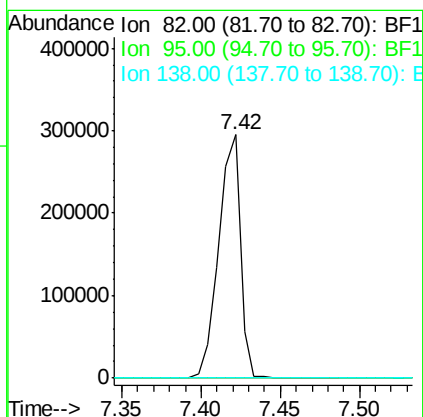


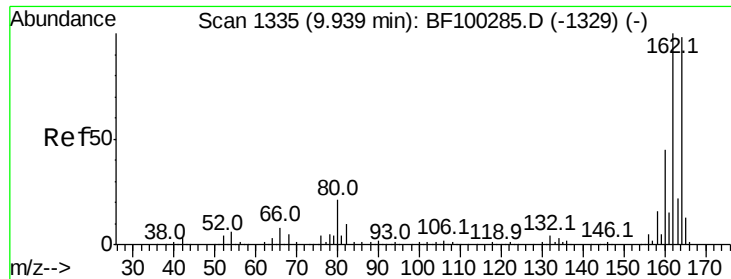




#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.89 min Scan# 1327
Delta R.T. -0.01 min
Lab File: BF100892.D
Acq: 27 Nov 2017 15:19

Instrument :
BNA_F
ClientSampled :

Tot Ion:164 Resp: 146026
Ion Ratio Lower Upper
164 100
162 105.3 86.1 129.1
160 45.1 38.3 57.5

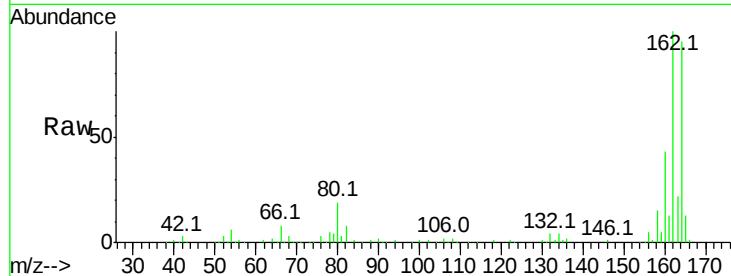


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

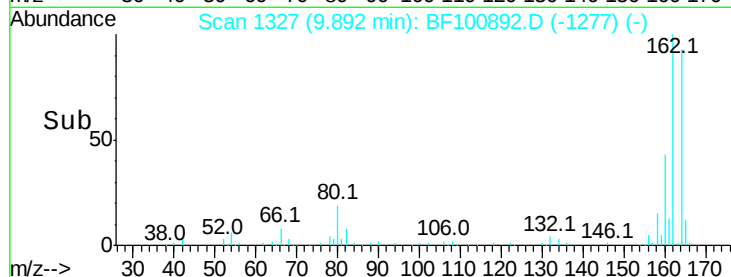
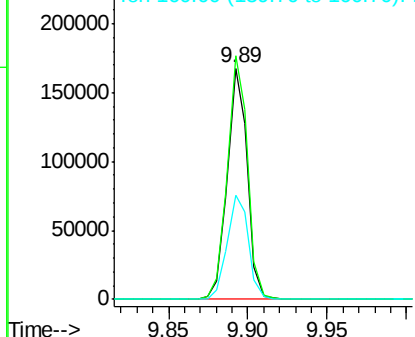



#41
2,4,6-Tribromophenol
Concen: 86.559 ng
RT: 10.69 min Scan# 1462
Delta R.T. -0.01 min
Lab File: BF100892.D
Acq: 27 Nov 2017 15:19

Tgt Ion:330 Resp: 128800
Ion Ratio Lower Upper
330 100
332 94.8 77.0 115.6
141 29.1 29.9 44.9#



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

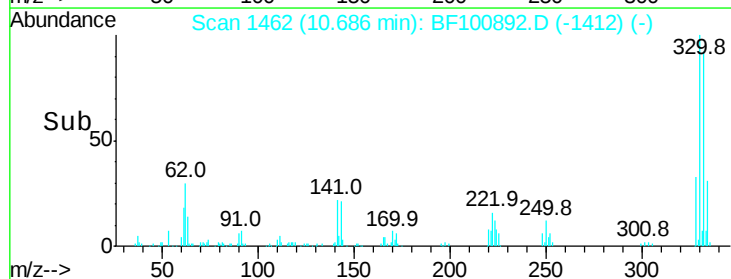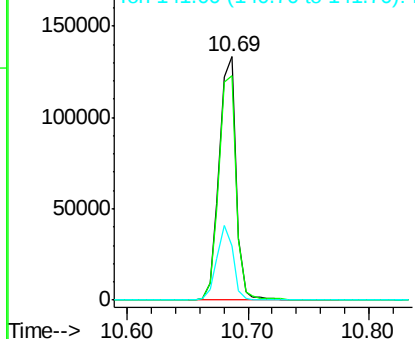




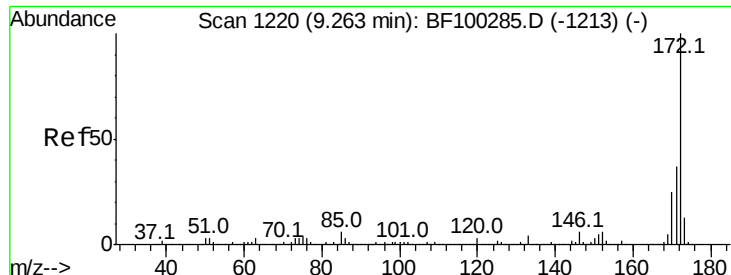


#44
 2-Fluorobiphenyl
 Concen: 56.211 ng
 RT: 9.22 min Scan# 1212
 Delta R.T. -0.01 min
 Lab File: BF100892.D
 Acq: 27 Nov 2017 15:19

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:172 Resp: 539059




Ion	Ratio	Lower	Upper
172	100		
171	35.6	29.7	44.5
170	23.3	19.6	29.4

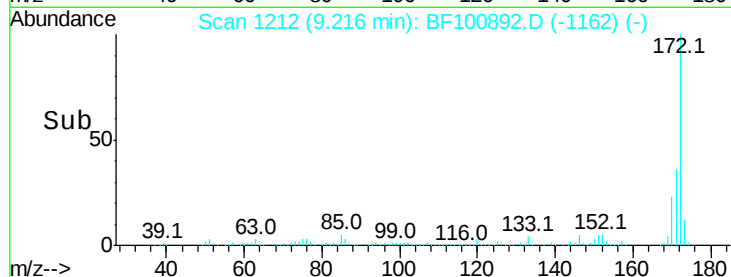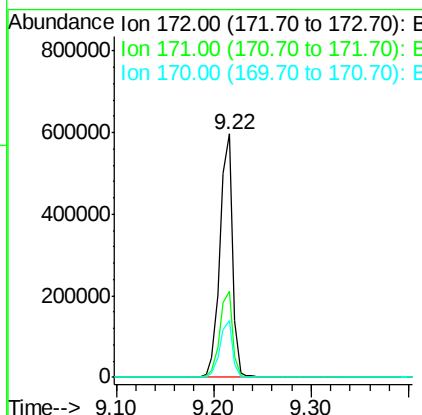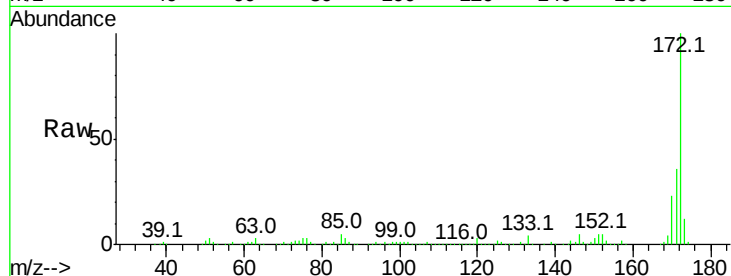


#47
 2-Nitroaniline
 Concen: 2.993 ng
 RT: 9.60 min Scan# 1278
 Delta R.T. 0.16 min
 Lab File: BF100892.D
 Acq: 27 Nov 2017 15:19

Tgt Ion: 65 Resp: 602

Ion	Ratio	Lower	Upper
65	100		
92	816.0	55.8	83.6#
138	0.0	91.2	136.8#


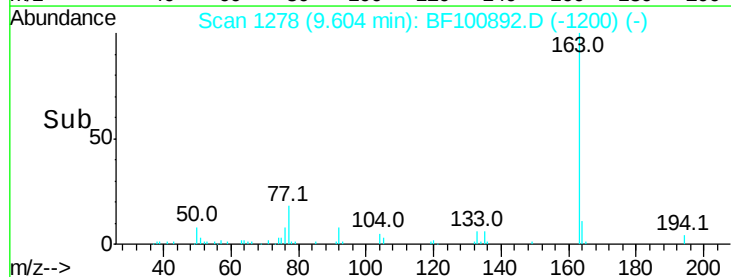
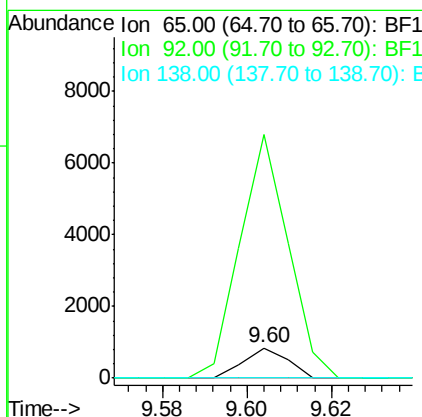
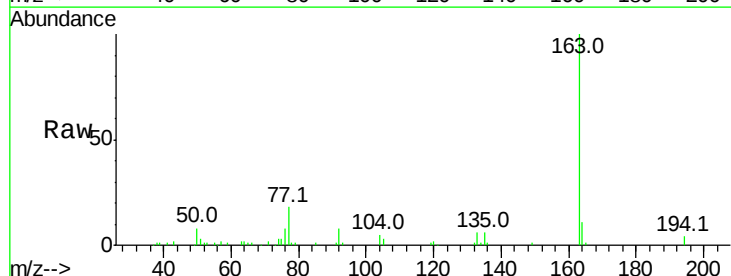


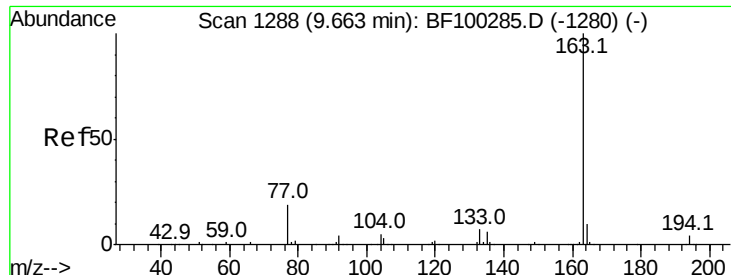

#49
Dimethylphthalate
Concen: 6.627 ng
RT: 9.60 min Scan# 1278
Delta R.T. -0.02 min
Lab File: BF100892.D
Acq: 27 Nov 2017 15:19




Instrument :
BNA_F
ClientSampleId :


Tot Ion:163 Resp: 73881
Ion Ratio Lower Upper
163 100
194 3.7 2.7 4.1
164 10.8 8.2 12.2

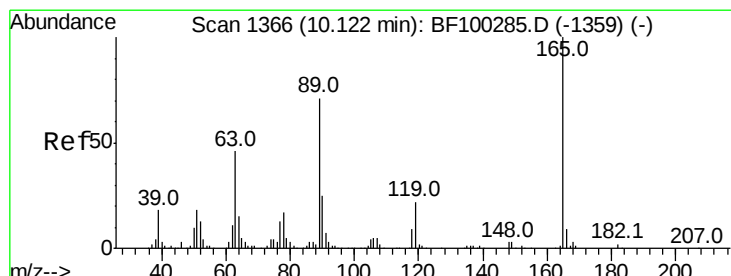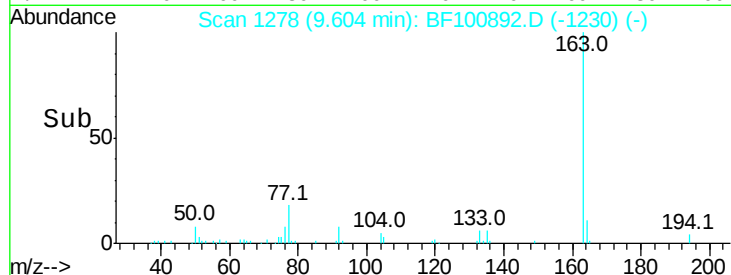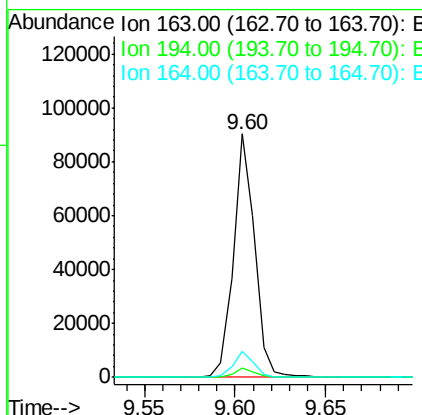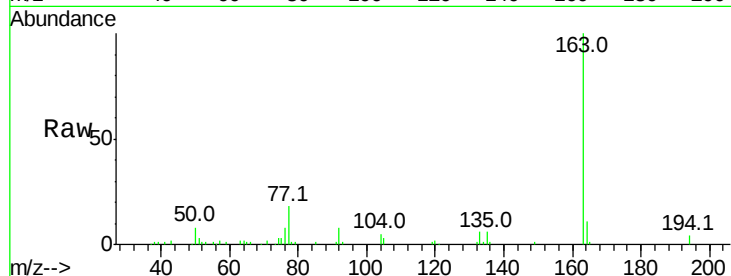

#56
2,4-Dinitrotoluene
Concen: 6.689 ng
RT: 9.89 min Scan# 1327
Delta R.T. -0.19 min
Lab File: BF100892.D
Acq: 27 Nov 2017 15:19

Tgt Ion:165 Resp: 18622
Ion Ratio Lower Upper
165 100
63 0.0 36.4 54.6#
89 0.0 57.8 86.6#
182 0.0 1.6 2.4#


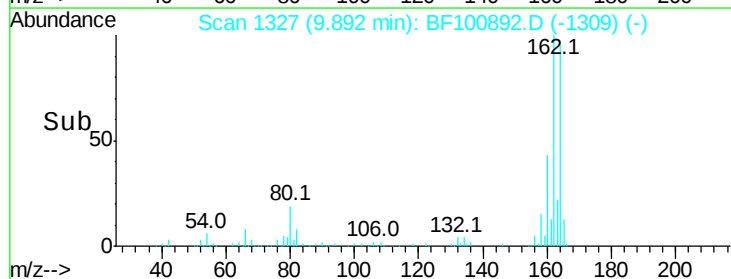
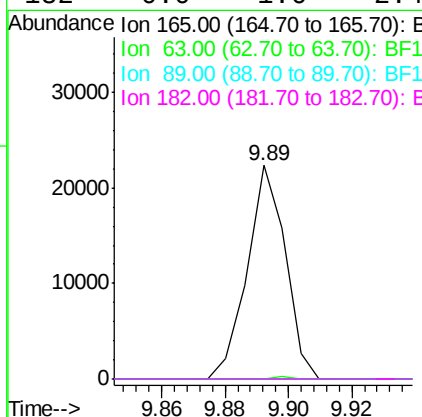
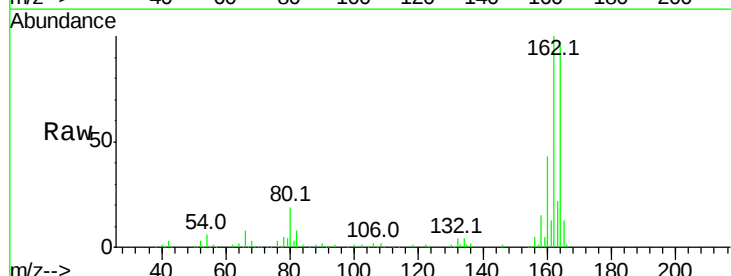


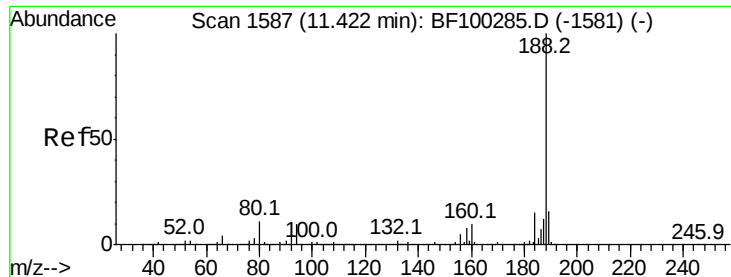

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.38 min Scan# 1580
 Delta R.T. -0.01 min
 Lab File: BF100892.D
 Acq: 27 Nov 2017 15:19




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:188 Resp: 270261
 Ion Ratio Lower Upper
 188 100
 94 9.1 8.5 12.7
 80 9.2 9.2 13.8

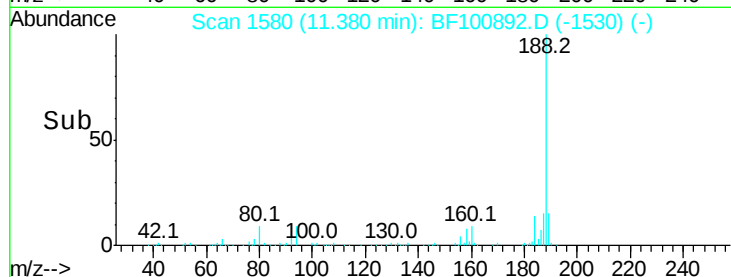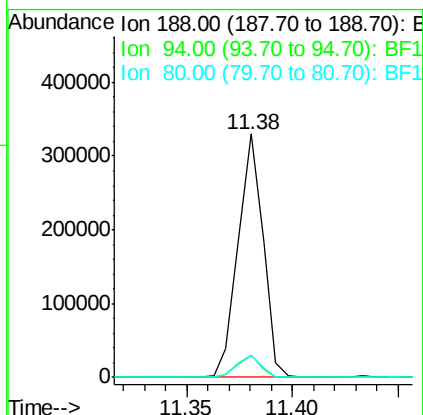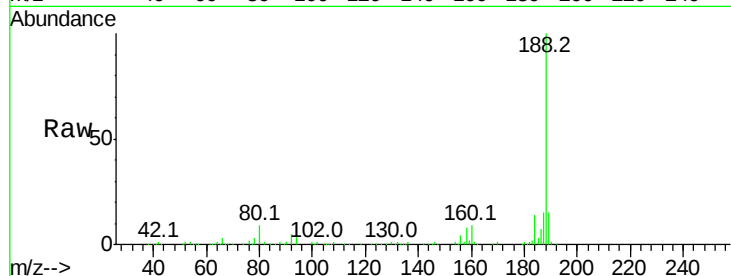

#66
 4-Bromophenyl-phenylether
 Concen: 2.854 ng
 RT: 10.69 min Scan# 1462
 Delta R.T. -0.24 min
 Lab File: BF100892.D
 Acq: 27 Nov 2017 15:19

Tgt Ion:248 Resp: 8268
 Ion Ratio Lower Upper
 248 100
 250 183.2 76.9 115.3#
 141 350.9 74.4 111.6#

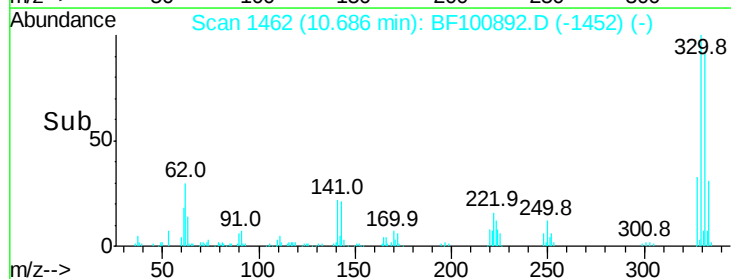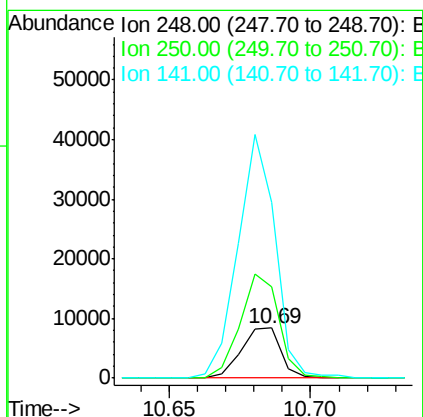

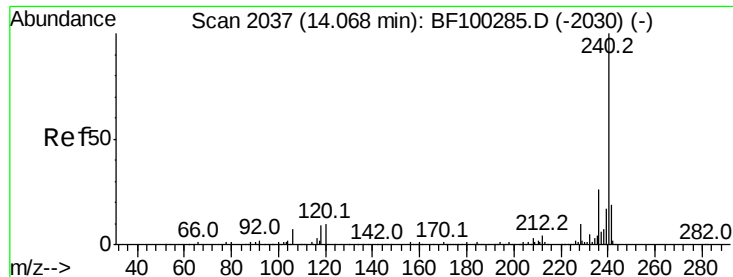

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.02 min Scan# 2029

Delta R.T. -0.01 min

Lab File: BF100892.D

Acq: 27 Nov 2017 15:19

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 164025

Ion Ratio Lower Upper

240 100

120 8.8 9.5 14.3#




236 25.8 20.7 31.1

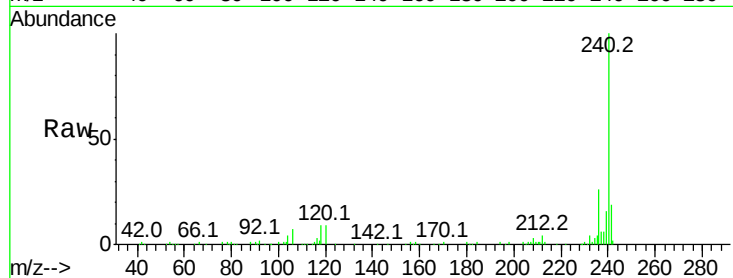

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

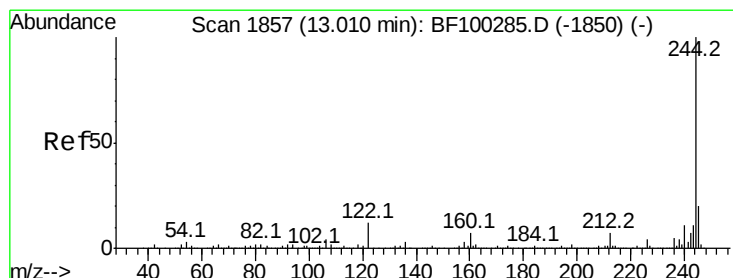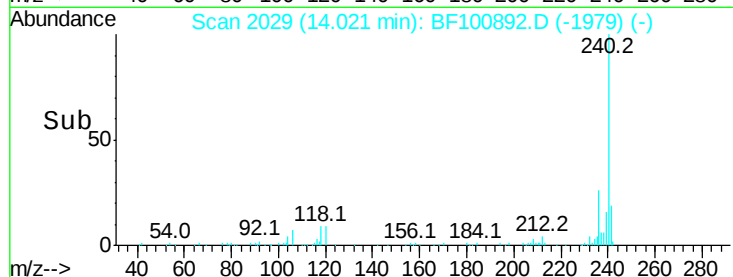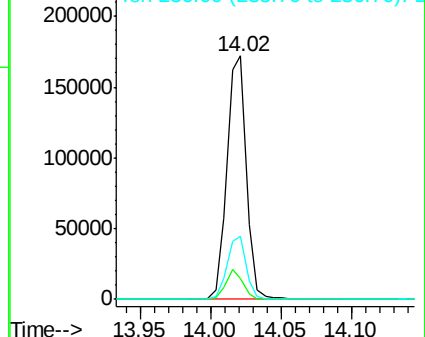

#78

Terphenyl-d14

Concen: 64.061 ng

RT: 12.96 min Scan# 1849

Delta R.T. -0.01 min

Lab File: BF100892.D

Acq: 27 Nov 2017 15:19


Tgt Ion:244 Resp: 457308

Ion Ratio Lower Upper

244 100

212 6.4 5.4 8.0



122 10.9 11.0 16.4#

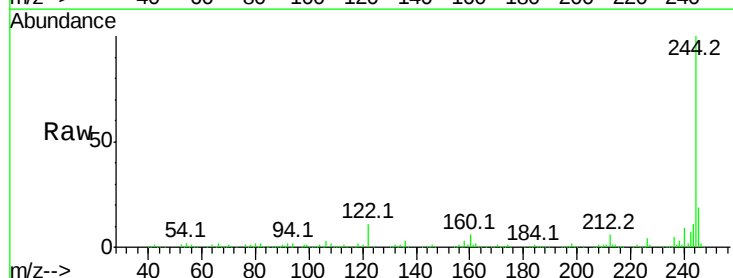


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



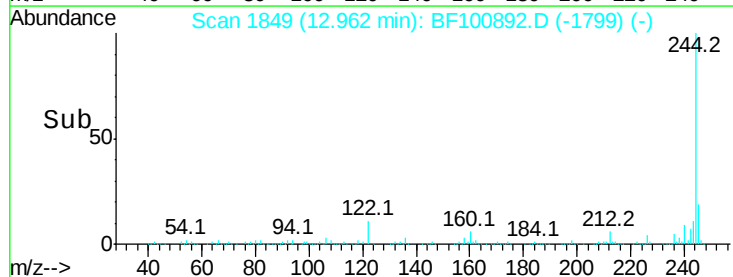
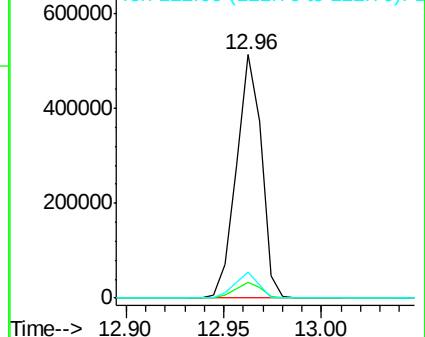


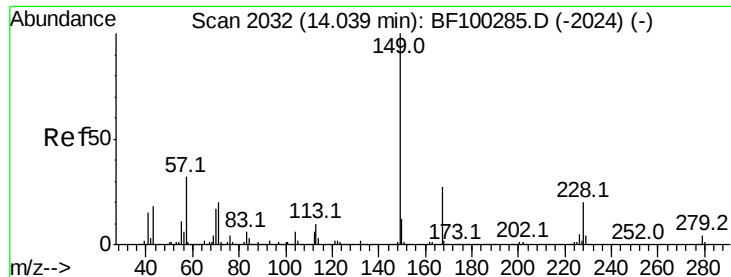

#83
Bis(2-ethylhexyl)phthalate
Concen: 3.055 ng
RT: 13.99 min Scan# 2024
Delta R.T. -0.00 min
Lab File: BF100892.D
Acq: 27 Nov 2017 15:19

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
149	100		
167	27.9	21.3	31.9
279	3.7	3.0	4.4

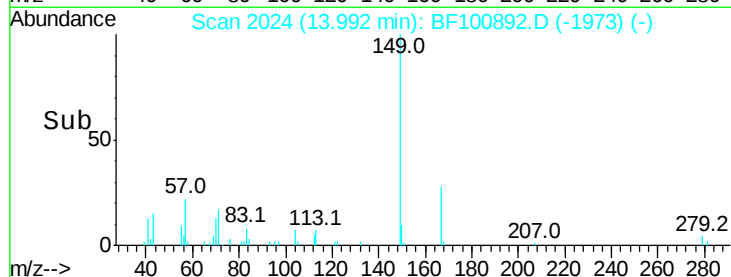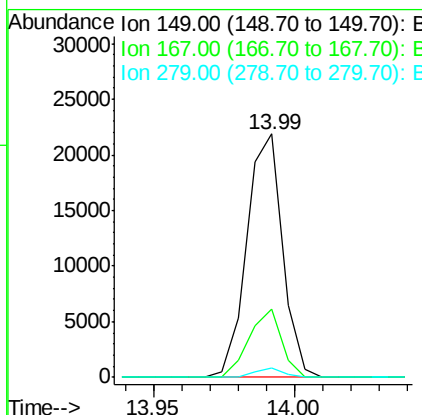

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.49 min Scan# 2278
Delta R.T. -0.01 min
Lab File: BF100892.D
Acq: 27 Nov 2017 15:19

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.8	19.2	28.8
265	21.8	17.5	26.3

