

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112717\
 Data File : BF100915.D
 Acq On : 28 Nov 2017 2:24
 Operator : SJ/JU
 Sample : I6584-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Nov 28 03:26:02 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 27 14:11:25 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	58911	20.00	ng	0.00
21) Naphthalene-d8	8.14	136	224533	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	102008	20.00	ng	0.00
63) Phenanthrene-d10	11.38	188	178428	20.00	ng	0.00
75) Chrysene-d12	14.02	240	124335	20.00	ng	-0.01
86) Perylene-d12	15.49	264	120385	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	150259	40.89	ng	0.00
7) Phenol-d6	6.48	99	108813	24.01	ng	-0.01
23) Nitrobenzene-d5	7.42	82	375198	110.48	ng	0.00
41) 2,4,6-Tribromophenol	10.68	330	98750	95.00	ng	-0.01
44) 2-Fluorobiphenyl	9.22	172	728065	108.68	ng	0.00
78) Terphenyl-d14	12.97	244	568685	105.09	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.42	70	49084	15.618	ng	# 79
25) Isophorone	7.42	82	375194	52.572	ng	# 64
47) 2-Nitroaniline	9.22	65	1047	3.305	ng	# 1
50) 2,6-Dinitrotoluene	9.89	165	12506	8.112	ng	# 24
56) 2,4-Dinitrotoluene	9.89	165	12506	6.430	ng	# 21
66) 4-Bromophenyl-phenylether	10.68	248	6409	3.351	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112717\
Data File : BF100915.D
Acq On : 28 Nov 2017 2:24
Operator : SJ/JU
Sample : I6584-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Nov 28 03:26:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 14:11:25 2017
Response via : Initial Calibration

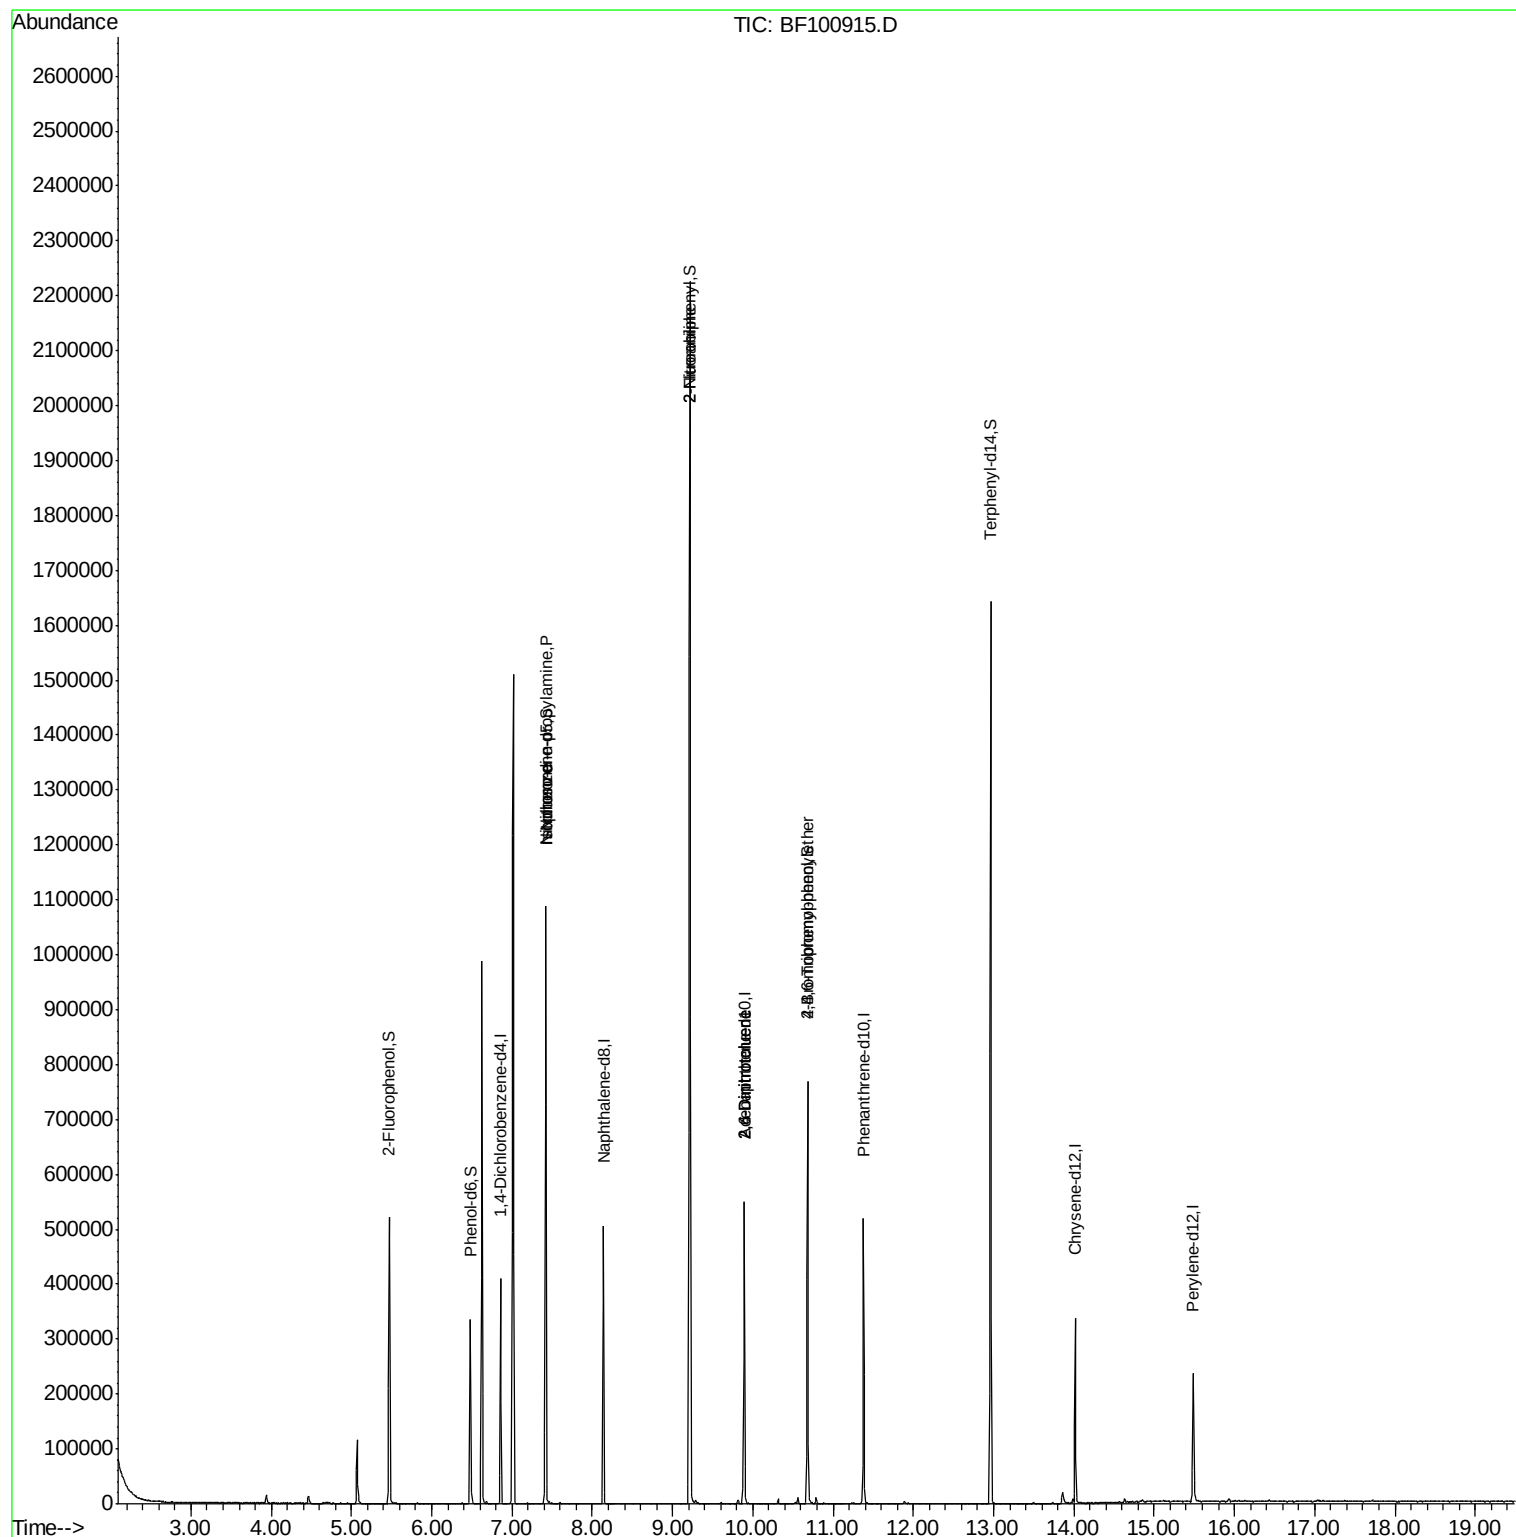

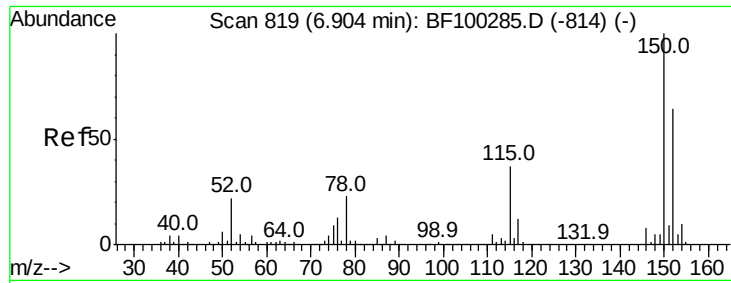


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.86 min Scan# 811
Delta R.T. 0.00 min
Lab File: BF100915.D
Acq: 28 Nov 2017 2:24

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.1	124.6	186.8
115	56.3	50.1	75.1

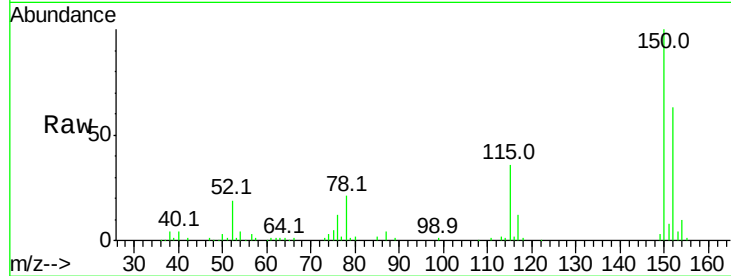


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

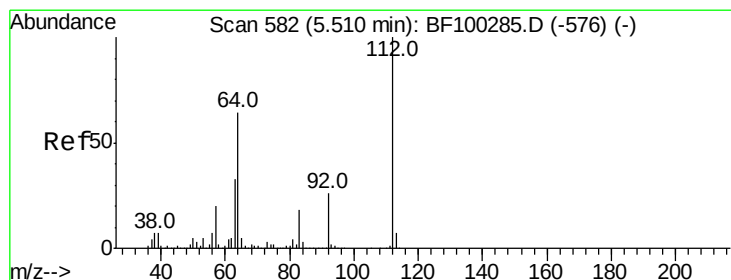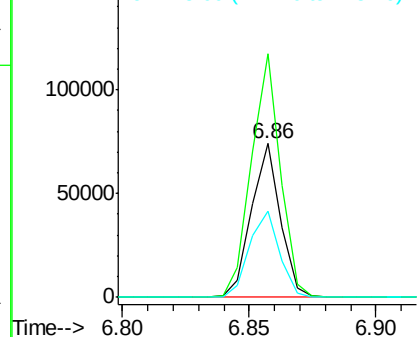



#5


2-Fluorophenol
Concen: 40.886 ng
RT: 5.47 min Scan# 576
Delta R.T. 0.00 min
Lab File: BF100915.D
Acq: 28 Nov 2017 2:24

Tgt Ion	Ratio	Lower	Upper
112	100		
64	53.2	47.9	71.9
63	26.9	23.7	35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

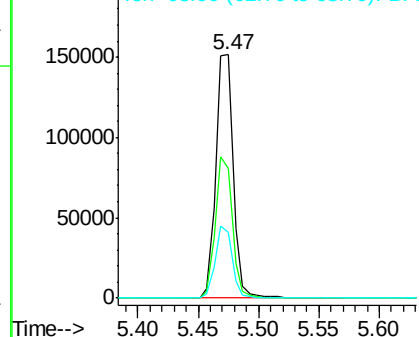

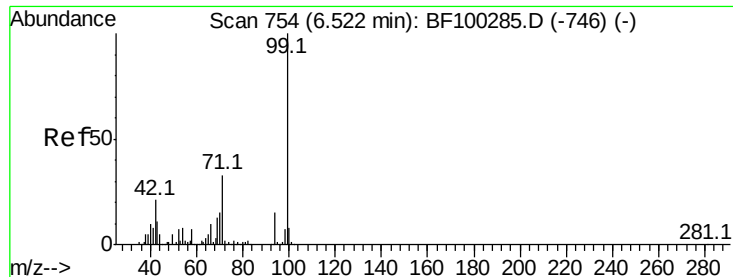

#7

Phenol-d6

Concen: 24.011 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.01 min

Lab File: BF100915.D

Acq: 28 Nov 2017 2:24

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 108813

Ion Ratio Lower Upper

99 100

42 17.0 14.5 21.7

71 32.7 25.4 38.0

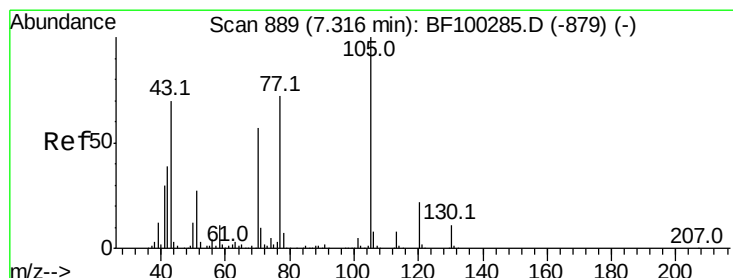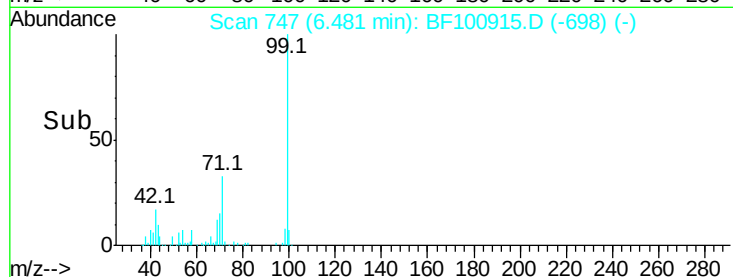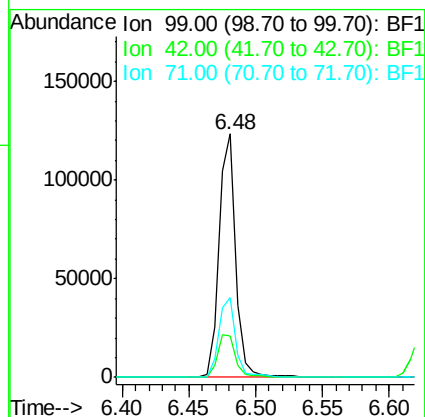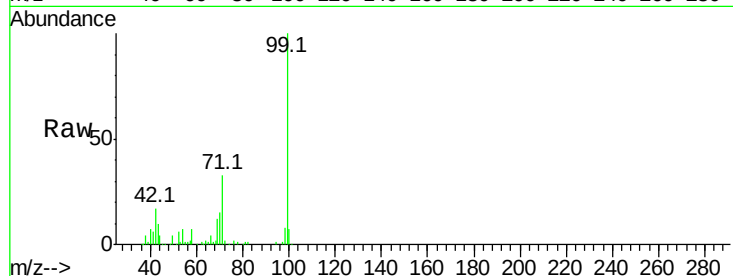

#19

n-Nitroso-di-n-propylamine

Concen: 15.618 ng

RT: 7.42 min Scan# 907

Delta R.T. 0.15 min

Lab File: BF100915.D

Acq: 28 Nov 2017 2:24

Tgt Ion: 70 Resp: 49084




Ion Ratio Lower Upper


70 100

42 49.6 47.5 71.3

101 0.0 7.4 11.2#

130 2.0 16.6 25.0#

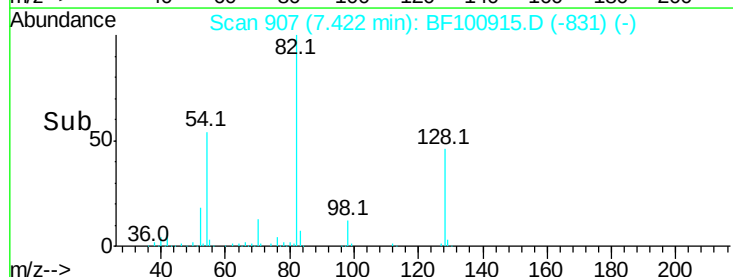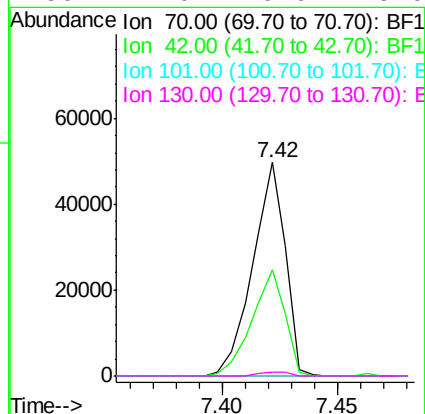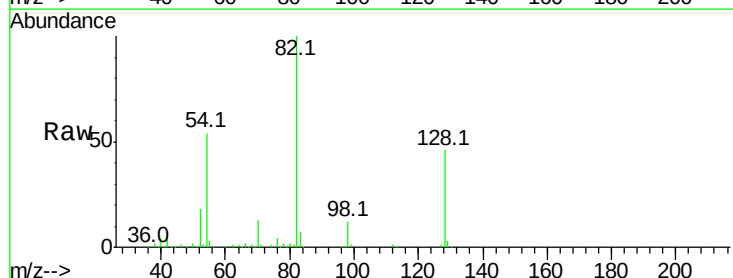

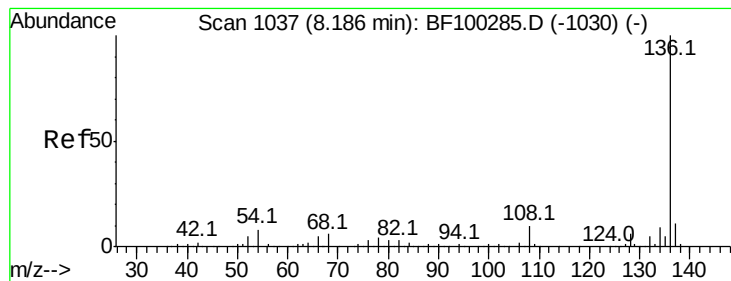

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.14 min Scan# 1029

Delta R.T. -0.01 min

Lab File: BF100915.D

Acq: 28 Nov 2017 2:24

Instrument :


BNA_F

ClientSampleId :

Tot Ion:136 Resp: 224533

Ion Ratio Lower Upper

136	100		
137	10.9	8.9	13.3
54	6.7	6.6	9.8
68	4.7	5.0	7.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

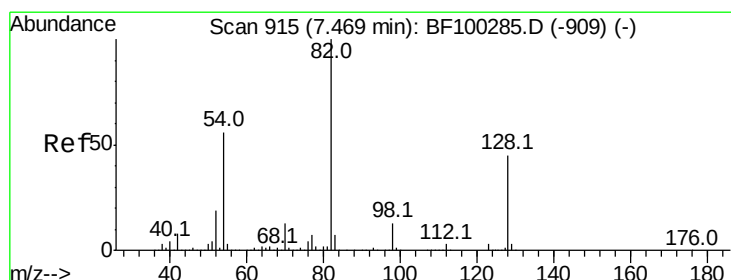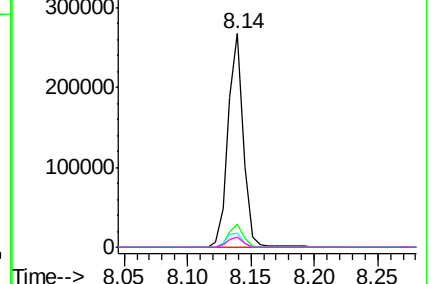

#23

Nitrobenzene-d5

Concen: 110.476 ng

RT: 7.42 min Scan# 907

Delta R.T. -0.01 min


Lab File: BF100915.D

Acq: 28 Nov 2017 2:24

Tgt Ion: 82 Resp: 375198

Ion Ratio Lower Upper



82	100		
128	45.8	36.1	54.1
54	53.9	41.4	62.2




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

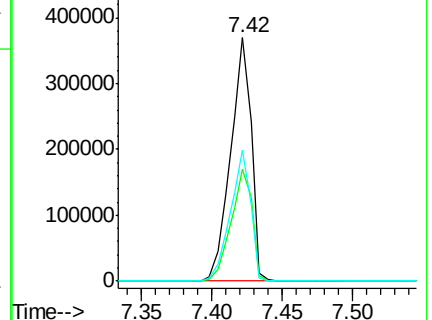

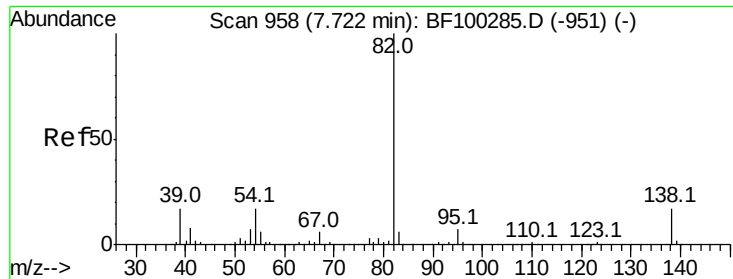

#25

Isophorone

Concen: 52.572 ng

RT: 7.42 min Scan# 907

Delta R.T. -0.26 min

Lab File: BF100915.D

Acq: 28 Nov 2017 2:24

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 82 Resp: 375194

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

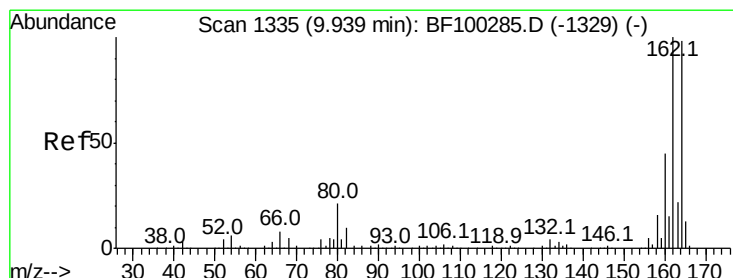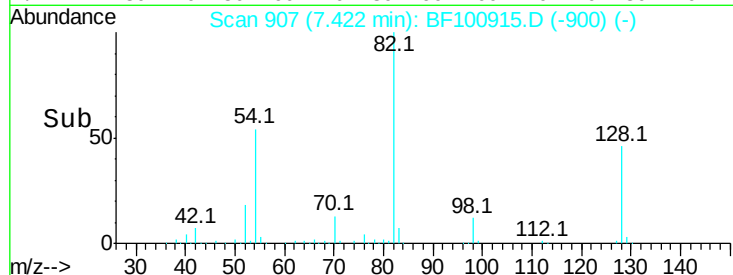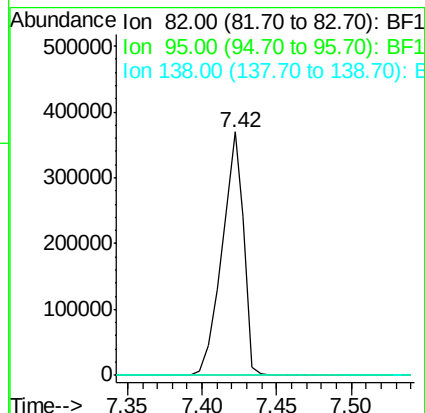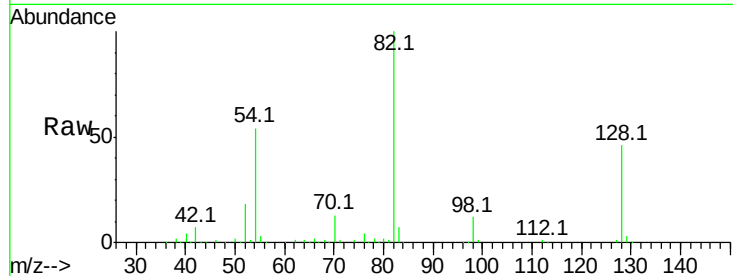

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.89 min Scan# 1327

Delta R.T. -0.01 min

Lab File: BF100915.D

Acq: 28 Nov 2017 2:24




Tgt Ion: 164 Resp: 102008


Ion Ratio Lower Upper

164 100

162 103.5 86.1 129.1

160 46.0 38.3 57.5

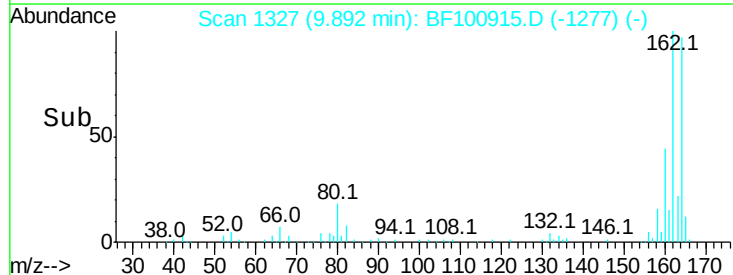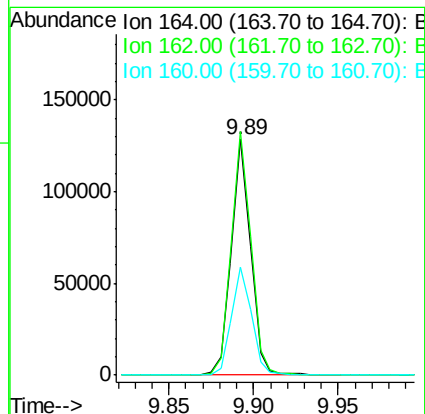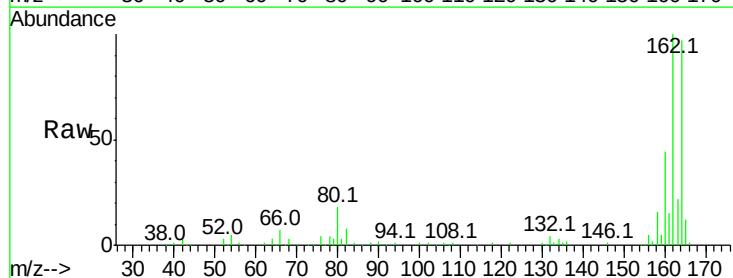







#41
 2,4,6-Tribromophenol
 Concen: 95.001 ng
 RT: 10.68 min Scan# 1461
 Delta R.T. -0.01 min
 Lab File: BF100915.D
 Acq: 28 Nov 2017 2:24

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	77.0	115.6
141	29.2	29.9	44.9#

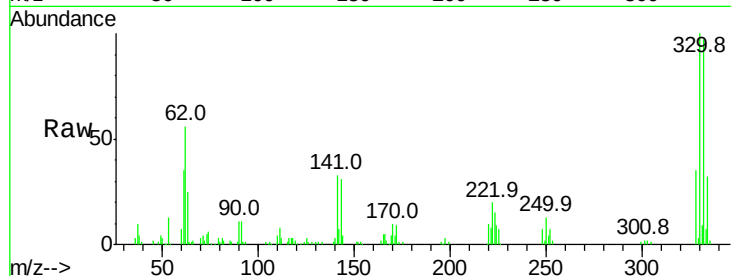


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


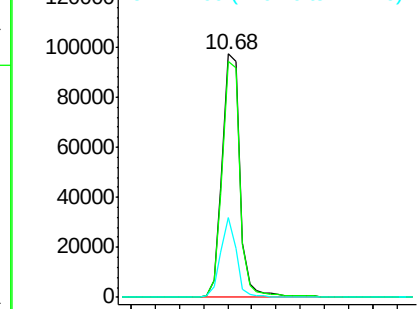



#44
 2-Fluorobiphenyl
 Concen: 108.681 ng
 RT: 9.22 min Scan# 1212
 Delta R.T. -0.01 min
 Lab File: BF100915.D
 Acq: 28 Nov 2017 2:24

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	29.7	44.5
170	24.3	19.6	29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

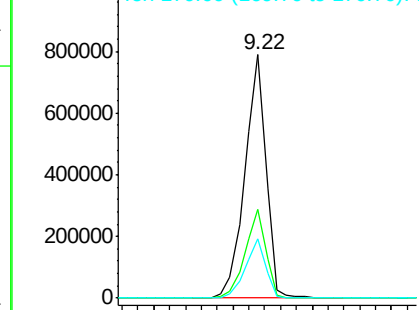

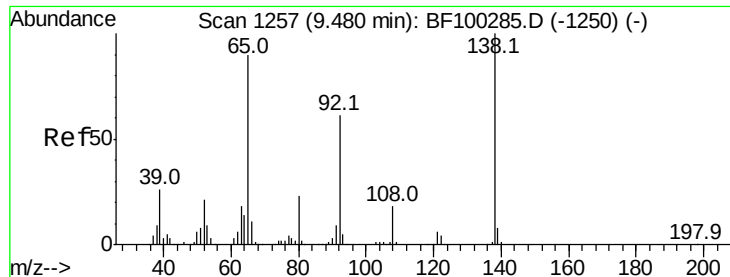

#47

2-Nitroaniline

Concen: 3.305 ng

RT: 9.22 min Scan# 1212

Delta R.T. -0.23 min

Lab File: BF100915.D

Acq: 28 Nov 2017 2:24

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 65 Resp: 1047

Ion Ratio Lower Upper

65 100

92 201.9 55.8 83.6#




138 0.0 91.2 136.8#

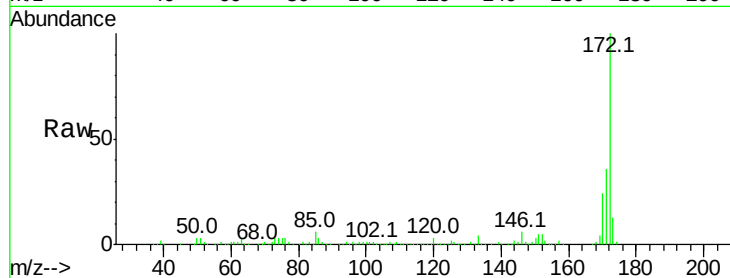

Abundance Ion 65.00 (64.70 to 65.70): BF1

Ion 92.00 (91.70 to 92.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

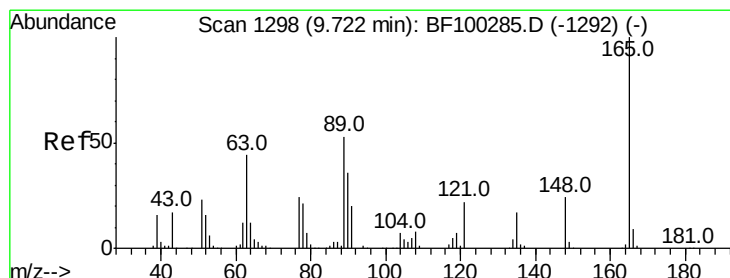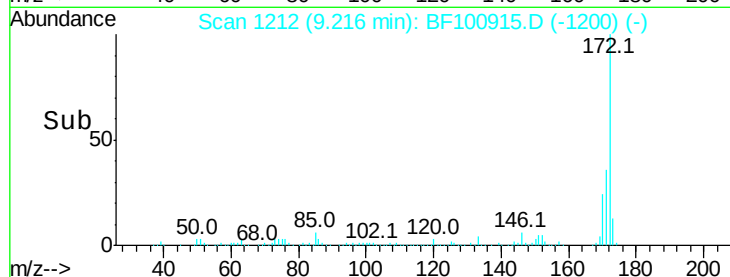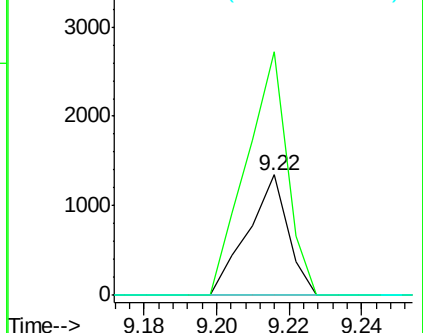

#50

2,6-Dinitrotoluene

Concen: 8.112 ng

RT: 9.89 min Scan# 1327

Delta R.T. 0.21 min

Lab File: BF100915.D

Acq: 28 Nov 2017 2:24


Tgt Ion: 165 Resp: 12506

Ion Ratio Lower Upper

165 100

63 0.0 44.7 67.1#



89 0.0 44.0 66.0#

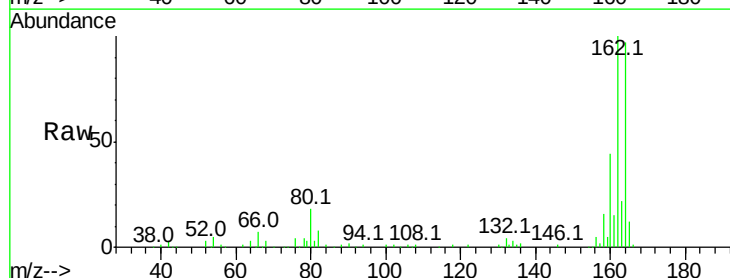


Abundance Ion 165.00 (164.70 to 165.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1



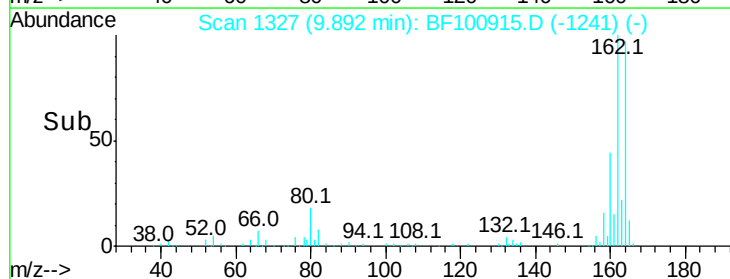
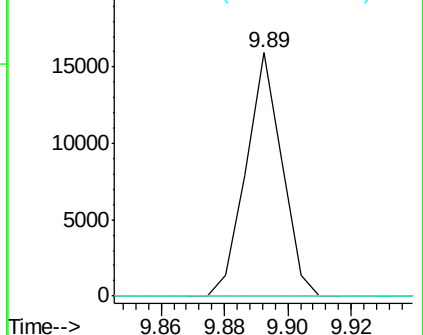




#56
 2,4-Dinitrotoluene
 Concen: 6.430 ng
 RT: 9.89 min Scan# 1327
 Delta R.T. -0.19 min
 Lab File: BF100915.D
 Acq: 28 Nov 2017 2:24




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:	165	Resp:	12506
Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.4	54.6#
89	0.0	57.8	86.6#
182	0.0	1.6	2.4#

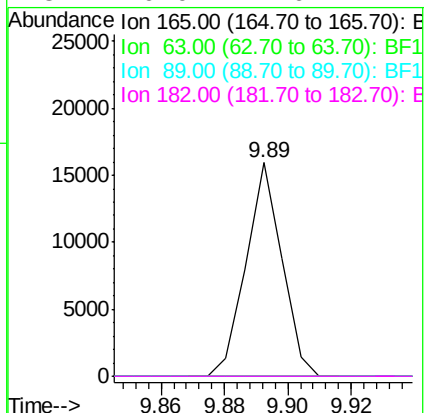

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.38 min Scan# 1580
 Delta R.T. -0.01 min
 Lab File: BF100915.D
 Acq: 28 Nov 2017 2:24

Tgt Ion:	188	Resp:	178428
Ion	Ratio	Lower	Upper
188	100		
94	7.4	8.5	12.7#
80	8.8	9.2	13.8#

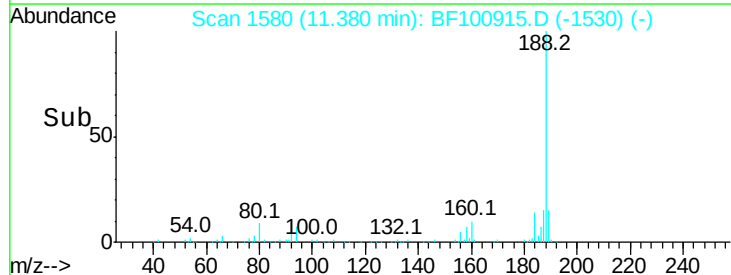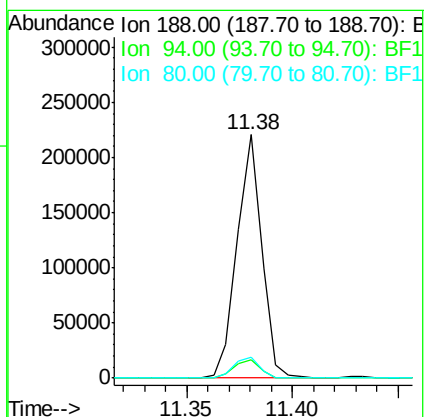


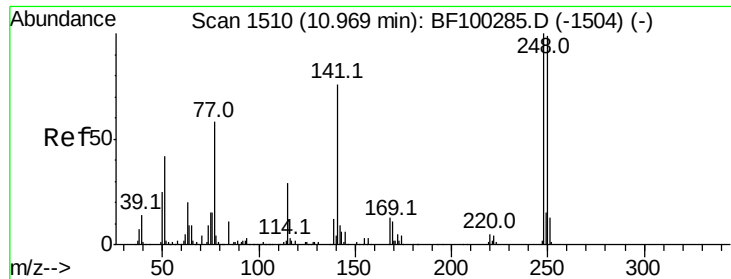




#66
 4-Bromophenyl-phenylether
 Concen: 3.351 ng
 RT: 10.68 min Scan# 1461
 Delta R.T. -0.25 min
 Lab File: BF100915.D
 Acq: 28 Nov 2017 2:24

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:248 Resp: 6409
 Ion Ratio Lower Upper
 248 100
 250 177.7 76.9 115.3#
 141 447.5 74.4 111.6#

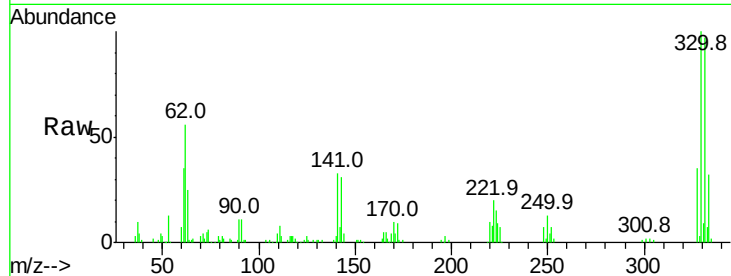


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E


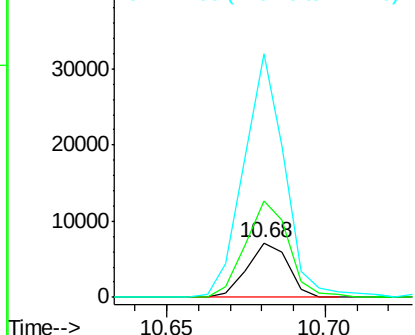



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.02 min Scan# 2028
 Delta R.T. -0.01 min
 Lab File: BF100915.D
 Acq: 28 Nov 2017 2:24

Tgt Ion:240 Resp: 124335
 Ion Ratio Lower Upper
 240 100
 120 11.8 9.5 14.3
 236 24.7 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

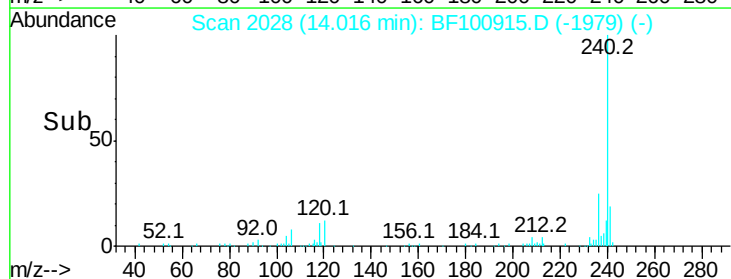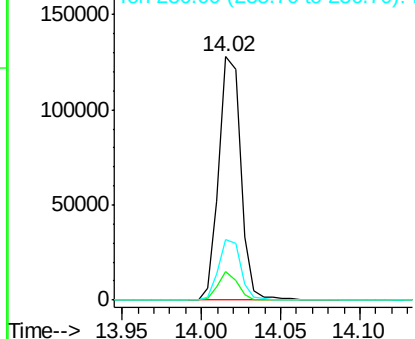







#78
 Terphenyl-d14
 Concen: 105.093 ng
 RT: 12.97 min Scan# 1850
 Delta R.T. 0.00 min
 Lab File: BF100915.D
 Acq: 28 Nov 2017 2:24

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
244	100		
212	7.0	5.4	8.0
122	9.8	11.0	16.4

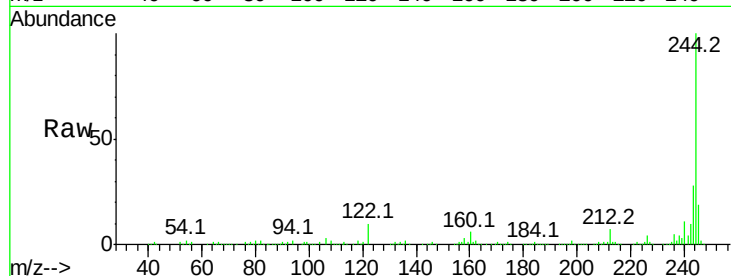


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

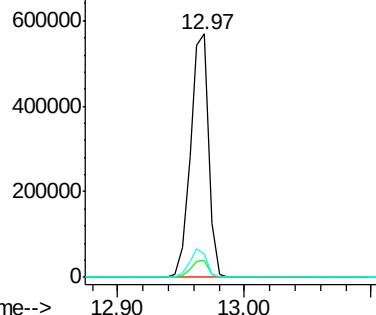

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.49 min Scan# 2278
 Delta R.T. -0.01 min
 Lab File: BF100915.D
 Acq: 28 Nov 2017 2:24

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.2	28.8
265	21.3	17.5	26.3



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

