
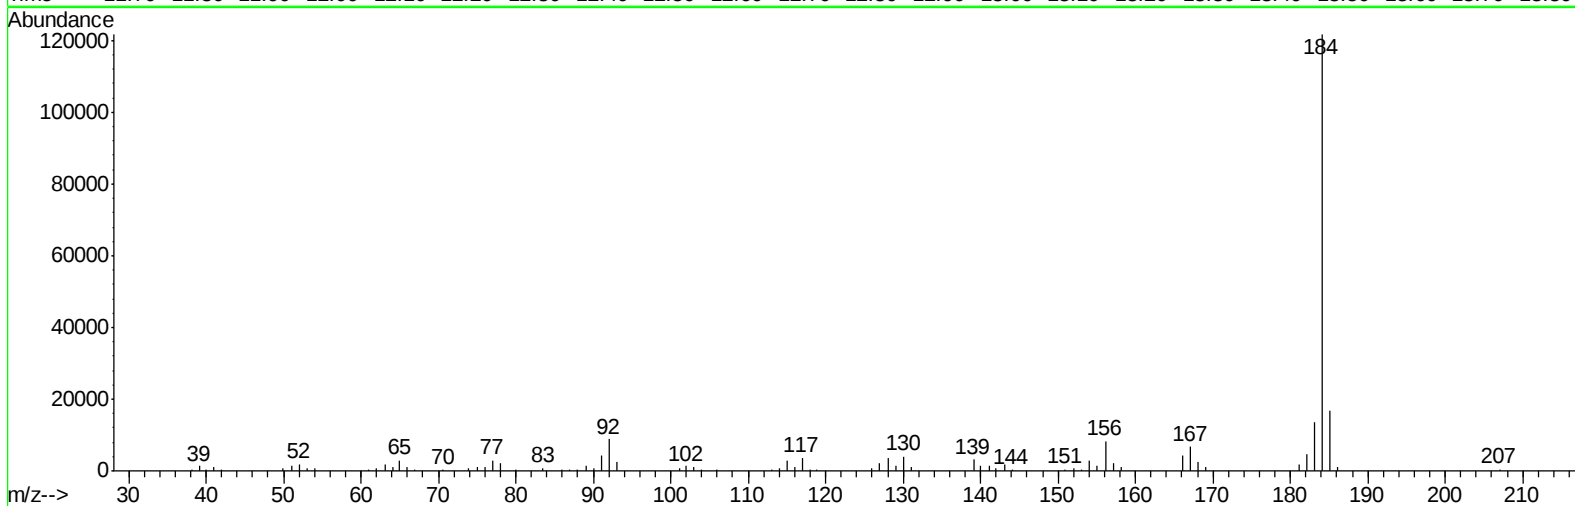


Data Path : Z:\HPCHEM1\BNA F\Data\BF112717\
Data File : BF100905.D
Acq On : 27 Nov 2017 21:34
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 08:22:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 14:11:25 2017
Response via : Initial Calibration

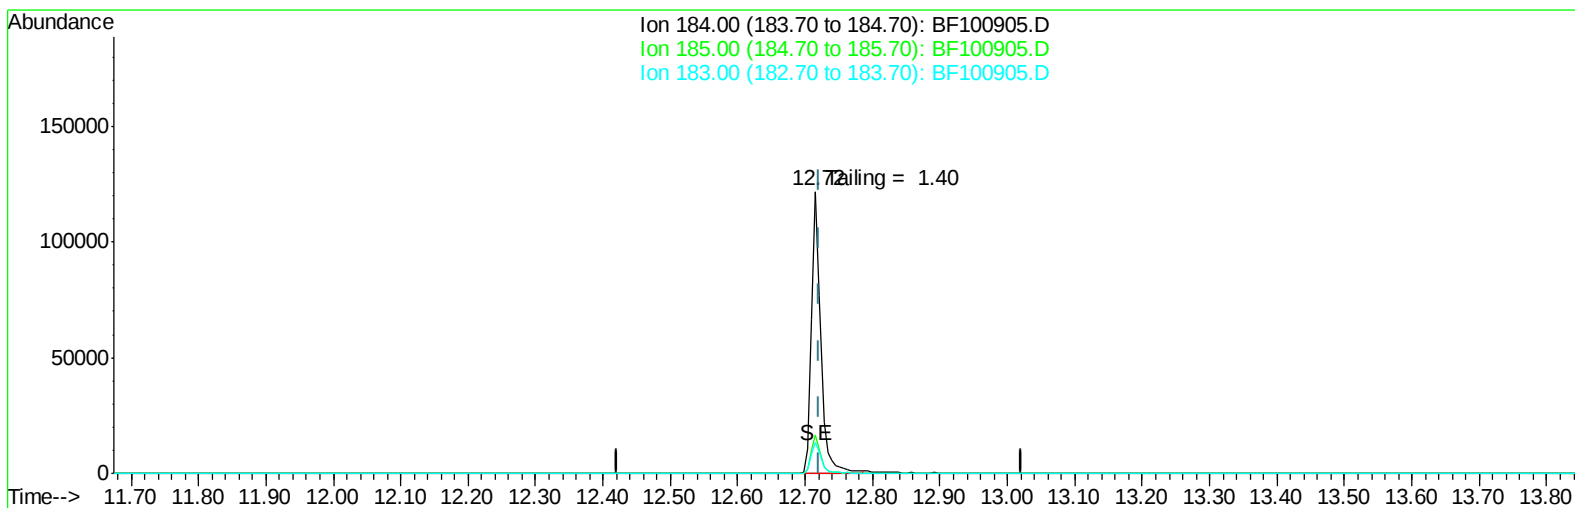

TIC: BF100905.D

(76) Benzidine


12.715min (-0.006) 0.00ng

response 117477

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.65
183.00	11.60	11.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF112717\
Data File : BF100905.D
Acq On : 27 Nov 2017 21:34
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 08:22:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 27 14:11:25 2017
Response via : Initial Calibration

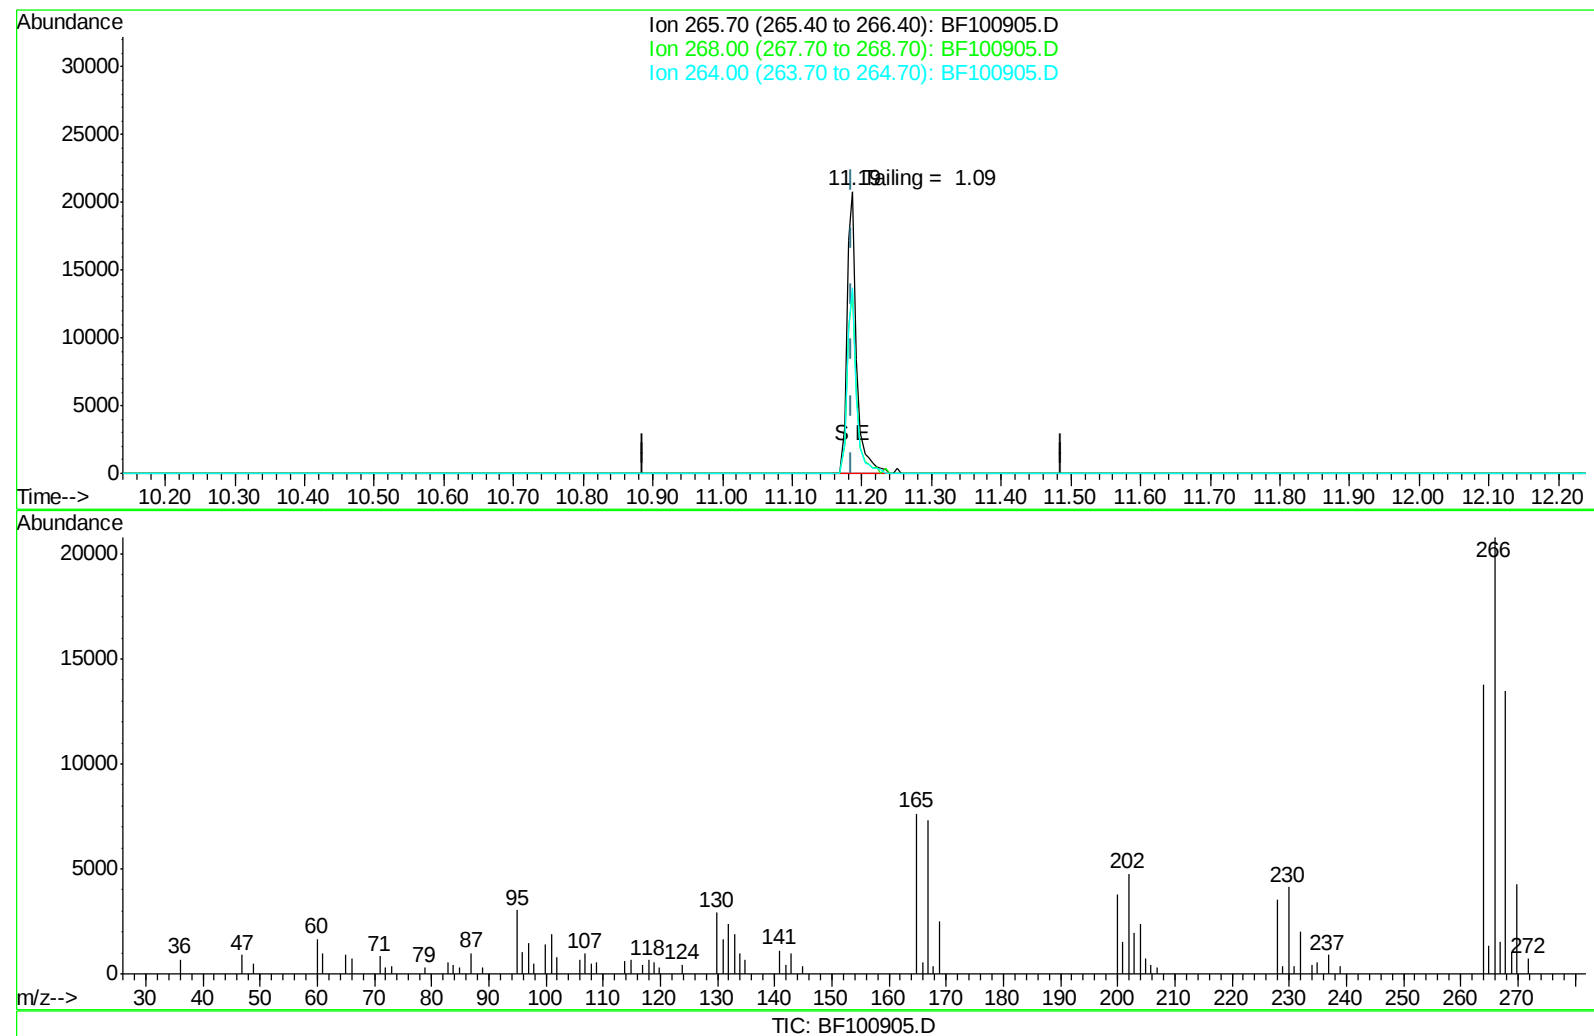

(69) Pentachlorophenol (C)

11.186min (-0.000) 0.00ng

response 20209

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.74
264.00	61.90	66.14
0.00	0.00	0.00