

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112717\
 Data File : BF100912.D
 Acq On : 28 Nov 2017 1:05
 Operator : SJ/JU
 Sample : I6584-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 112117-JETT-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.063	504	506	512	rBV	27137	28063	4.35%	0.537%
2	5.469	571	575	583	rBV	144330	133051	20.63%	2.547%
3	6.481	743	747	757	rBB	84473	86700	13.45%	1.660%
4	6.622	768	771	775	rBV	342997	275063	42.66%	5.266%
5	6.857	807	811	814	rBV	450807	356010	55.21%	6.815%
6	7.010	833	837	841	rBV	483754	398146	61.74%	7.622%
7	7.416	902	906	909	rBV	390442	311501	48.31%	5.963%
8	8.139	1024	1029	1032	rBV	544244	462613	71.74%	8.856%
9	9.210	1207	1211	1220	rBV	764111	644831	100.00%	12.344%
10	9.892	1322	1327	1339	rBV	557808	505093	78.33%	9.669%
11	10.680	1458	1461	1468	rBV	244889	210242	32.60%	4.025%
12	11.380	1576	1580	1587	rBV	576072	468064	72.59%	8.960%
13	12.962	1845	1849	1852	rBV	663115	551526	85.53%	10.558%
14	14.021	2025	2029	2032	rBV	408853	357661	55.47%	6.847%
15	14.462	2096	2104	2108	rBV3	9978	23952	3.71%	0.459%
16	14.551	2112	2119	2121	rBV4	5638	13651	2.12%	0.261%
17	14.780	2149	2158	2163	rBV6	10742	25604	3.97%	0.490%
18	15.492	2274	2279	2289	rVB	259687	334025	51.80%	6.394%
19	15.927	2349	2353	2360	rVB4	6849	13484	2.09%	0.258%
20	16.439	2433	2440	2445	rBV4	6920	14399	2.23%	0.276%
21	17.027	2534	2540	2545	rBV6	4856	10018	1.55%	0.192%


Sum of corrected areas: 5223697

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112717\
Data File : BF100912.D
Acq On : 28 Nov 2017 1:05
Operator : SJ/JU
Sample : I6584-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112117-JETT-F-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

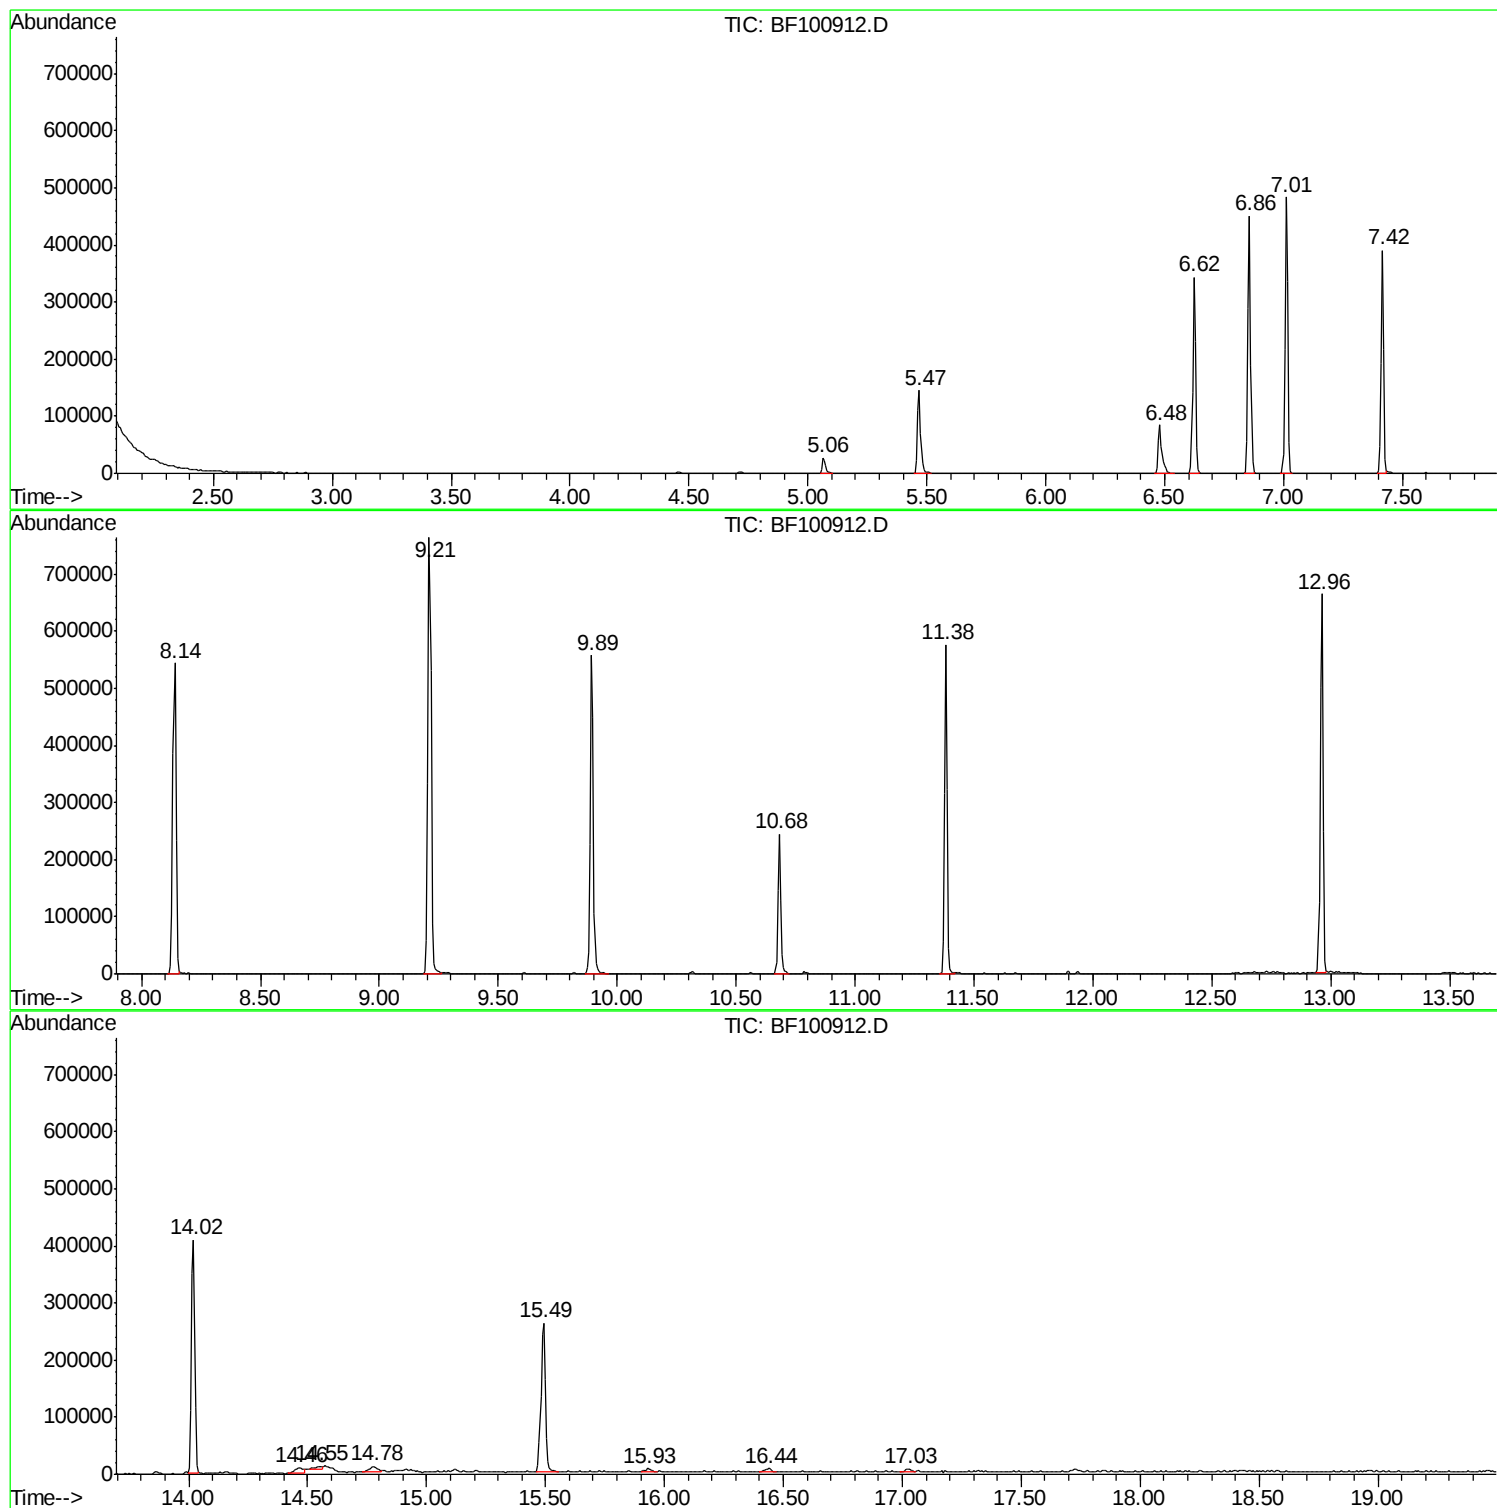

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF112717\
Data_File : BF100912.D
Acq_On : 28-Nov-2017 1:055
Operator : SJ/JUU
Sample : I6584-011
Misc :
ALS_Vial : 32 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
112117-JETT-F-D-B

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
