


Data Path : Z:\HPCHEM1\BNA F\DATA\BF112717\  
 Data File : BF100879.D  
 Acq On : 27 Nov 2017 9:10  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Nov 27 14:11:25 2017

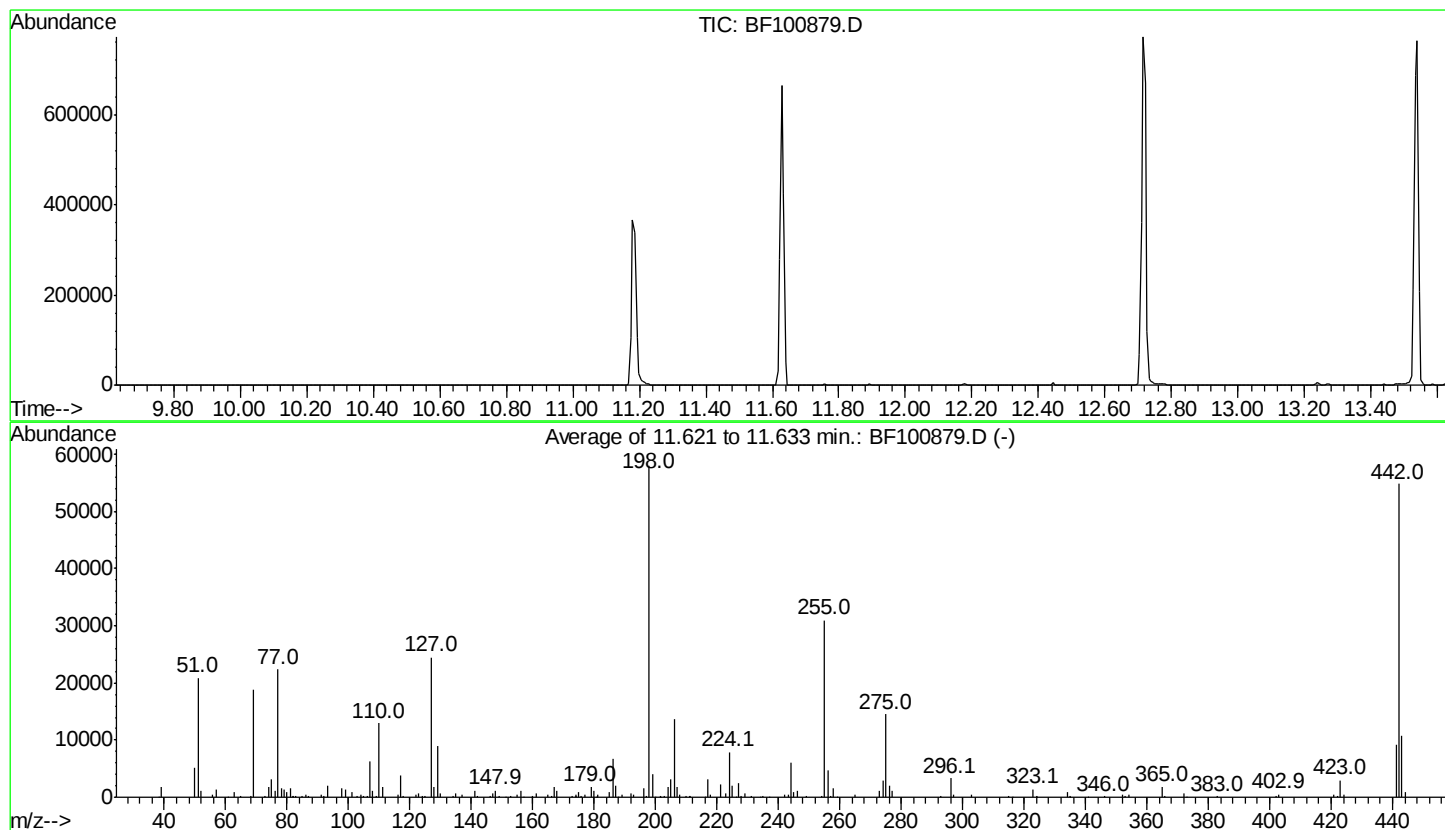

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 35.9      | 20847   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 314     | PASS             |
| 69          | 198          | 0.00         | 100          | 32.5      | 18833   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 42.2      | 24488   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.3       | 155     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 58024   | PASS             |
| 199         | 198          | 5            | 9            | 7.0       | 4033    | PASS             |
| 275         | 198          | 10           | 60           | 25.0      | 14524   | PASS             |
| 365         | 198          | 1            | 100          | 3.2       | 1867    | PASS             |
| 441         | 443          | 0.01         | 100          | 84.8      | 9170    | PASS             |
| 442         | 198          | 50           | 100          | 94.4      | 54776   | PASS             |
| 443         | 442          | 15           | 24           | 19.7      | 10813   | PASS             |