


Data Path : Z:\HPCHEM1\BNA F\DATA\BF112717\
 Data File : BF100905.D
 Acq On : 27 Nov 2017 21:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 27 14:11:25 2017

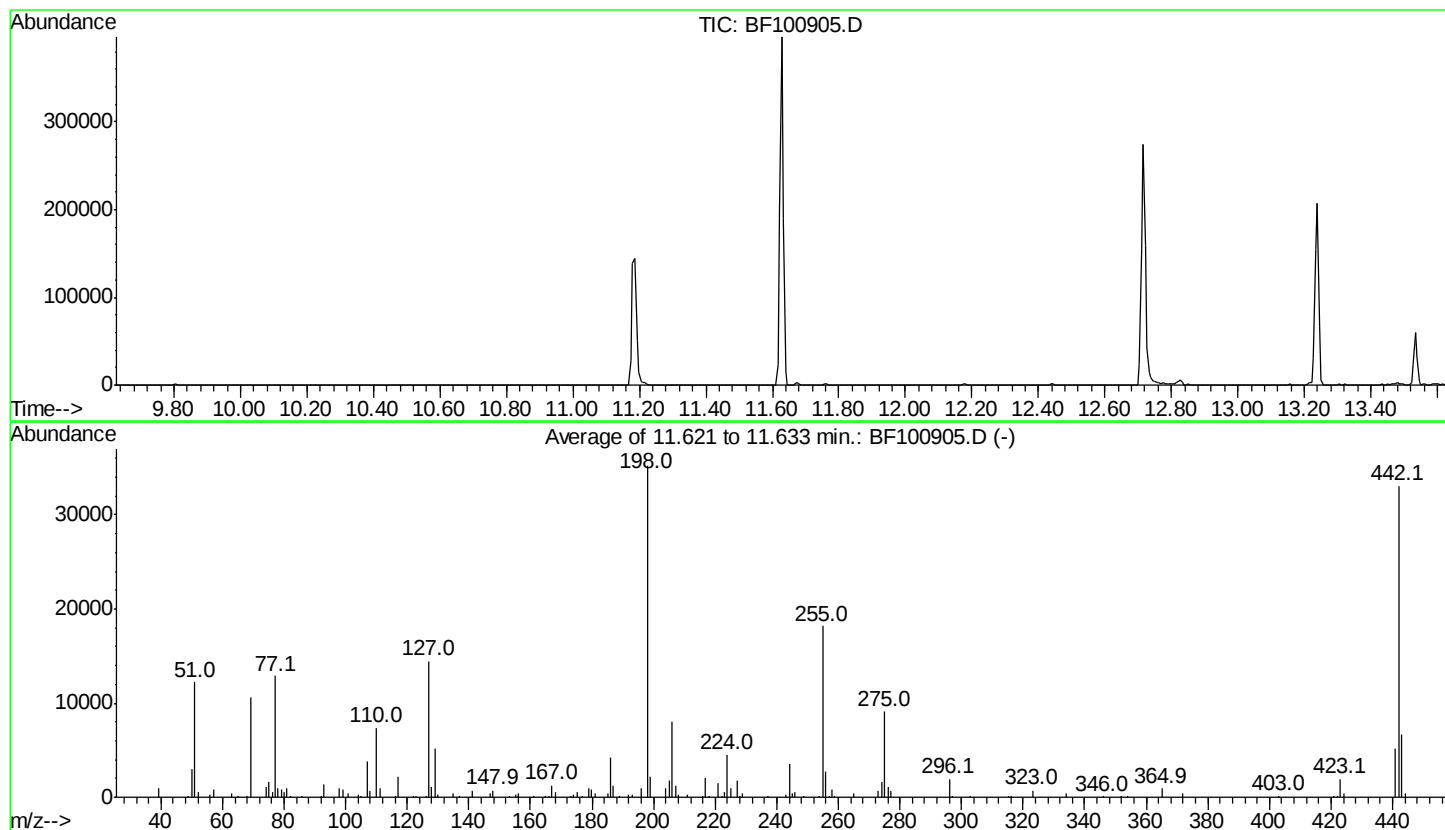

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	12182	PASS
68	69	0.00	2	1.2	127	PASS
69	198	0.00	100	30.3	10664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.1	14476	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35232	PASS
199	198	5	9	6.0	2130	PASS
275	198	10	60	25.8	9076	PASS
365	198	1	100	2.7	946	PASS
441	443	0.01	100	77.7	5168	PASS
442	198	50	100	94.0	33118	PASS
443	442	15	24	20.1	6654	PASS