
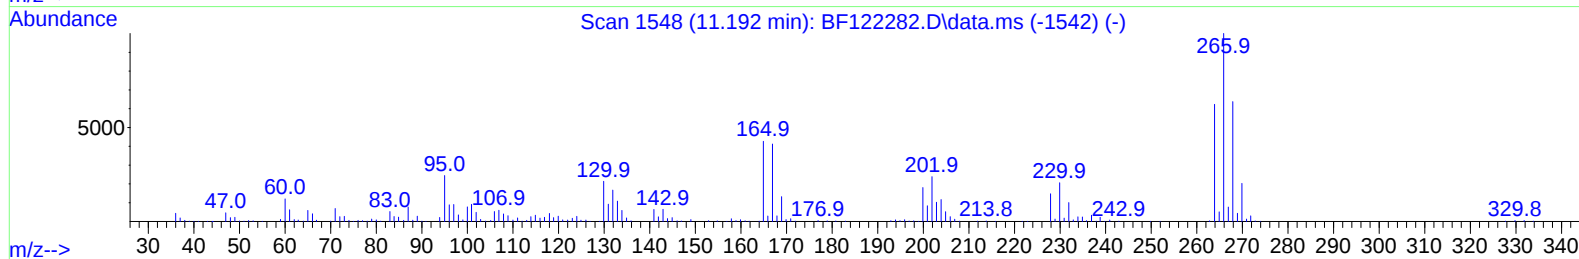
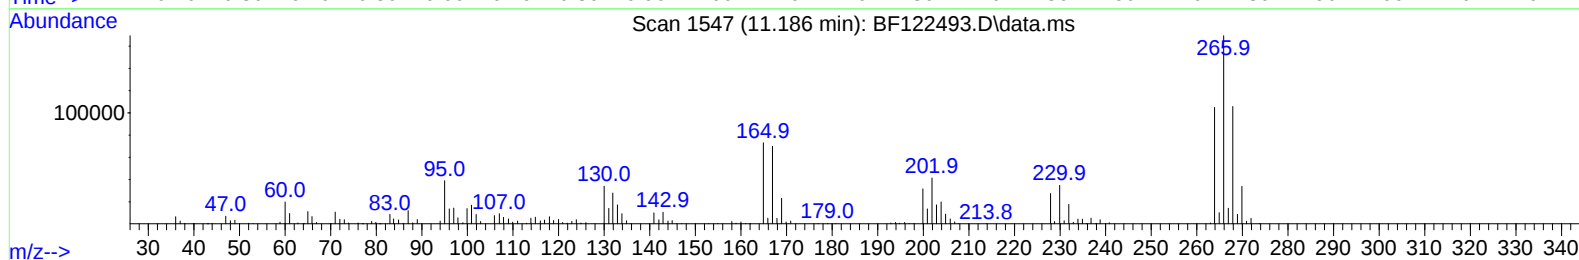


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112720\
Data File : BF122493.D
Acq On : 27 Nov 2020 9:47
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 23:53:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 14:38:56 2020
Response via : Initial Calibration

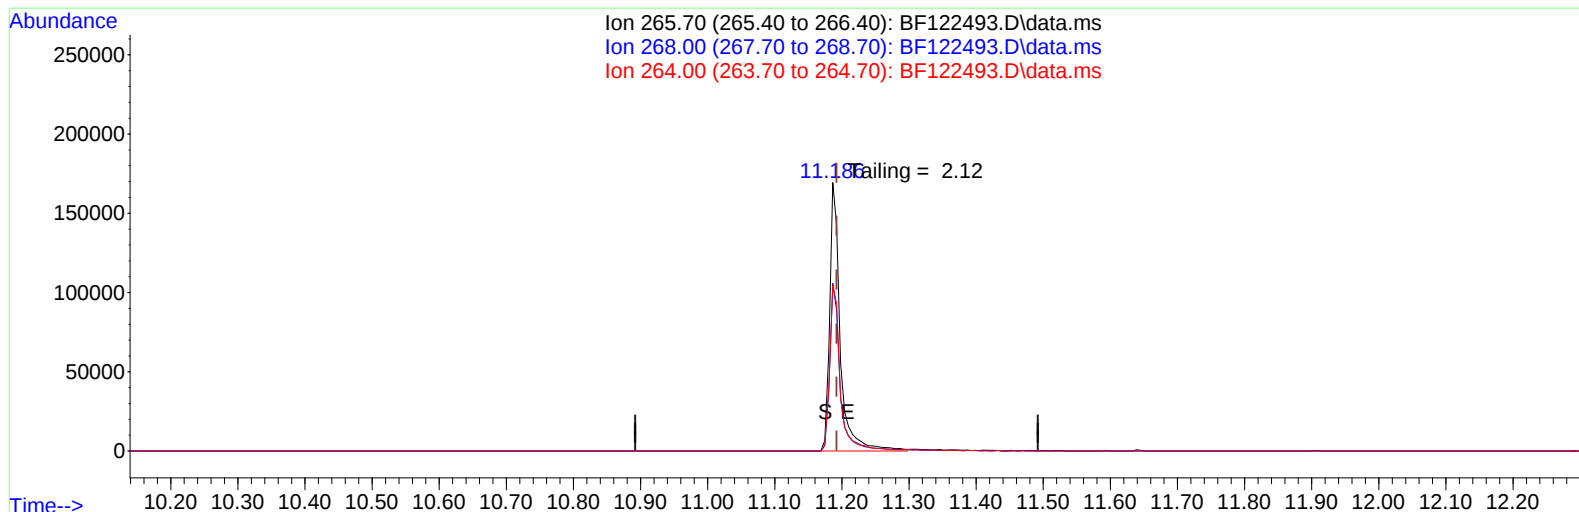

TIC: BF122493.D\data.ms

(70) Pentachlorophenol (C)




11.186min (-0.006) 38706.06 ng

response 186862

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	62.45
264.00	62.40	61.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112720\
Data File : BF122493.D
Acq On : 27 Nov 2020 9:47
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 23:53:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 14:38:56 2020
Response via : Initial Calibration

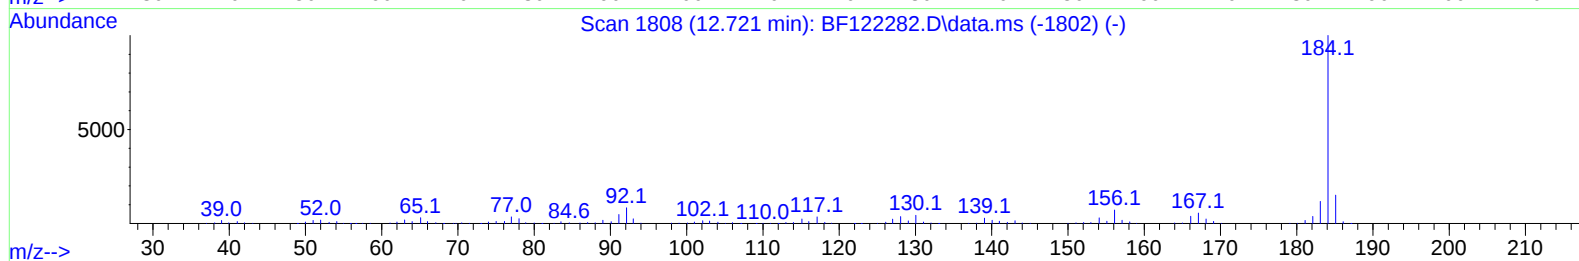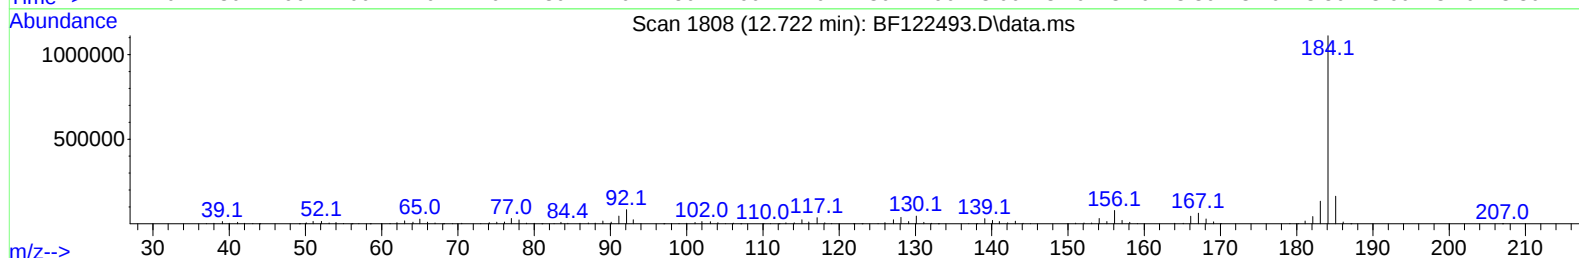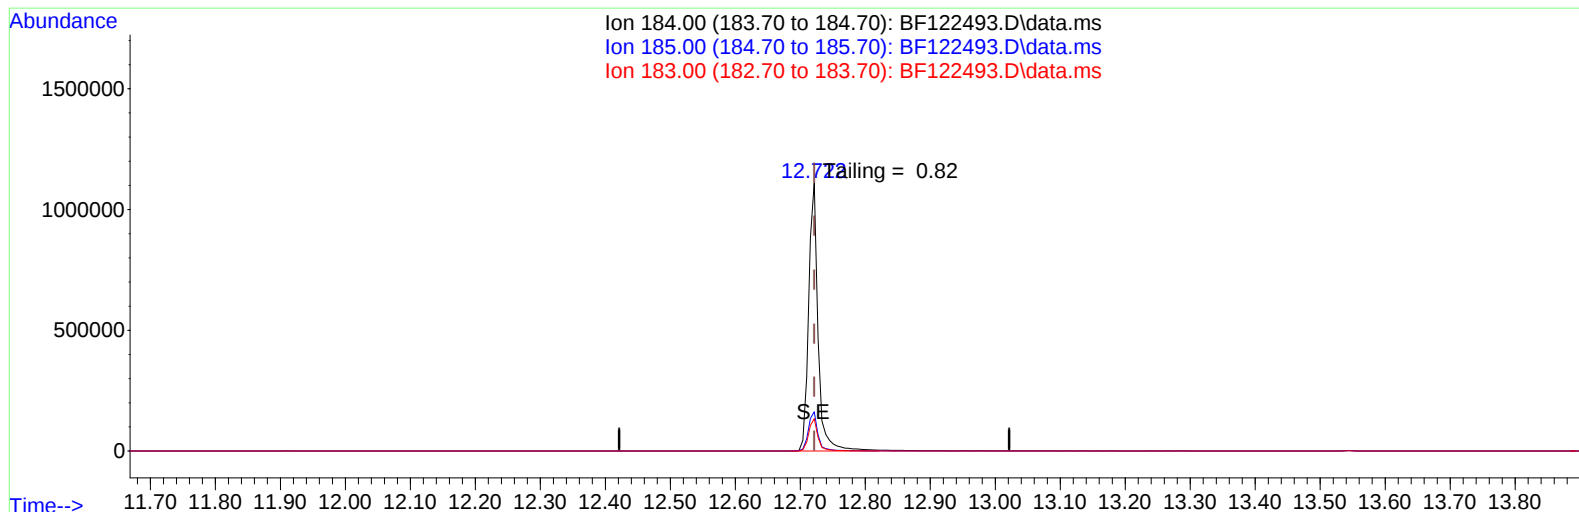

TIC: BF122493.D\data.ms

(77) Benzidine

12.722min (-0.000) 185547.12 ng

response 1137340

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.63
183.00	11.70	12.05
0.00	0.00	0.00