

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112720\
 Data File : BF122495.D
 Acq On : 27 Nov 2020 11:06
 Operator : JU/CG
 Sample : PB133227BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB133227BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.210	17	21	33	rVB	62782	95101	1.11%	0.200%
2	5.087	504	510	518	rBV	88595	106770	1.24%	0.225%
3	5.487	573	578	581	rBV	4083541	3783964	44.00%	7.970%
4	6.486	743	748	751	rBV	3619803	3829052	44.52%	8.065%
5	6.857	807	811	814	rBV	1469160	1273591	14.81%	2.682%
6	7.016	833	838	841	rBV	5420333	5183341	60.27%	10.917%
7	7.422	900	907	910	rBV	3820057	4209757	48.95%	8.867%
8	8.139	1024	1029	1049	rBV	1758161	1640323	19.07%	3.455%
9	9.222	1206	1213	1216	rBV	6521630	7521587	87.45%	15.842%
10	9.898	1322	1328	1343	rBV	1905969	1900744	22.10%	4.003%
11	10.686	1456	1462	1479	rBV	2778239	2946225	34.26%	6.205%
12	11.380	1575	1580	1588	rBV	1934402	1972894	22.94%	4.155%
13	12.974	1844	1851	1854	rBV	7332610	8600536	100.00%	18.115%
14	14.021	2025	2029	2043	rVB	2162849	2138376	24.86%	4.504%
15	15.492	2273	2279	2295	rBV	1446490	2129955	24.77%	4.486%
16	16.939	2514	2525	2532	rBV4	36594	146179	1.70%	0.308%




Sum of corrected areas: 47478395

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112720\
Data File : BF122495.D
Acq On : 27 Nov 2020 11:06
Operator : JU/CG
Sample : PB133227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133227BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

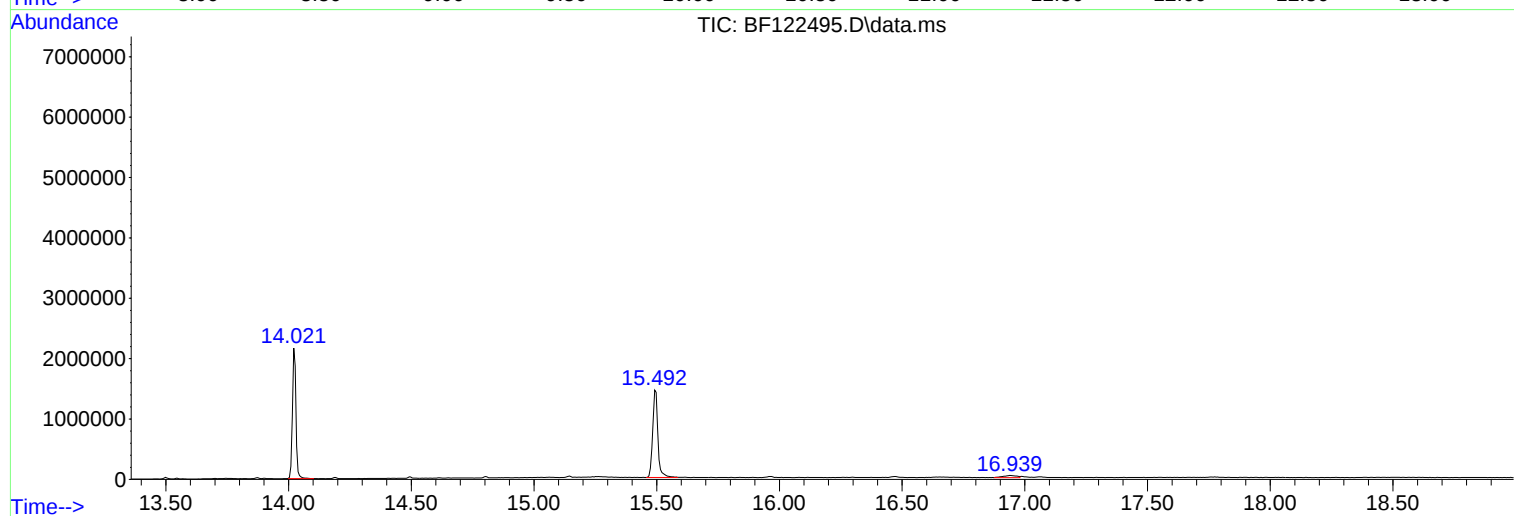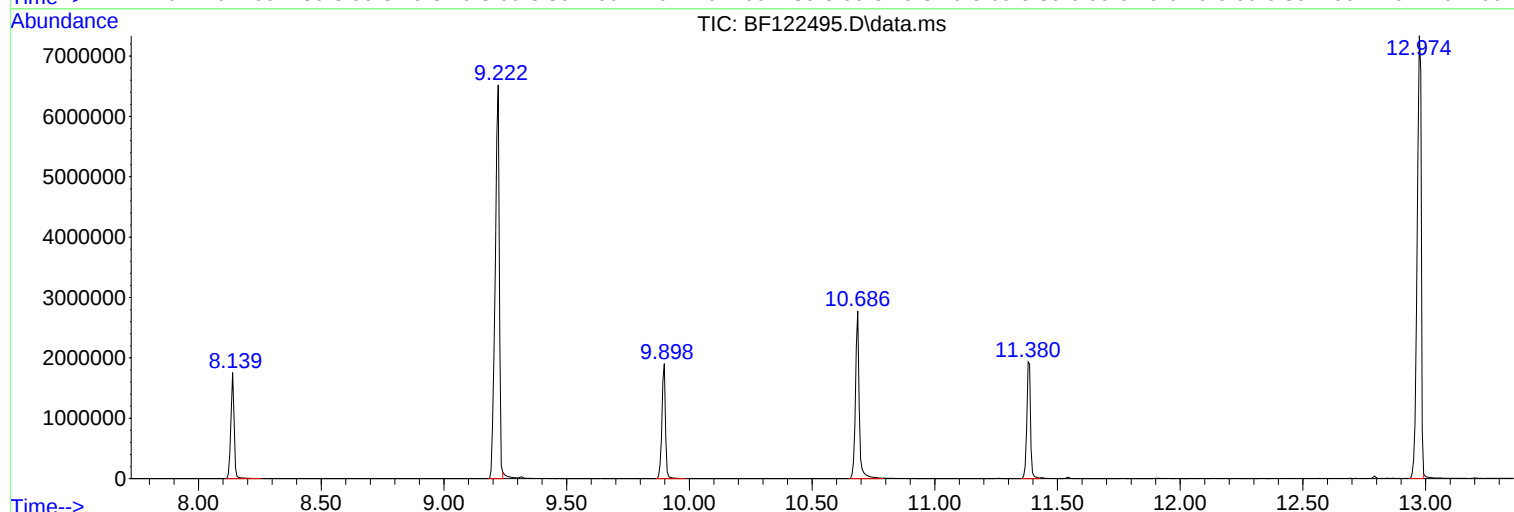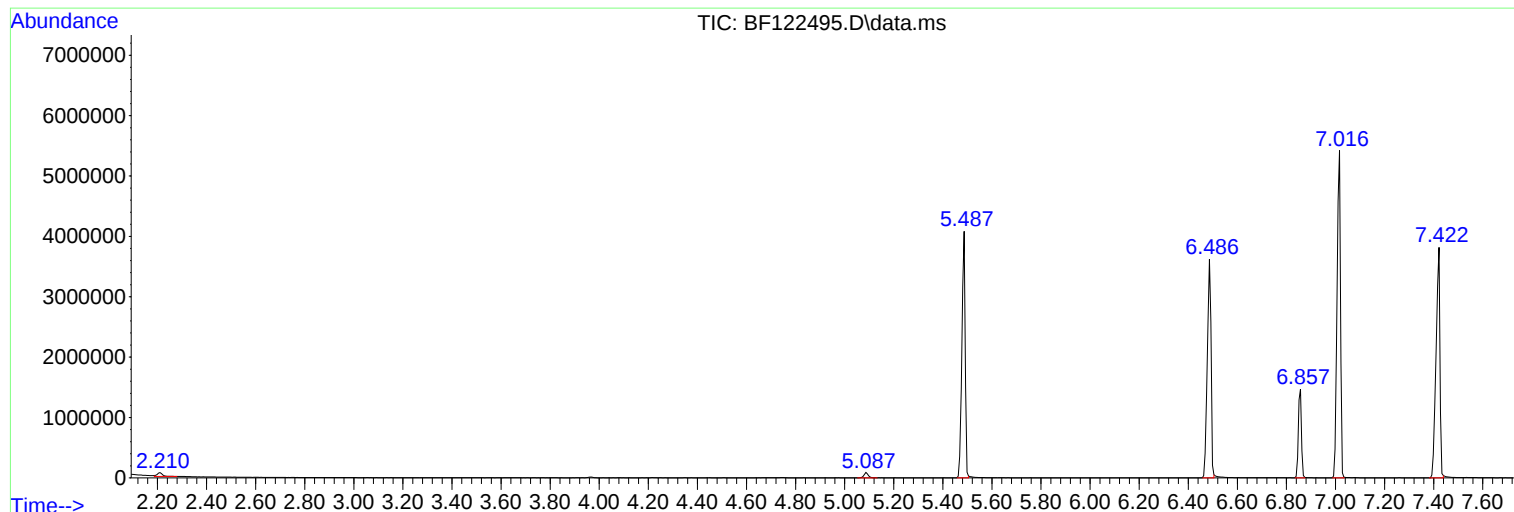

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112720\
Data File : BF122495.D
Acq On : 27 Nov 2020 11:06
Operator : JU/CG
Sample : PB133227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133227BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112720\
Data File : BF122495.D
Acq On : 27 Nov 2020 11:06
Operator : JU/CG
Sample : PB133227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133227BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------