


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112720\
 Data File : BF122493.D
 Acq On : 27 Nov 2020 9:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 24 14:38:56 2020

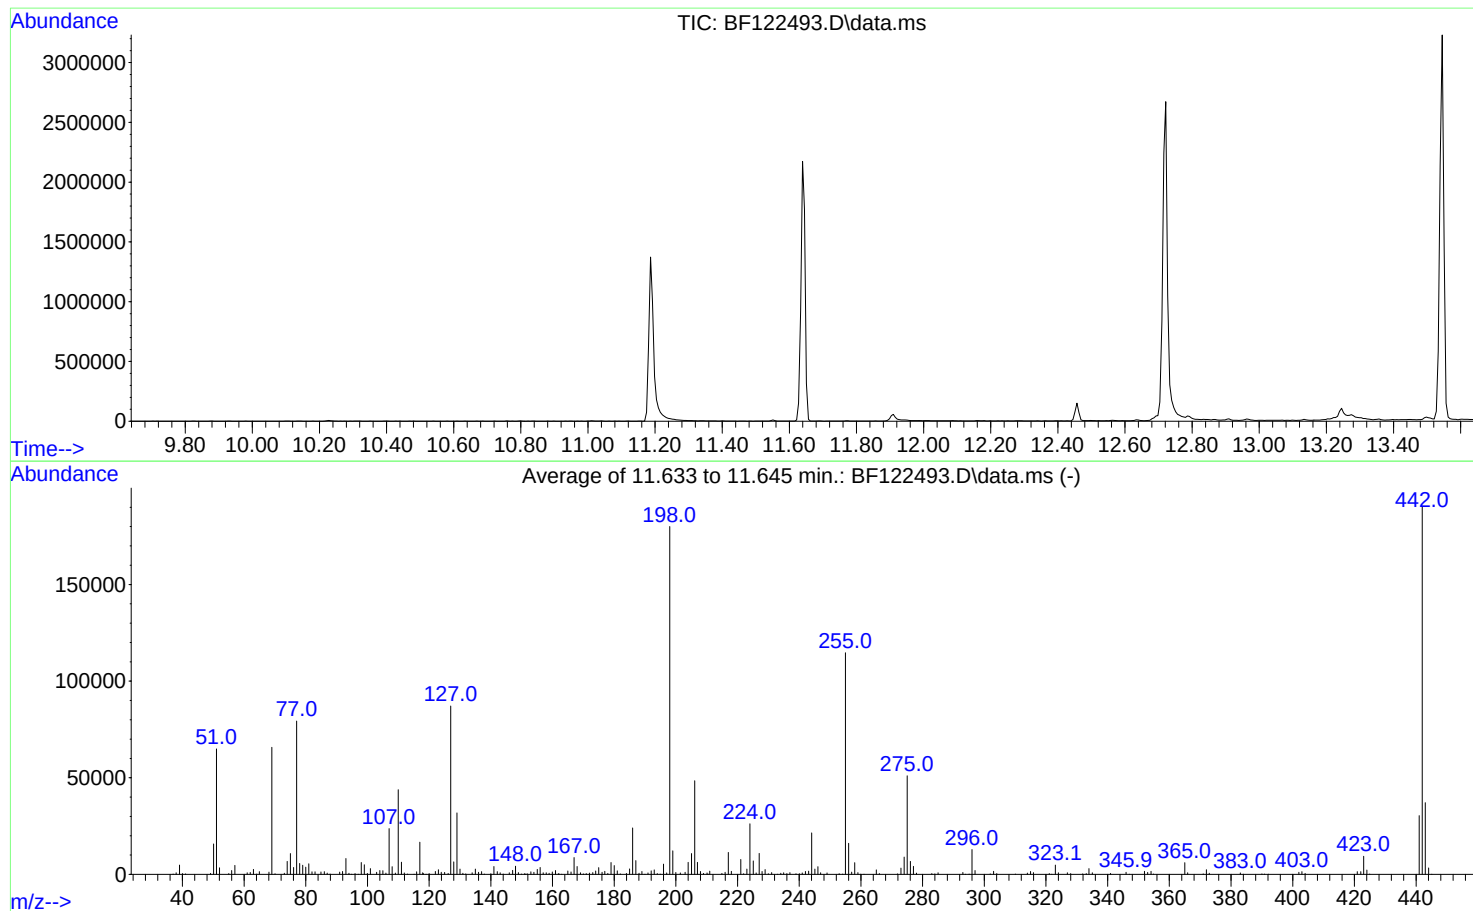

Spectrum Information: Average of 11.633 to 11.645 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	64917	PASS
68	69	0.00	2	1.7	1138	PASS
69	198	0.00	100	36.5	65736	PASS
70	69	0.00	2	0.5	304	PASS
127	198	10	80	48.4	87136	PASS
197	198	0.00	2	0.4	735	PASS
198	198	100	100	100.0	180072	PASS
199	198	5	9	6.7	12144	PASS
275	198	10	60	28.3	51037	PASS
365	198	1	100	3.4	6090	PASS
441	198	0.01	100	16.9	30373	PASS
442	442	100	100	100.0	190397	PASS
443	442	15	24	19.5	37125	PASS