


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112816\
 Data File : BF091311.D
 Acq On : 28 Nov 2016 12:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 23 13:22:53 2016

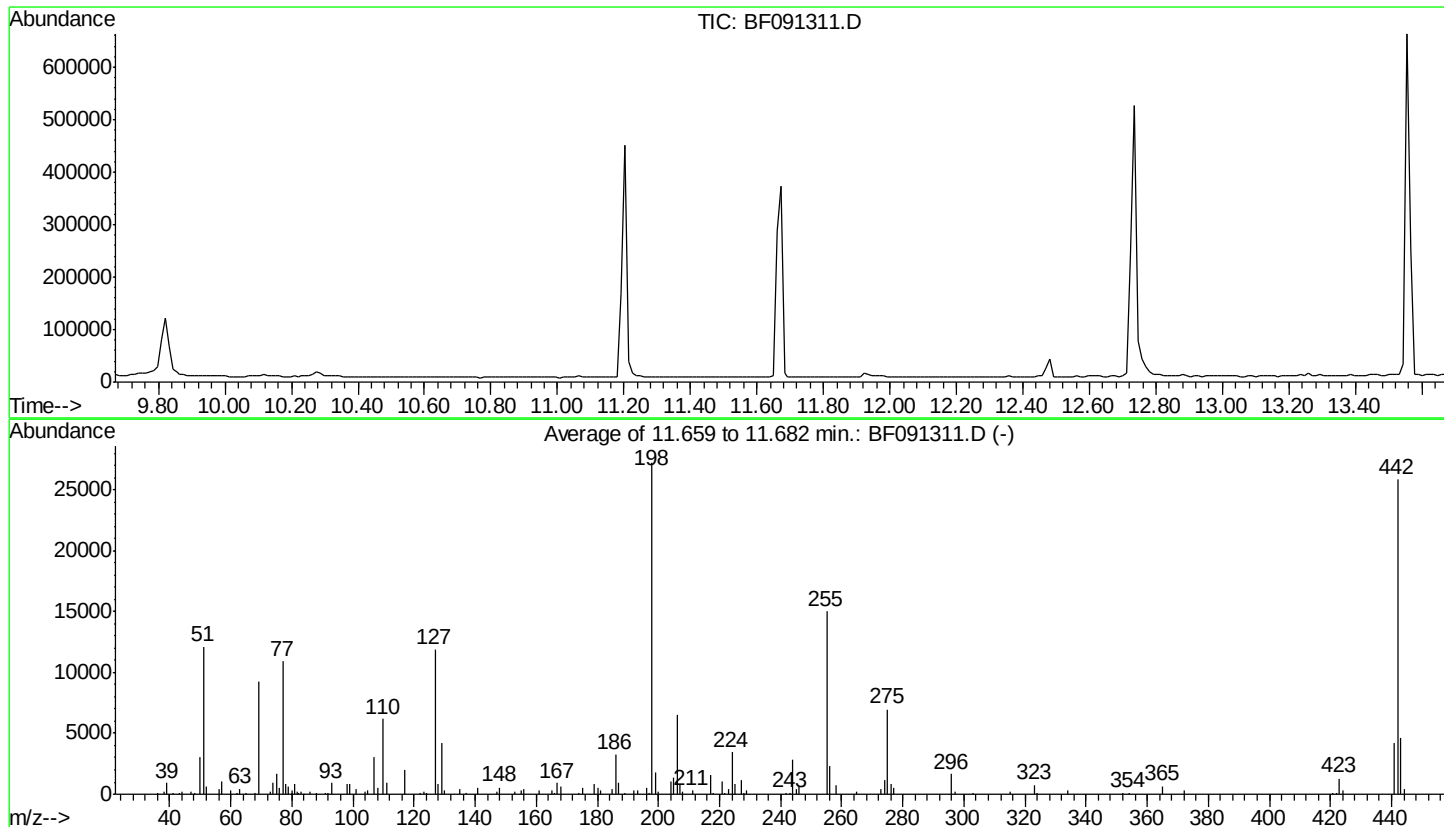

AutoFind: Scans 820, 821, 822; Background Corrected with Scan 816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	12112	PASS
68	69	0.00	2	1.3	123	PASS
69	198	0.00	100	33.9	9219	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.5	11832	PASS
197	198	0.00	2	0.5	142	PASS
198	198	100	100	100.0	27218	PASS
199	198	5	9	6.7	1836	PASS
275	198	10	60	25.5	6947	PASS
365	198	1	100	2.5	672	PASS
441	442	0.01	24	16.3	4200	PASS
442	198	50	100	94.9	25835	PASS
443	442	15	24	18.0	4657	PASS