
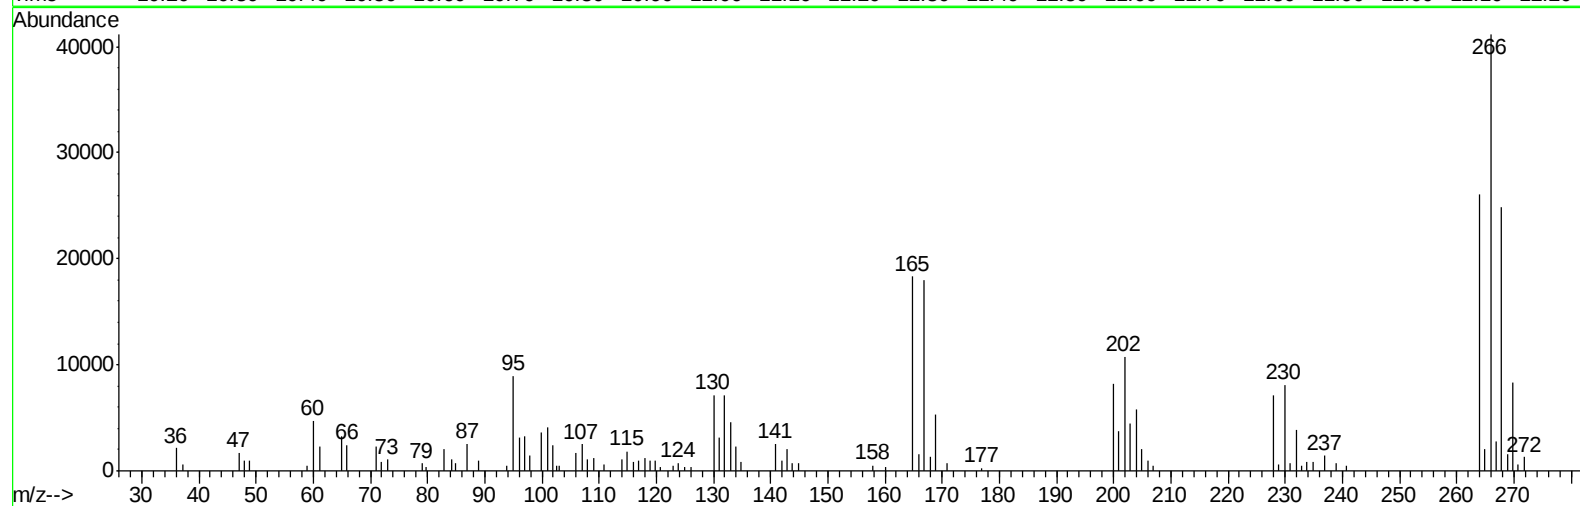


Data Path : Z:\HPCHEM1\BNA F\Data\BF112817\
Data File : BF100922.D
Acq On : 28 Nov 2017 9:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 08:16:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 15:21:02 2017
Response via : Initial Calibration

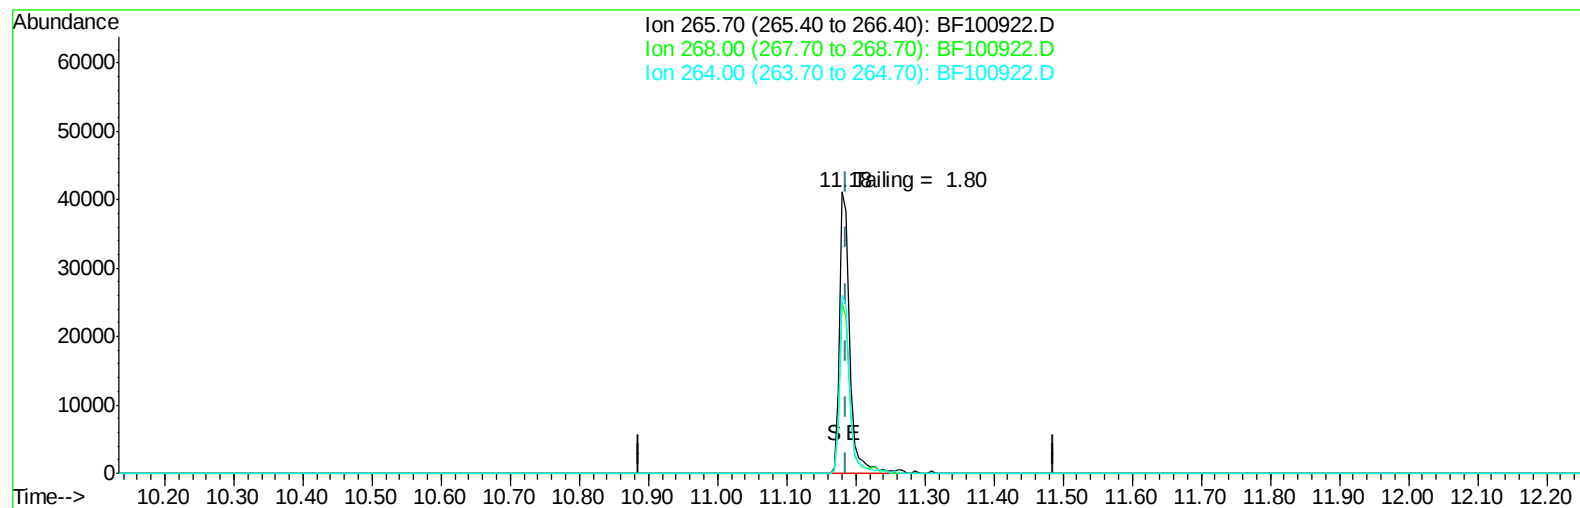

TIC: BF100922.D

(69) Pentachlorophenol (C)



11.180min (-0.006) 38632.42ng

response 41618

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.36
264.00	61.90	63.28
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF112817\
Data File : BF100922.D
Acq On : 28 Nov 2017 9:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 08:16:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 15:21:02 2017
Response via : Initial Calibration

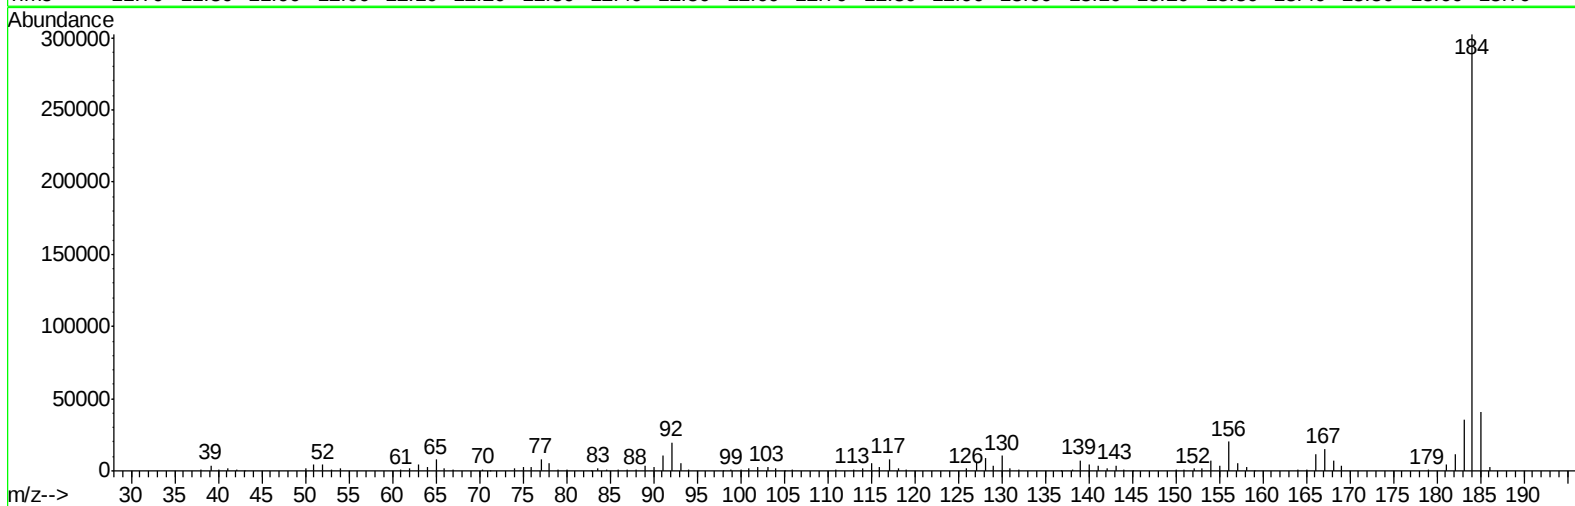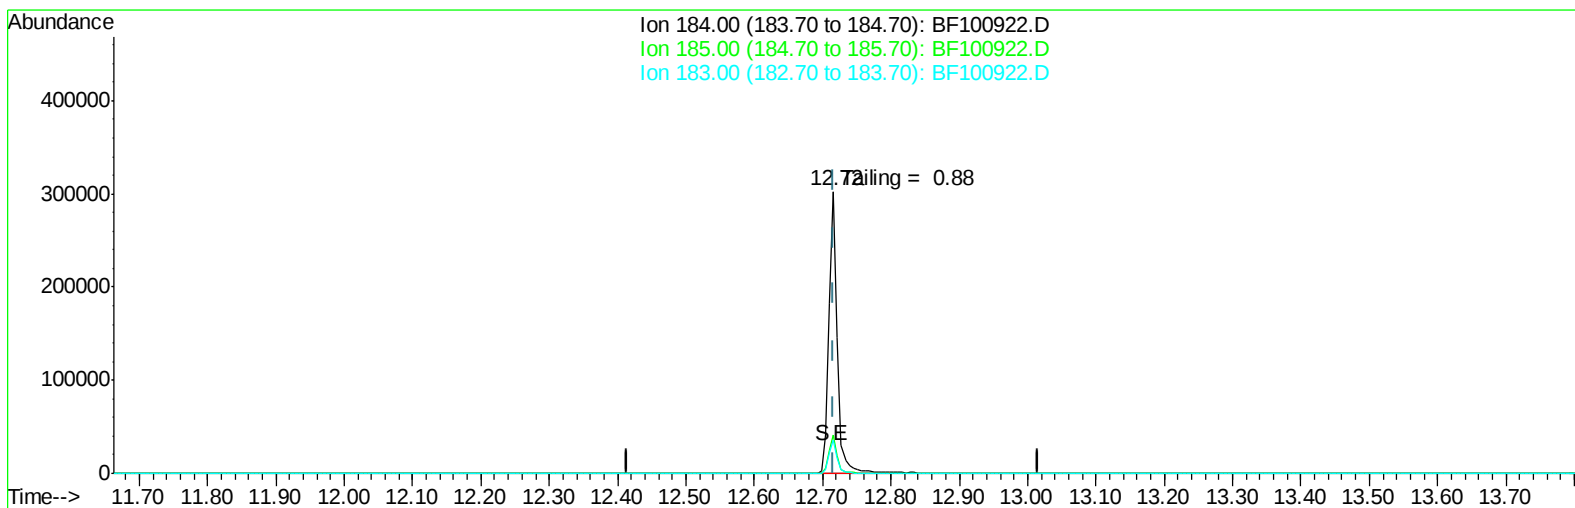

TIC: BF100922.D

(76) Benzidine

12.716min (+0.000) 0.00ng

response 265860

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.57
183.00	11.60	11.80
0.00	0.00	0.00