

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112817\
 Data File : BF100964.D
 Acq On : 29 Nov 2017 5:45
 Operator : SJ/JU
 Sample : I6603-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 112217-JETT-F-D-S

Quant Time: Nov 29 06:36:17 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 28 15:21:02 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	67492	20.00	ng	0.00
21) Naphthalene-d8	8.14	136	250151	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	112031	20.00	ng	0.00
63) Phenanthrene-d10	11.38	188	194020	20.00	ng	0.00
75) Chrysene-d12	14.02	240	139722	20.00	ng	0.00
86) Perylene-d12	15.49	264	124264	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	178215	42.33	ng	0.00
7) Phenol-d6	6.48	99	131711	25.37	ng	-0.01
23) Nitrobenzene-d5	7.43	82	410647	108.53	ng	0.00
41) 2,4,6-Tribromophenol	10.69	330	108784	95.29	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	848169	115.28	ng	0.00
78) Terphenyl-d14	12.97	244	598292	98.39	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112817\
Data File : BF100964.D
Acq On : 29 Nov 2017 5:45
Operator : SJ/JU
Sample : I6603-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112217-JETT-F-D-S

Quant Time: Nov 29 06:36:17 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 15:21:02 2017
Response via : Initial Calibration

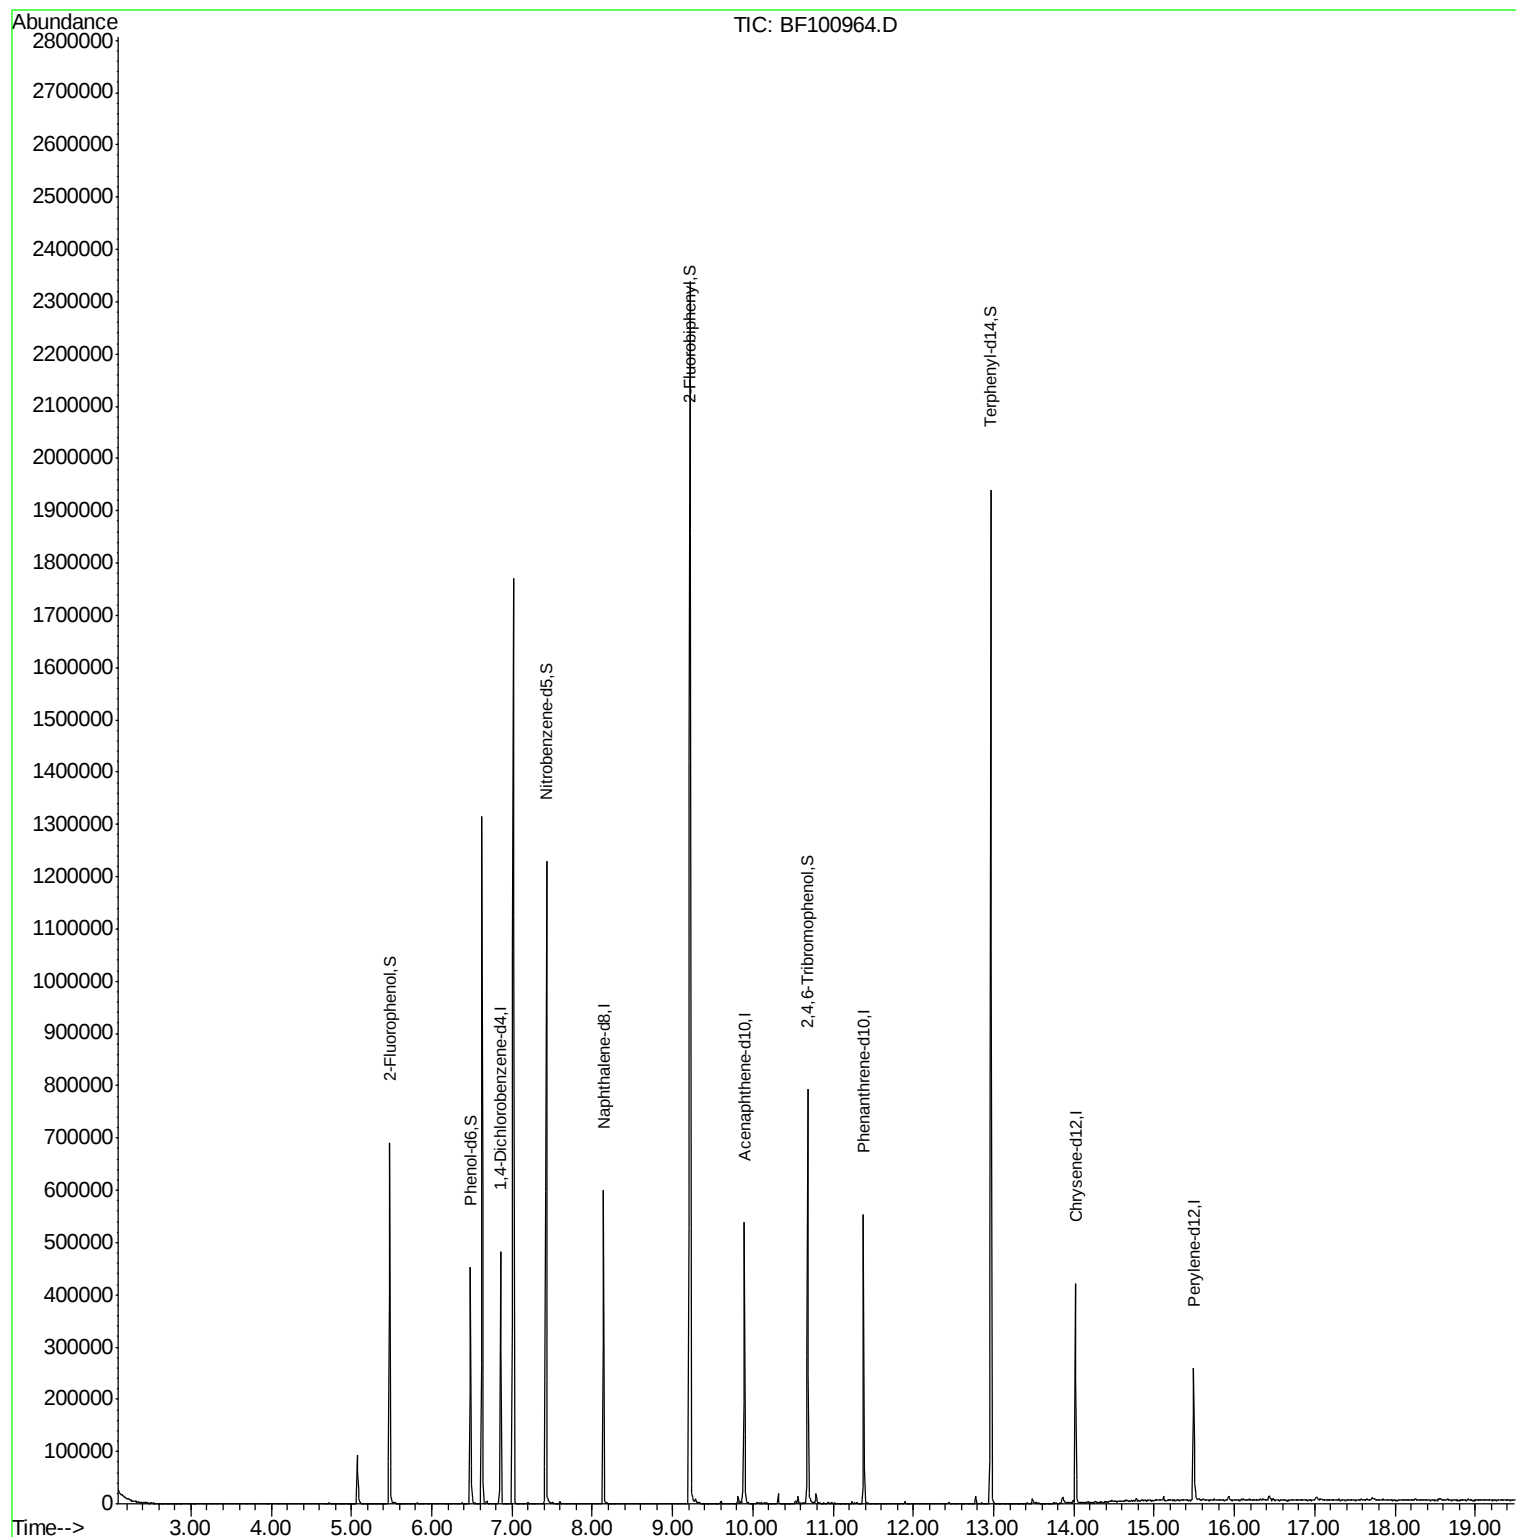

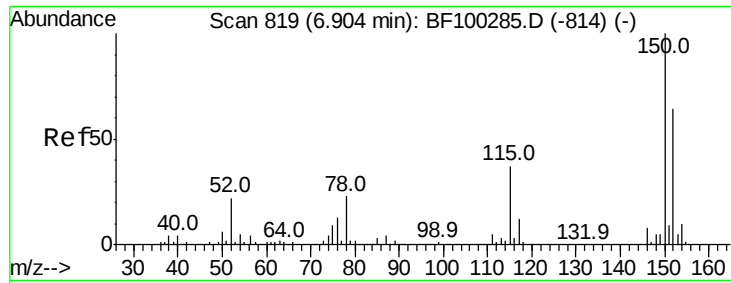


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.86 min Scan# 811
 Delta R.T. -0.00 min
 Lab File: BF100964.D
 Acq: 29 Nov 2017 5:45

Instrument :
 BNA_F
 ClientSampleId :
 112217-JETT-F-D-S

Tot Ion:152 Resp: 67492
 Ion Ratio Lower Upper
 152 100
 150 154.9 124.6 186.8
 115 56.7 50.1 75.1

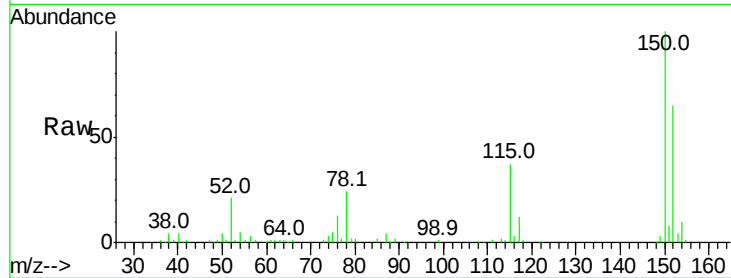


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

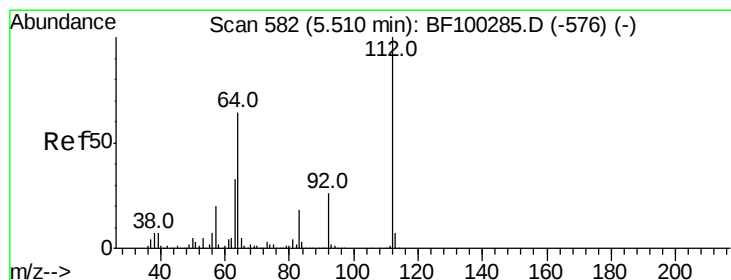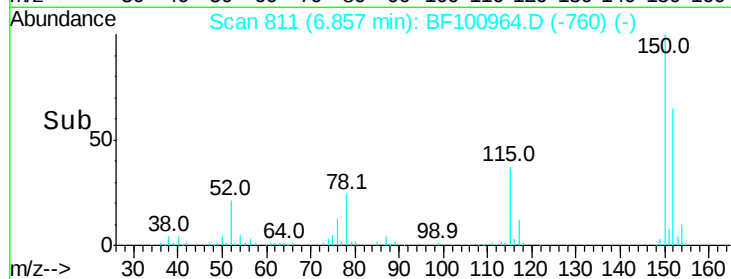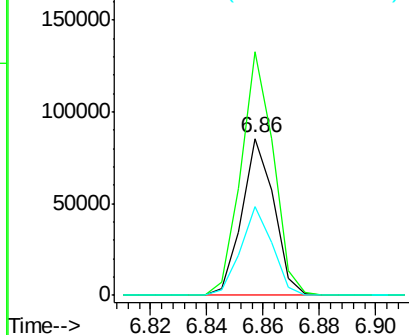



#5

2-Fluorophenol
 Concen: 42.327 ng
 RT: 5.47 min Scan# 576
 Delta R.T. -0.00 min
 Lab File: BF100964.D
 Acq: 29 Nov 2017 5:45

Tgt Ion:112 Resp: 178215
 Ion Ratio Lower Upper
 112 100
 64 59.3 47.9 71.9
 63 31.0 23.7 35.5

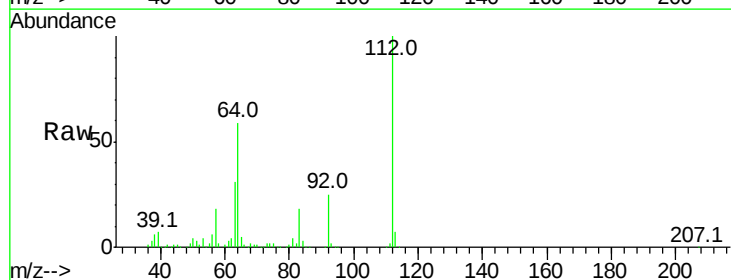

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

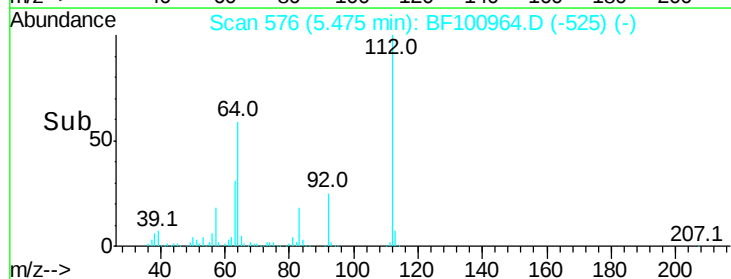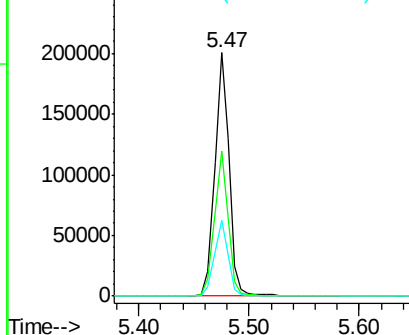



#7

Phenol-d6

Concen: 25.368 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.01 min

Lab File: BF100964.D

Acq: 29 Nov 2017 5:45

Instrument :

BNA_F

ClientSampleId :

112217-JETT-F-D-S





Tot Ion: 99 Resp: 131711

Ion Ratio Lower Upper

99 100

42 19.1 14.5 21.7

71 34.6 25.4 38.0

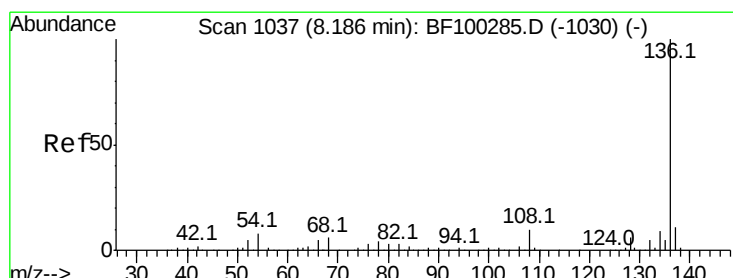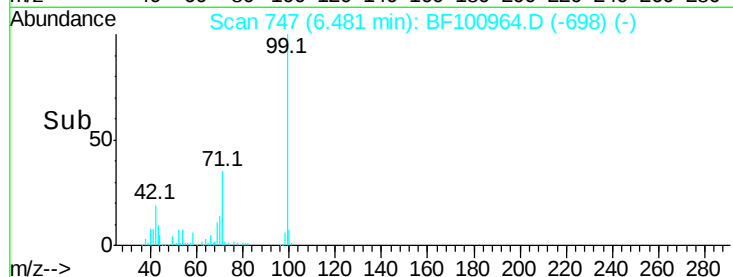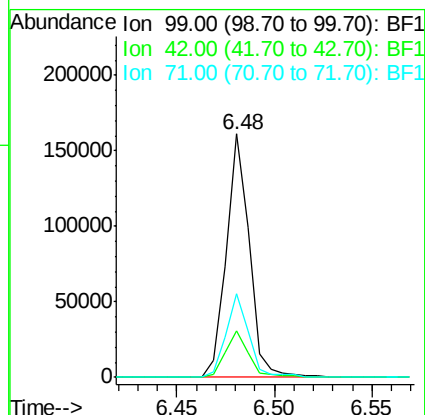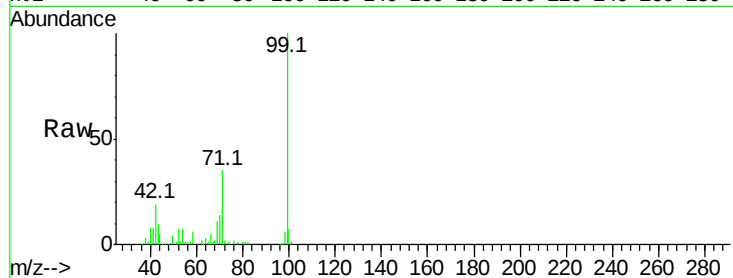

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.14 min Scan# 1029

Delta R.T. -0.00 min

Lab File: BF100964.D

Acq: 29 Nov 2017 5:45

Tgt Ion: 136 Resp: 250151




Ion Ratio Lower Upper

136 100

137 10.8 8.9 13.3

54 7.5 6.6 9.8

68 4.9 5.0 7.4#

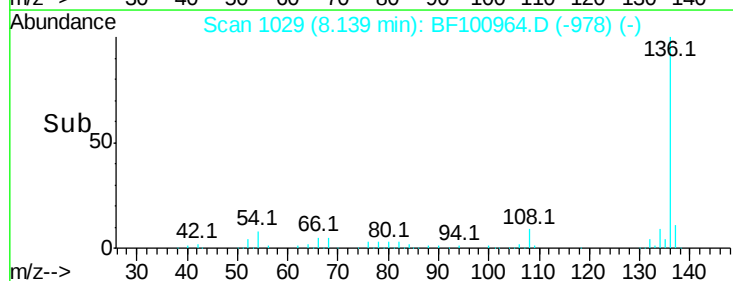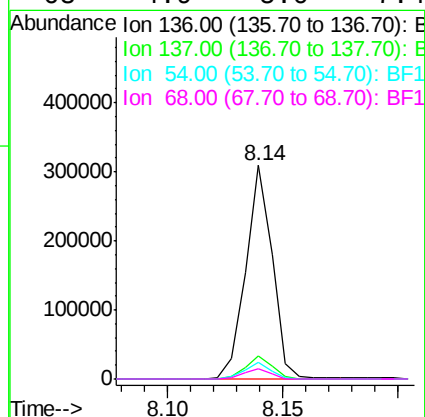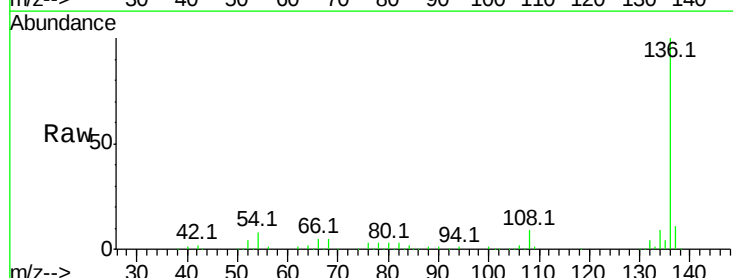



#23

Nitrobenzene-d5

Concen: 108.531 ng

RT: 7.43 min Scan# 908

Delta R.T. -0.00 min

Lab File: BF100964.D

Acq: 29 Nov 2017 5:45

Instrument :

BNA_F

ClientSampleId :

112217-JETT-F-D-S


Tot Ion: 82 Resp: 410647

Ion Ratio Lower Upper

82 100

128 47.6 36.1 54.1




54 52.4 41.4 62.2

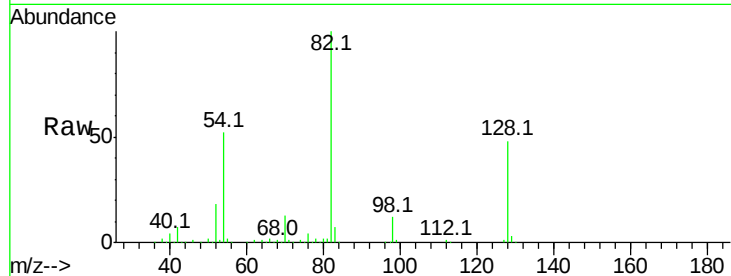

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

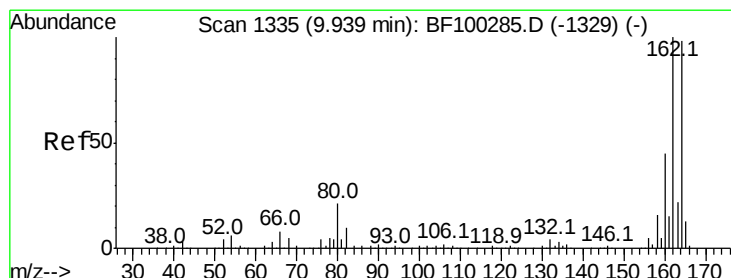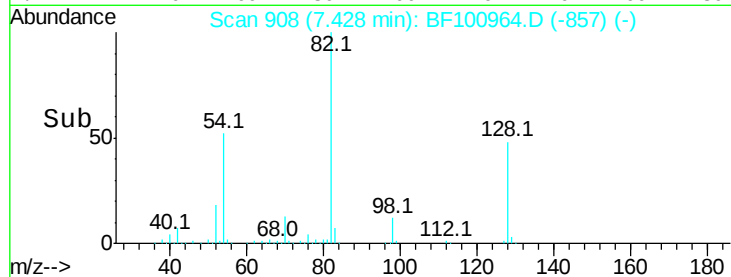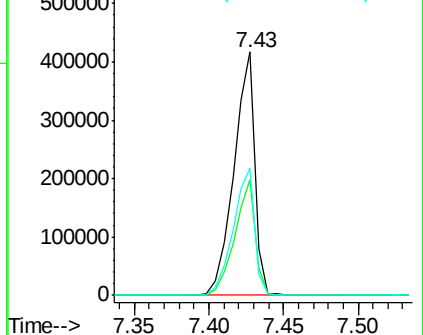

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.89 min Scan# 1327

Delta R.T. -0.01 min

Lab File: BF100964.D

Acq: 29 Nov 2017 5:45


Tgt Ion: 164 Resp: 112031

Ion Ratio Lower Upper

164 100

162 104.0 86.1 129.1



160 45.8 38.3 57.5

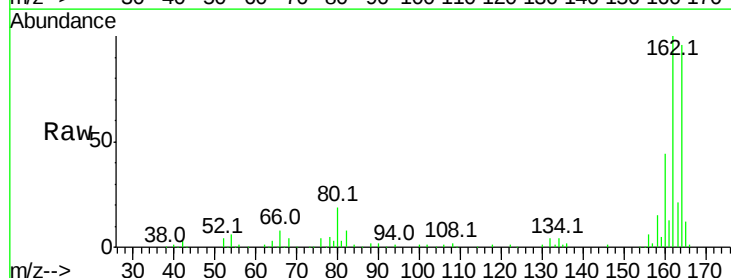

Abundance Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1

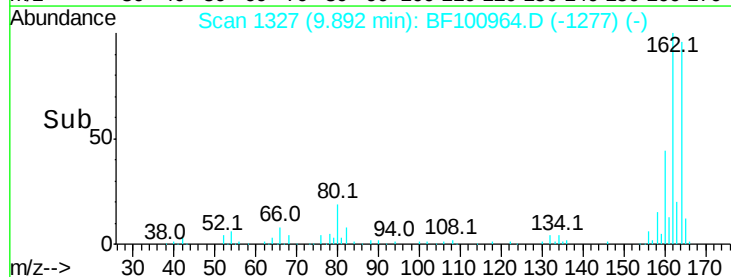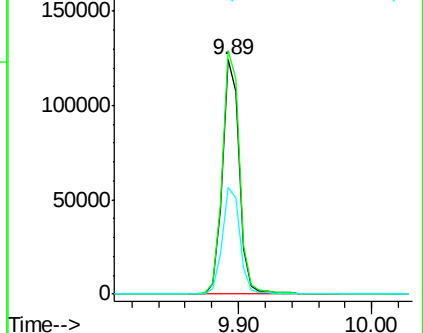







#41
 2,4,6-Tribromophenol
 Concen: 95.291 ng
 RT: 10.69 min Scan# 1462
 Delta R.T. -0.00 min
 Lab File: BF100964.D
 Acq: 29 Nov 2017 5:45

Instrument :
 BNA_F
 ClientSampleId :
 112217-JETT-F-D-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.1	77.0	115.6
141	29.4	29.9	44.9#

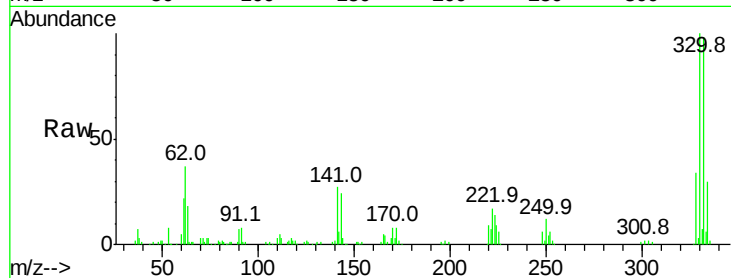


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

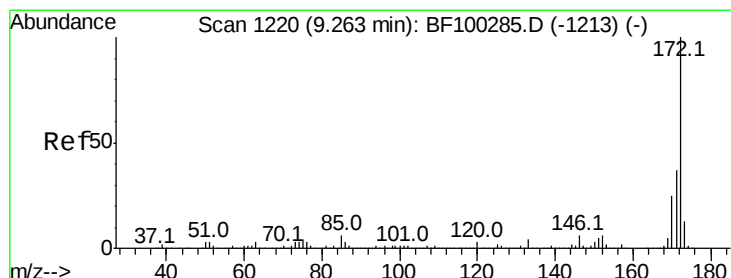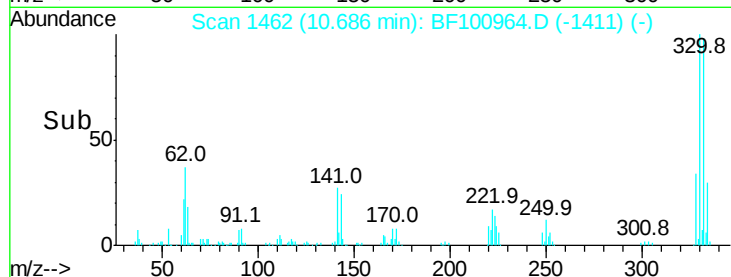
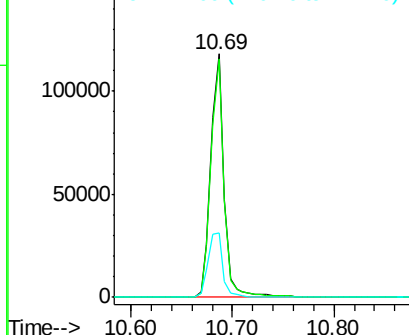


#44
 2-Fluorobiphenyl
 Concen: 115.282 ng
 RT: 9.22 min Scan# 1212
 Delta R.T. -0.00 min
 Lab File: BF100964.D
 Acq: 29 Nov 2017 5:45

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	29.7	44.5
170	24.2	19.6	29.4

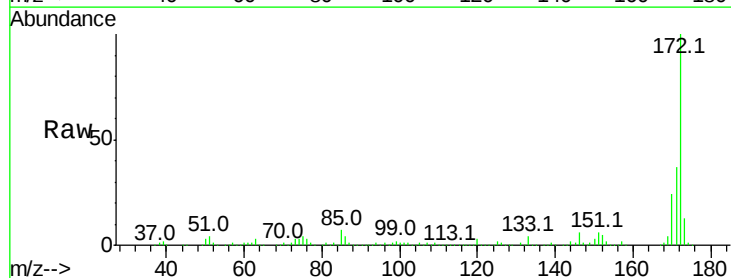

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



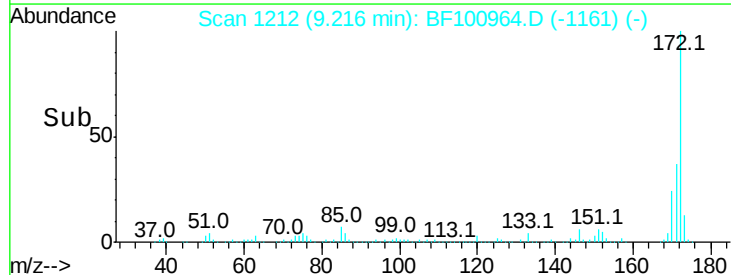
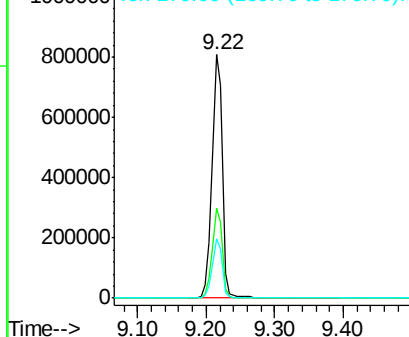




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.38 min Scan# 1580
Delta R.T. -0.00 min
Lab File: BF100964.D
Acq: 29 Nov 2017 5:45




Instrument :
BNA_F
ClientSampleId :
112217-JETT-F-D-S


Tot Ion	Ratio	Lower	Upper
188	100		
94	8.8	8.5	12.7
80	9.3	9.2	13.8

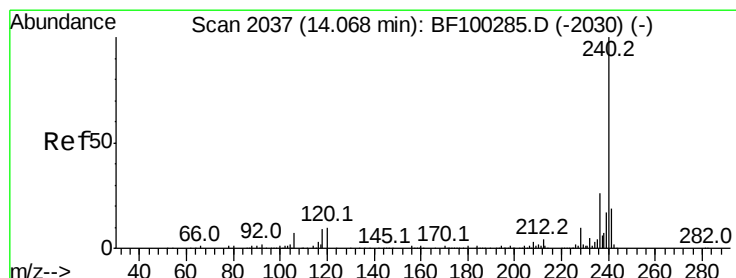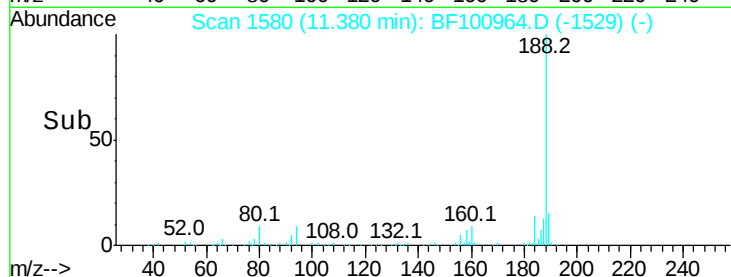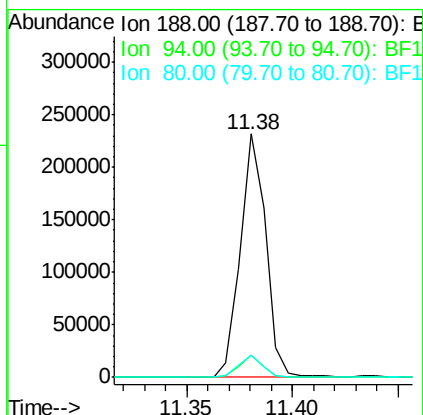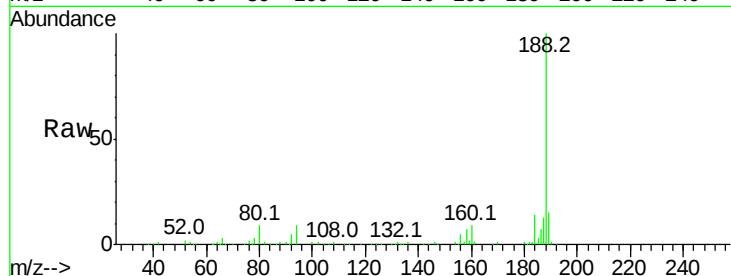

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.02 min Scan# 2029
Delta R.T. -0.01 min
Lab File: BF100964.D
Acq: 29 Nov 2017 5:45

Tgt Ion	Ratio	Lower	Upper
240	100		
120	9.6	9.5	14.3
236	26.0	20.7	31.1

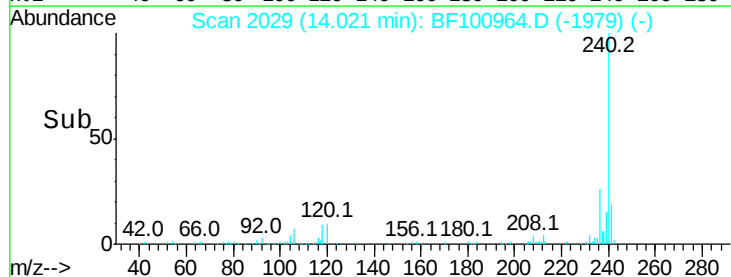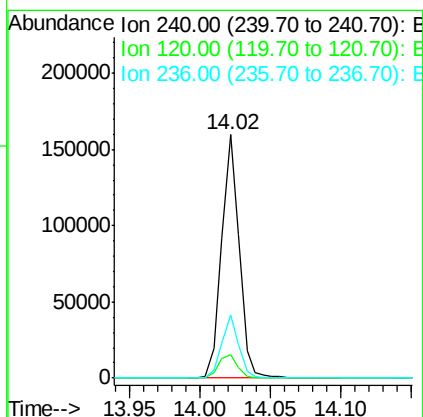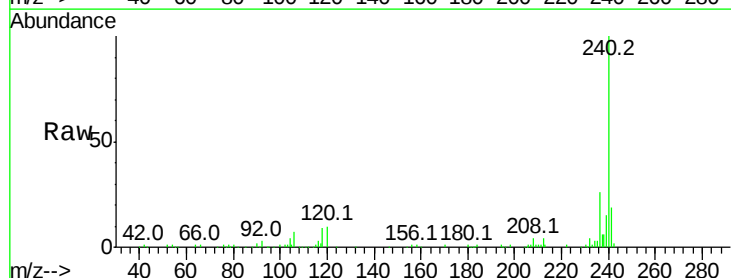

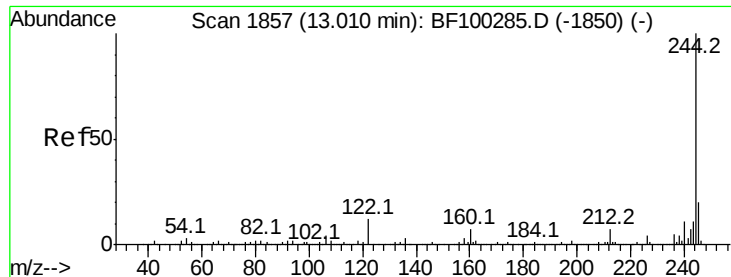

#78

Terphenyl-d14

Concen: 98.388 ng

RT: 12.97 min Scan# 1850

Delta R.T. -0.00 min

Lab File: BF100964.D

Acq: 29 Nov 2017 5:45

Instrument :

BNA_F

ClientSampleId :

112217-JETT-F-D-S


Tot Ion:244 Resp: 598292

Ion Ratio Lower Upper

244 100

212 7.3 5.4 8.0



122 11.3 11.0 16.4

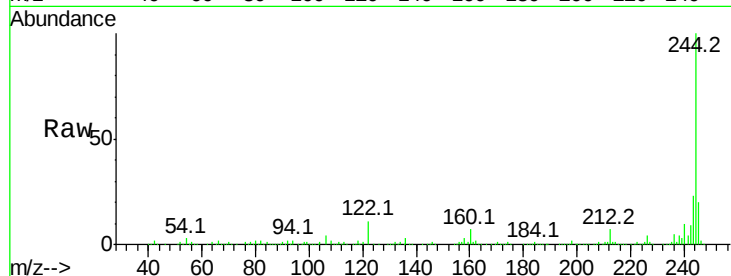

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

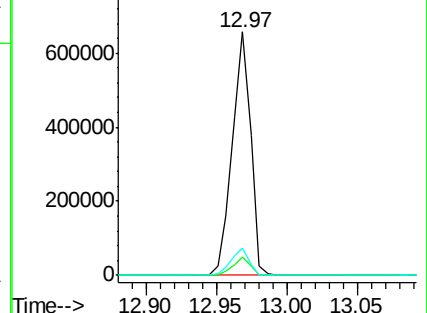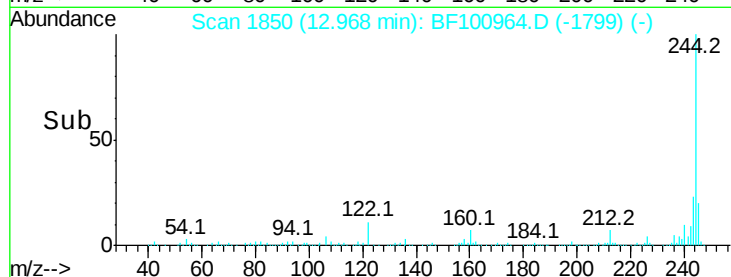

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.49 min Scan# 2279

Delta R.T. -0.00 min

Lab File: BF100964.D

Acq: 29 Nov 2017 5:45


Tgt Ion:264 Resp: 124264

Ion Ratio Lower Upper

264 100

260 23.0 19.2 28.8

265 21.1 17.5 26.3

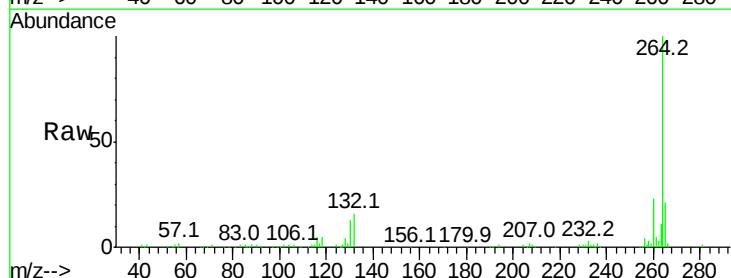

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

