
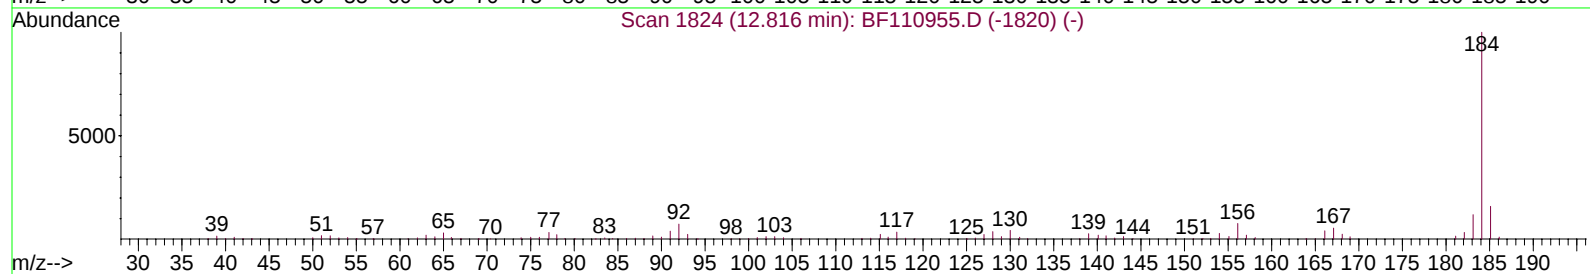
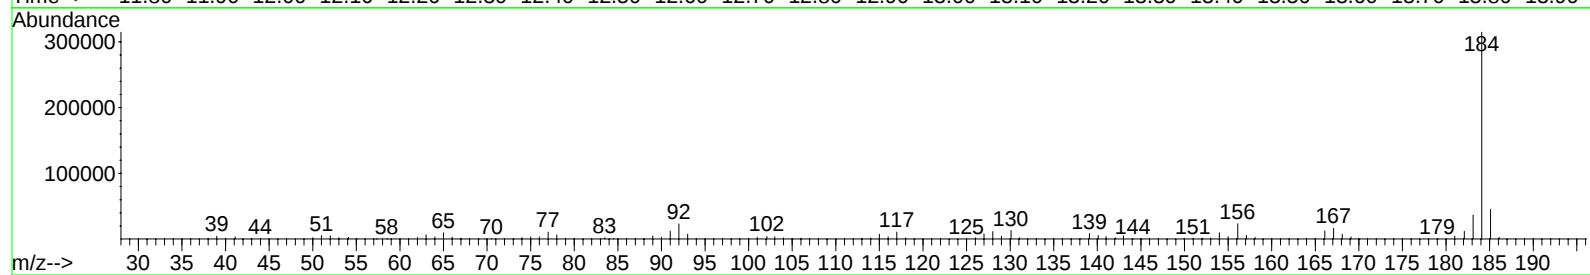


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112818\
 Data File : BF111040.D
 Acq On : 28 Nov 2018 12:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 13:20:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 27 15:32:10 2018
 Response via : Initial Calibration

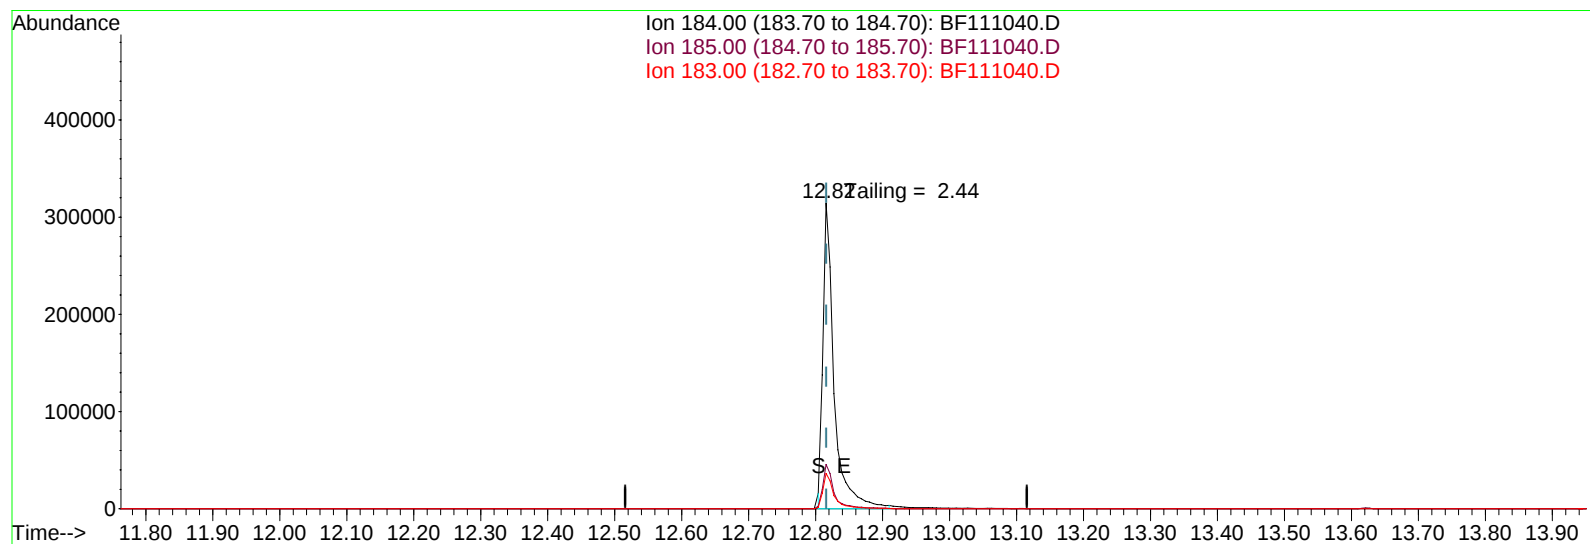

TIC: BF111040.D

(77) Benzidine




12.816min (+0.000) 0.00ng

response 376640

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.52
183.00	11.80	11.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112818\
 Data File : BF111040.D
 Acq On : 28 Nov 2018 12:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 13:20:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 27 15:32:10 2018
 Response via : Initial Calibration

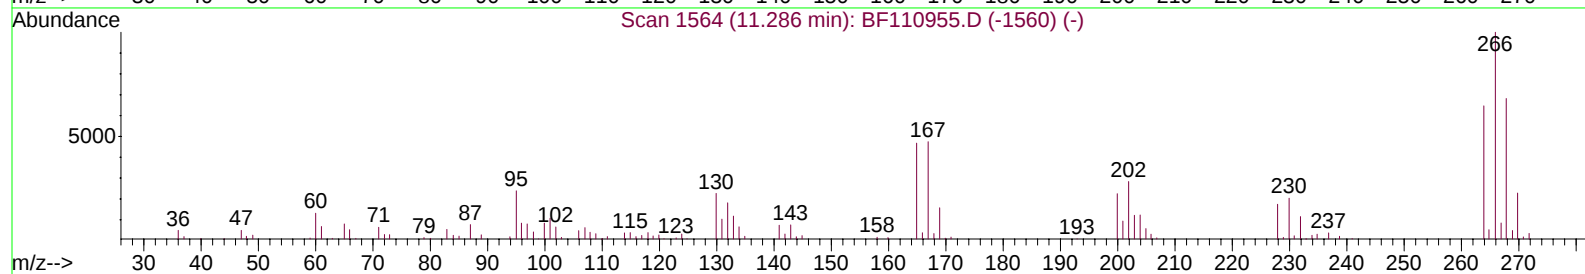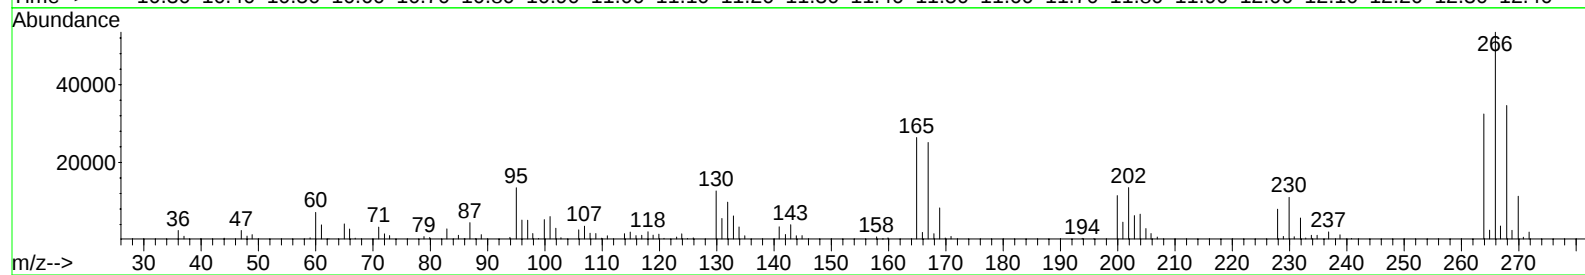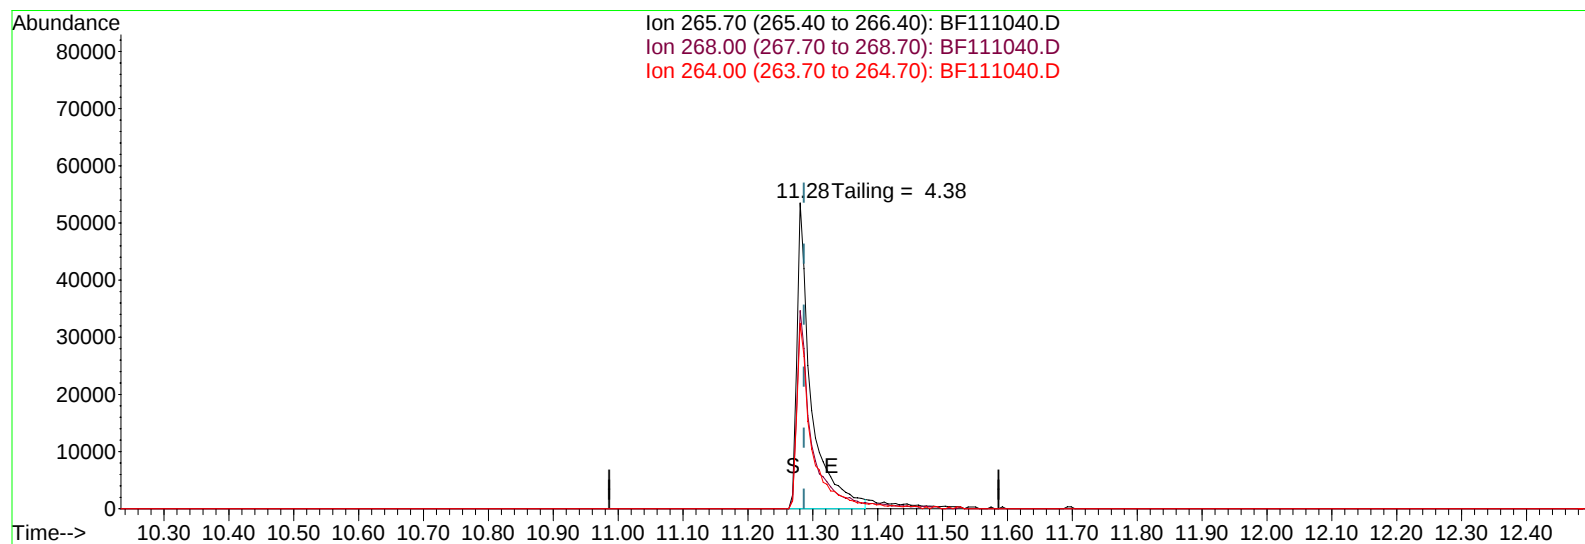

TIC: BF111040.D

(70) Pentachlorophenol (C)

11.280min (-0.006) 133042.49ng

response 87190

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	64.77
264.00	63.20	60.64
0.00	0.00	0.00