
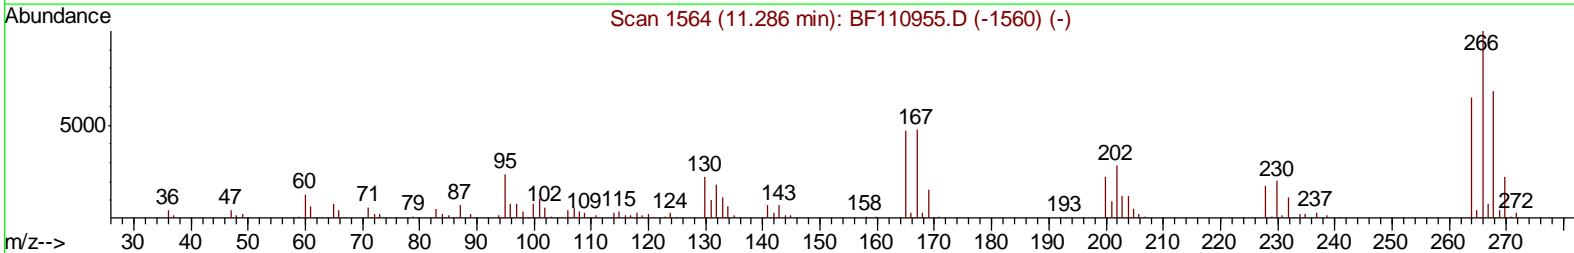
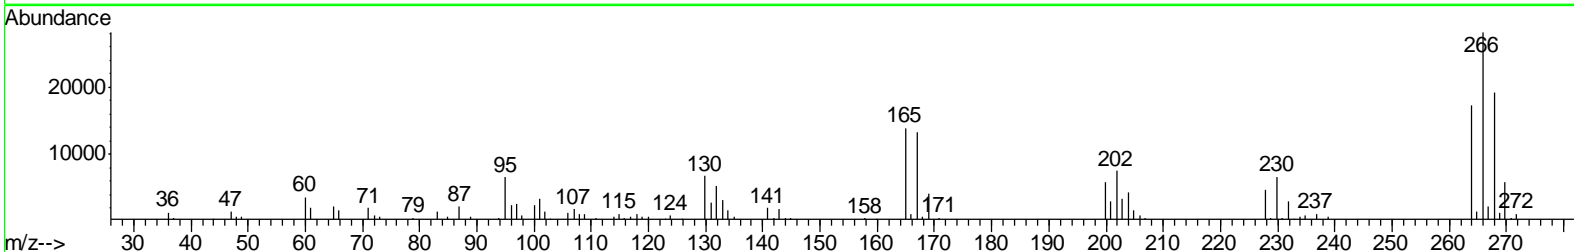


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112818\
 Data File : BF111065.D
 Acq On : 29 Nov 2018 1:15
 Operator : JU/SJ
 Sample : DF7TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 06:55:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF112618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 27 15:32:10 2018
 Response via : Initial Calibration

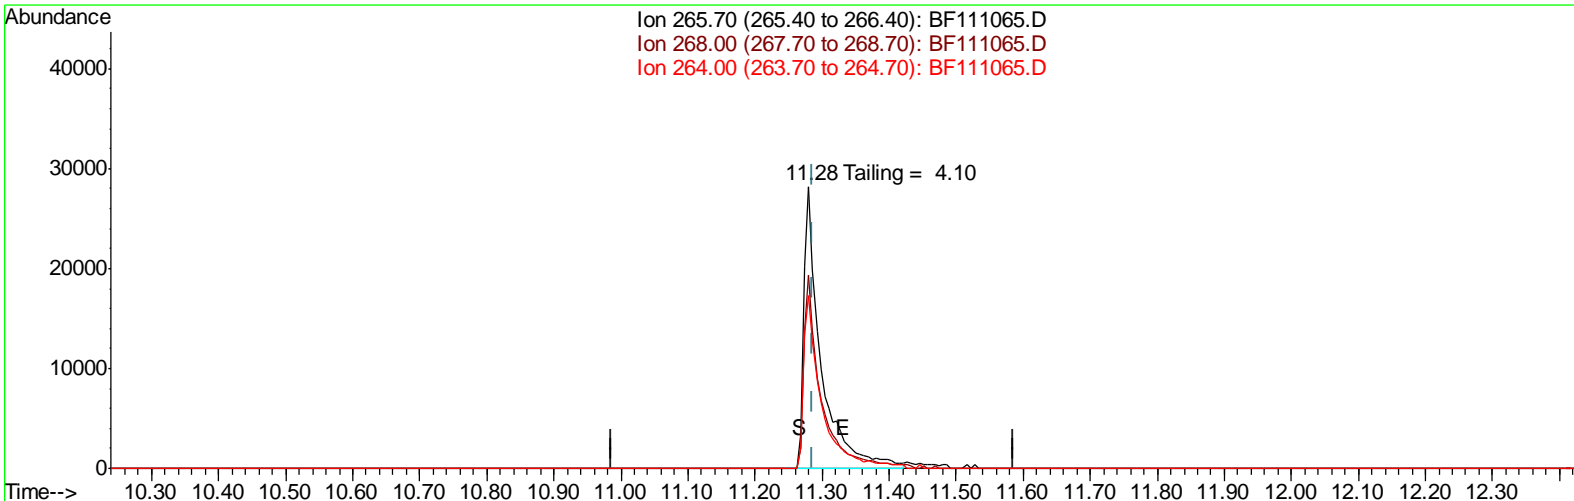

TIC: BF111065.D

(70) Pentachlorophenol (C)




11.280min (-0.006) 0.00ng

response 49776

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	68.49
264.00	63.20	61.45
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112818\
 Data File : BF111065.D
 Acq On : 29 Nov 2018 1:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 06:55:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF112618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 27 15:32:10 2018
 Response via : Initial Calibration

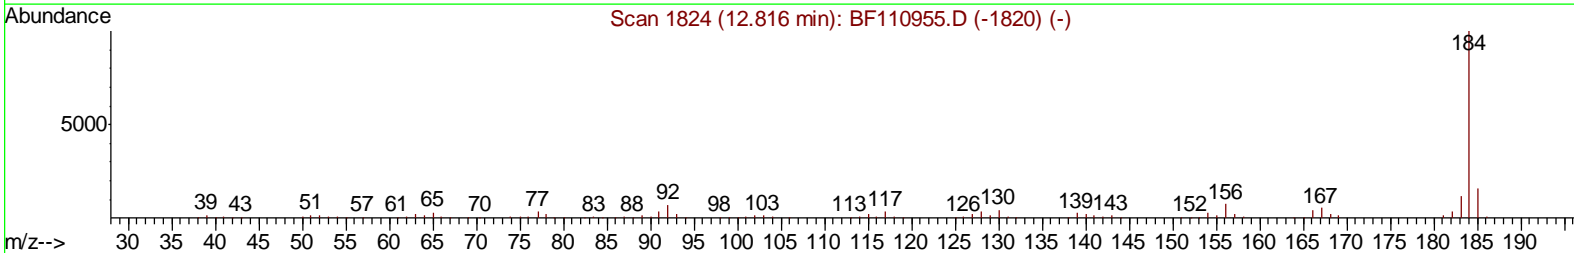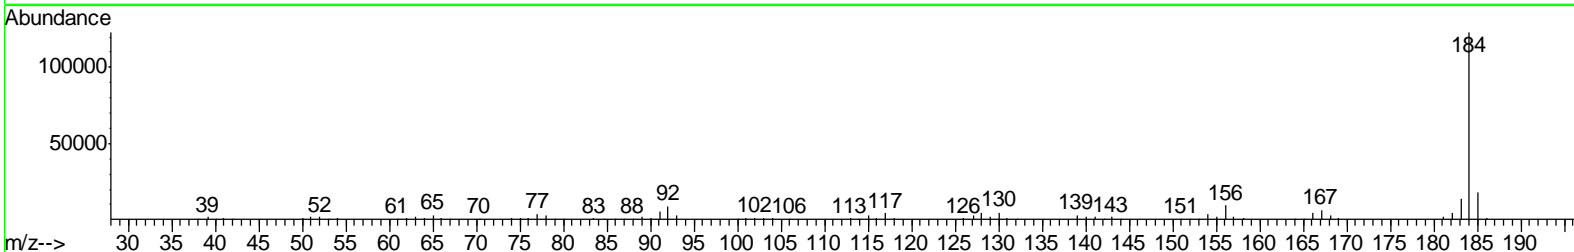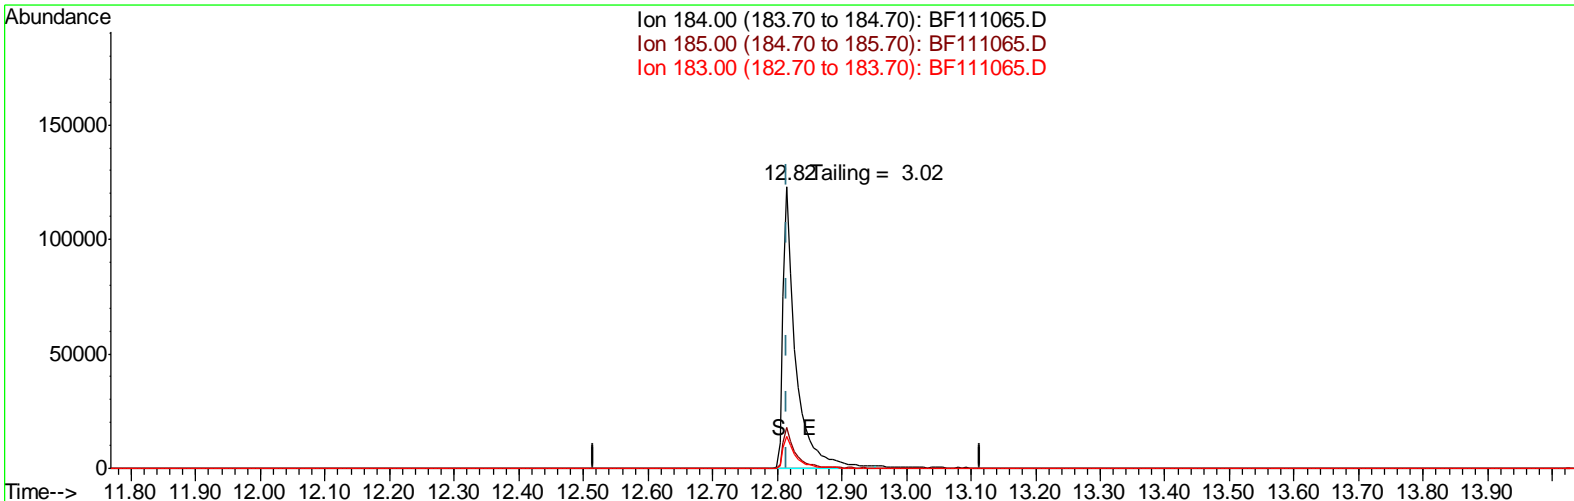

TIC: BF111065.D

(77) Benzidine

12.816min (-0.000) 0.00ng

response 175307

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.44
183.00	11.80	11.29
0.00	0.00	0.00