


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112818\
 Data File : BF111065.D
 Acq On : 29 Nov 2018 1:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF112618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 27 15:32:10 2018

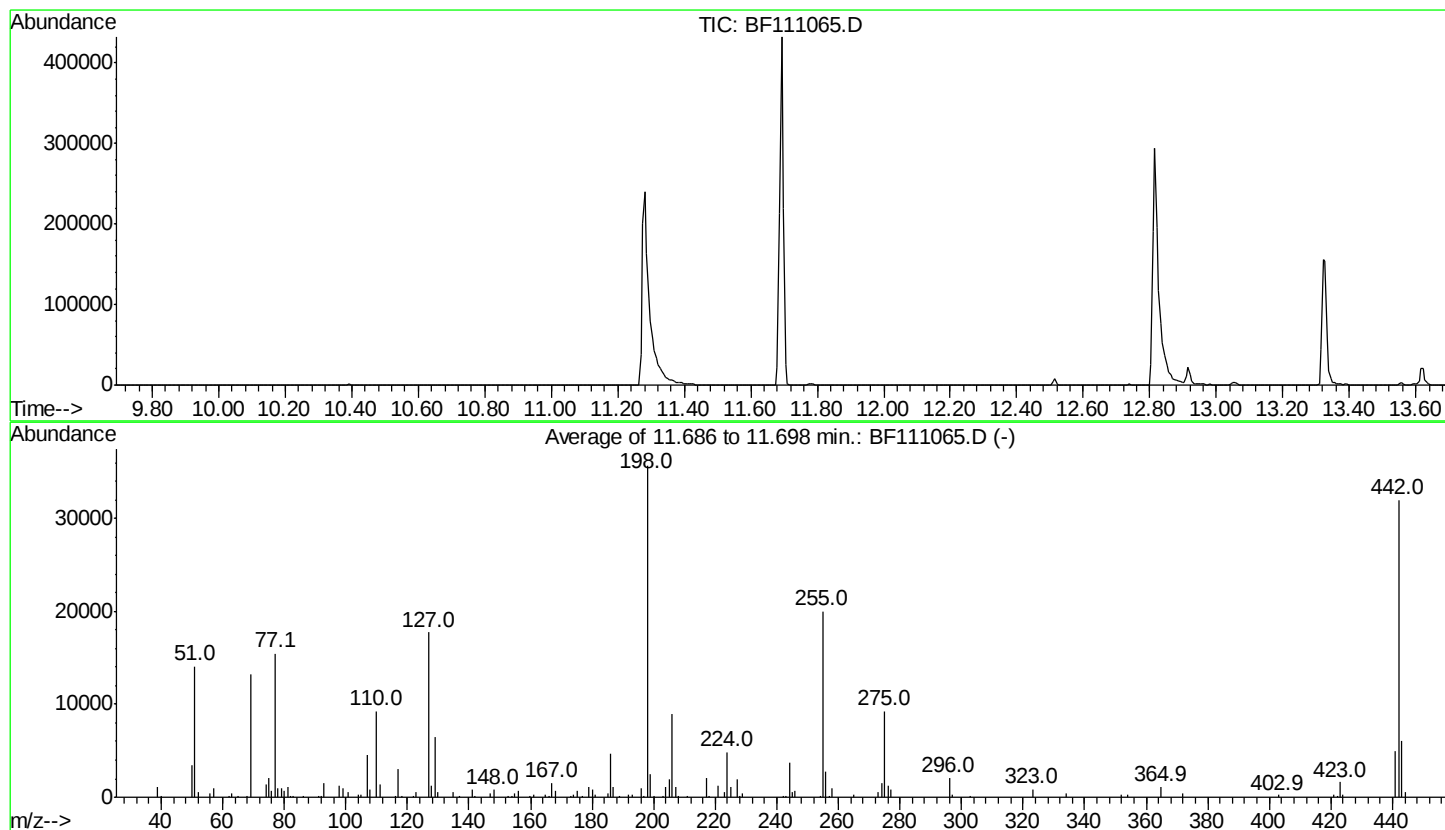

AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	14095	PASS
68	69	0.00	2	0.9	116	PASS
69	198	0.00	100	37.1	13239	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	17749	PASS
197	198	0.00	2	0.4	145	PASS
198	198	100	100	100.0	35698	PASS
199	198	5	9	6.9	2464	PASS
275	198	10	60	26.0	9275	PASS
365	198	1	100	3.3	1161	PASS
441	198	0.01	100	13.8	4927	PASS
442	198	50	100	89.7	32006	PASS
443	442	15	24	18.9	6041	PASS