
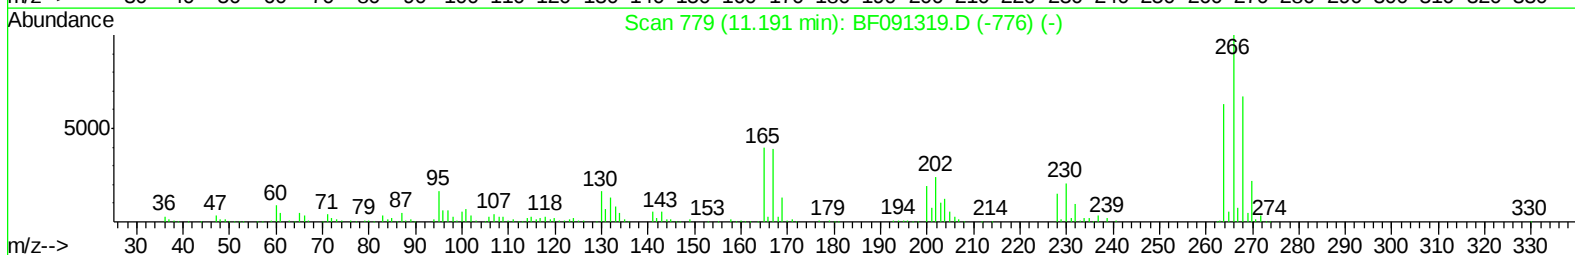
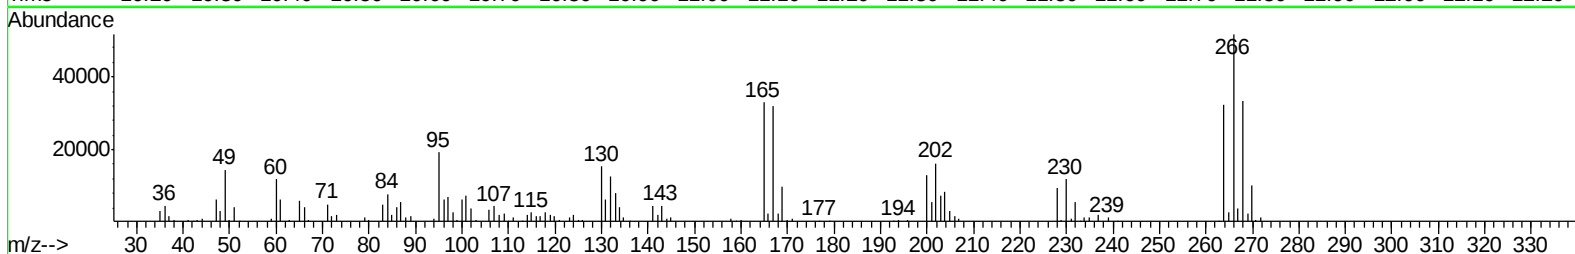


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112916\
Data File : BF091315.D
Acq On : 29 Nov 2016 9:33
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 06:31:36 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

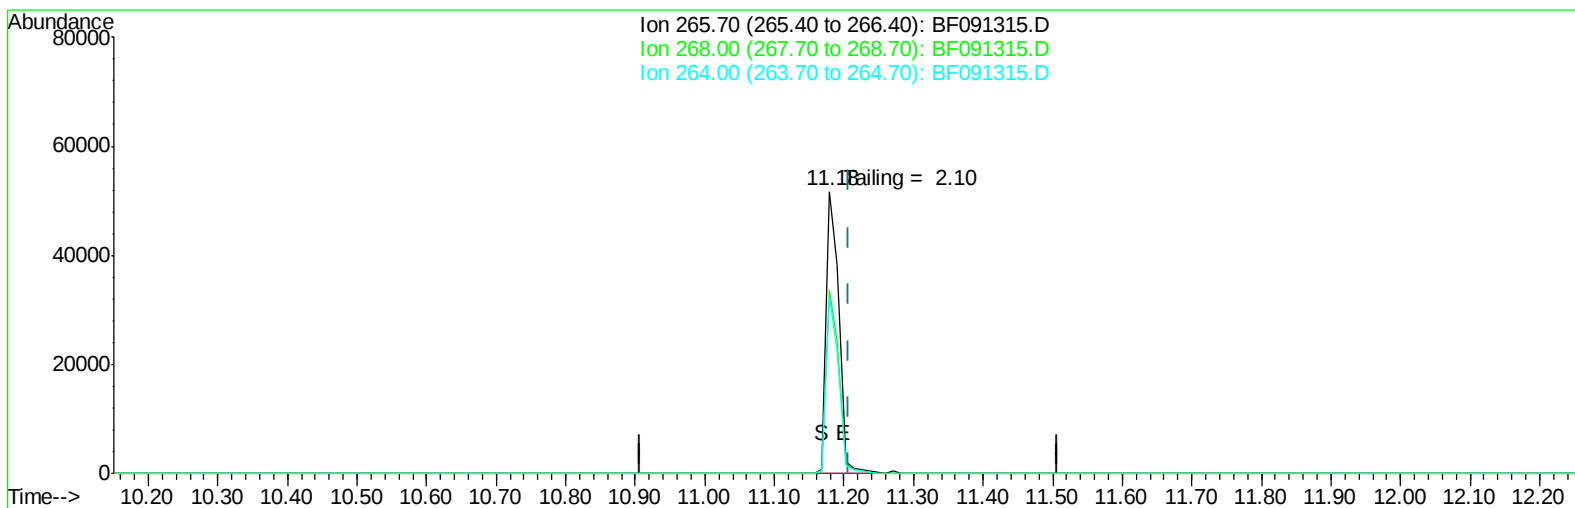

TIC: BF091315.D

(69) Pentachlorophenol (C)




11.179min (-0.029) 22573.22ng

response 65289

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	64.85
264.00	60.20	62.65
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112916\
Data File : BF091315.D
Acq On : 29 Nov 2016 9:33
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 06:31:36 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

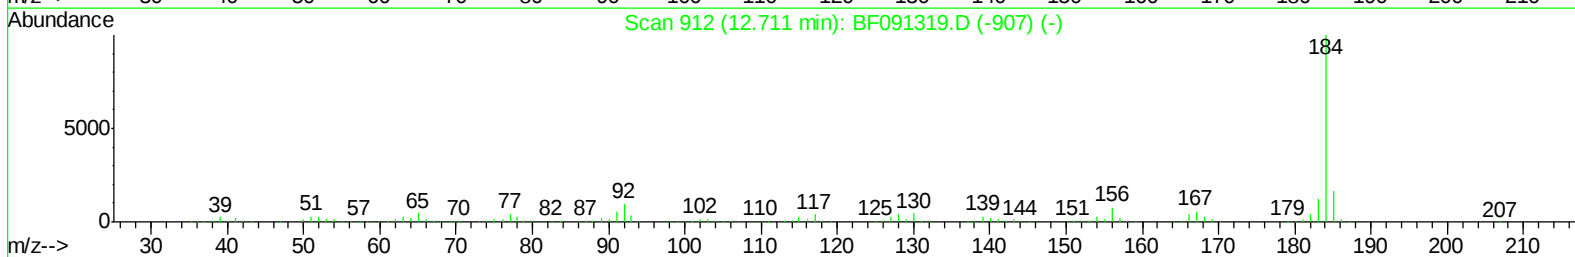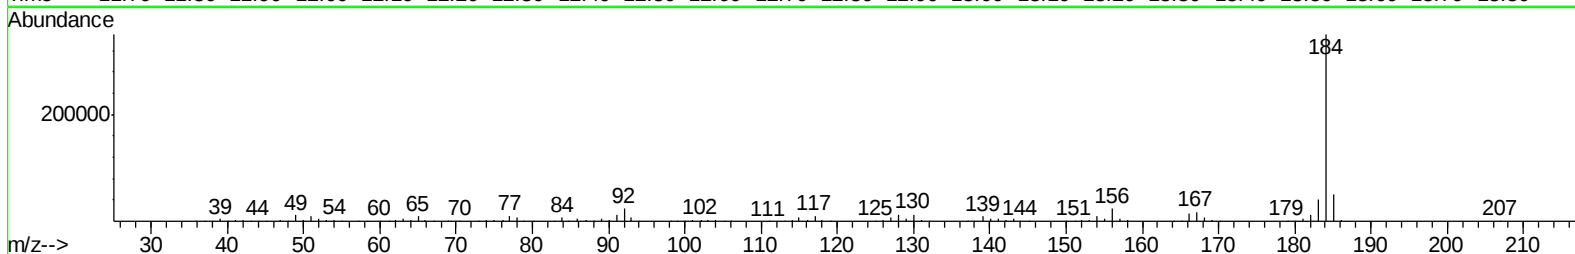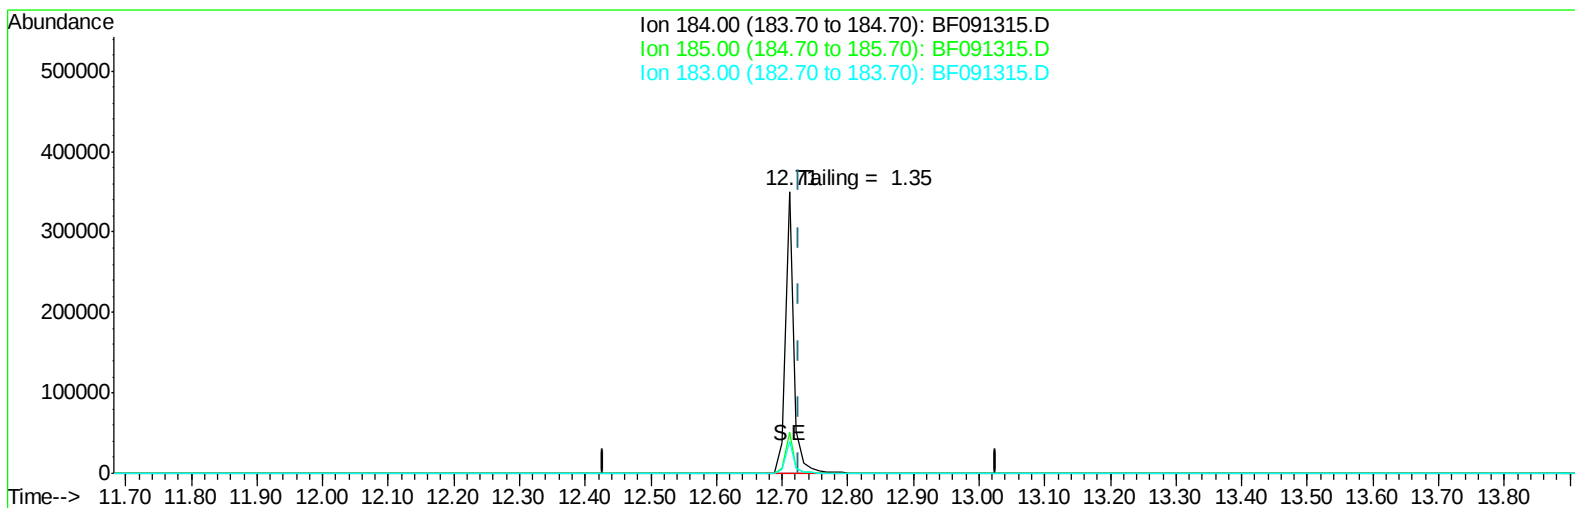

TIC: BF091315.D

(76) Benzidine

12.711min (-0.016) 3244.48ng

response 323265

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	14.56
183.00	11.10	11.54
0.00	0.00	0.00