


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112916\
 Data File : BF091315.D
 Acq On : 29 Nov 2016 9:33
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 13:33:46 2016

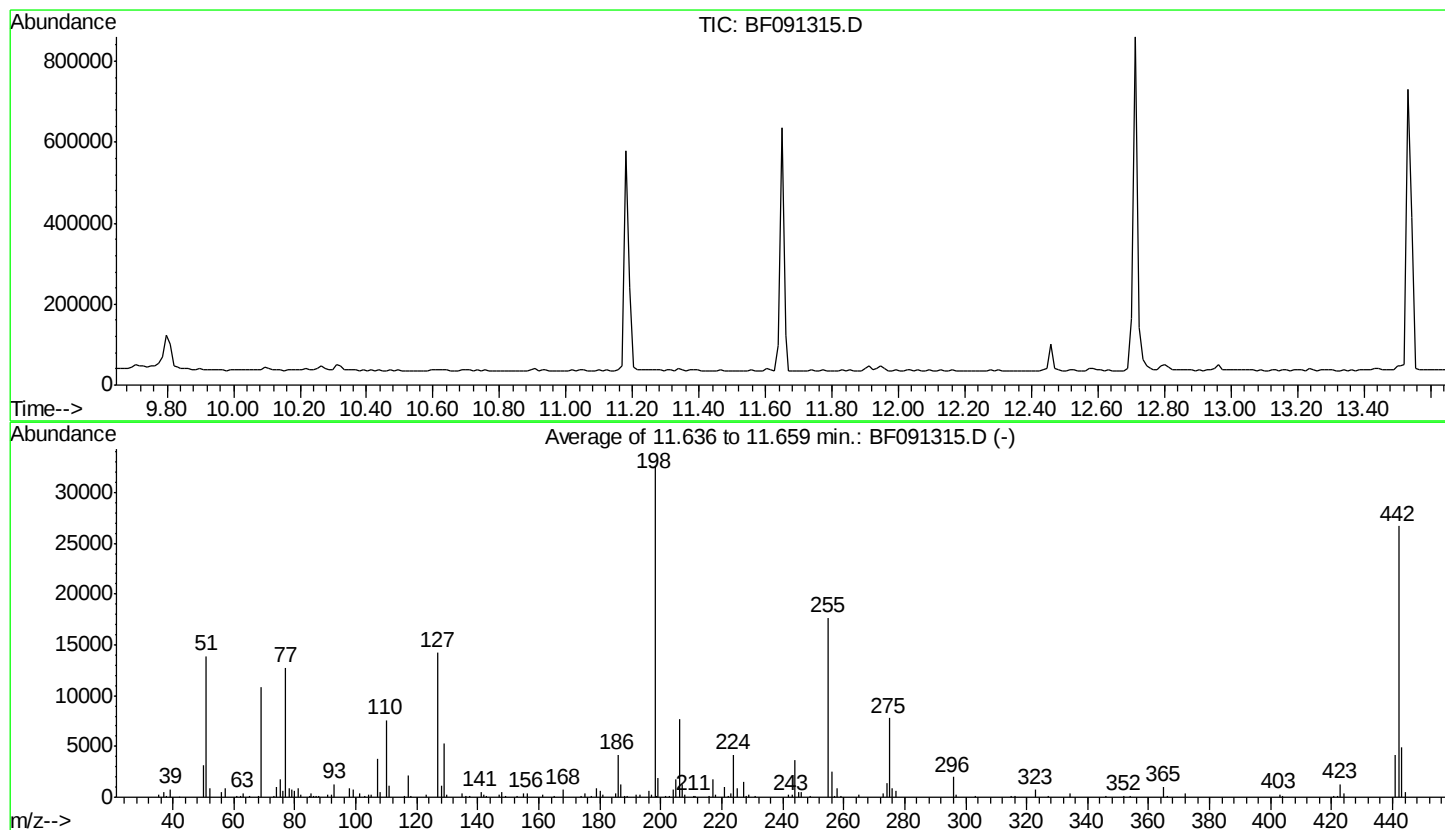

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	13928	PASS
68	69	0.00	2	1.4	153	PASS
69	198	0.00	100	33.3	10861	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.6	14224	PASS
197	198	0.00	2	0.7	224	PASS
198	198	100	100	100.0	32654	PASS
199	198	5	9	5.9	1938	PASS
275	198	10	60	23.9	7799	PASS
365	198	1	100	3.2	1054	PASS
441	442	0.01	24	15.8	4205	PASS
442	198	50	100	81.7	26676	PASS
443	442	15	24	18.4	4917	PASS