
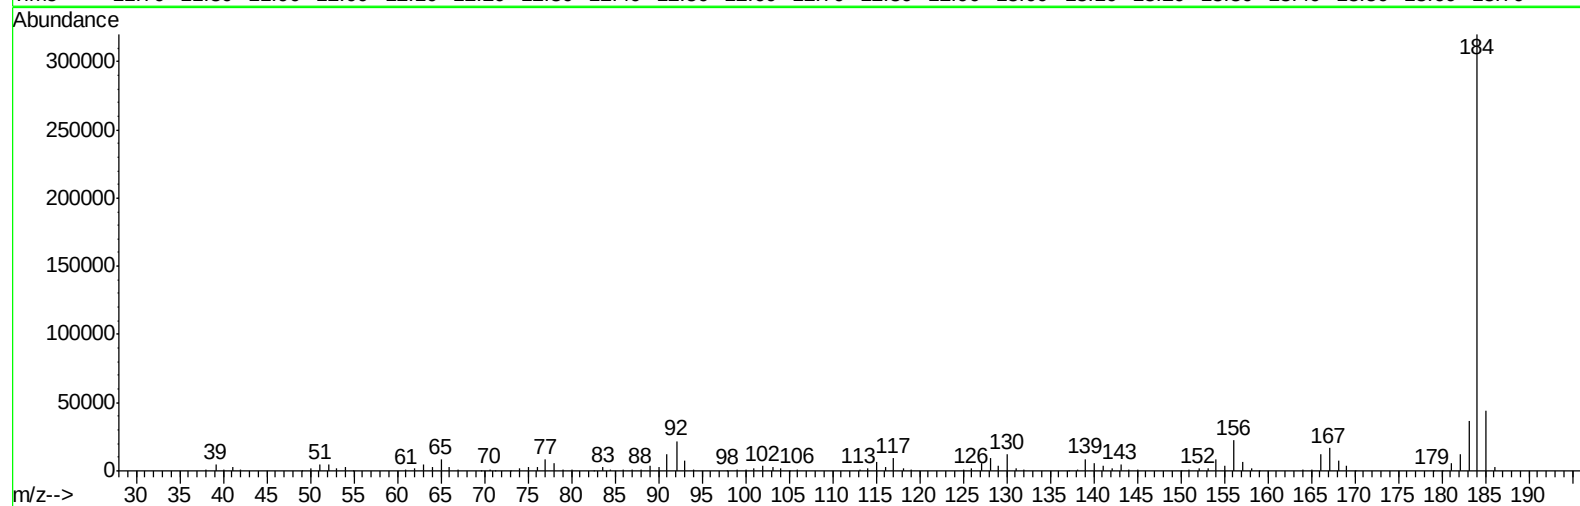


Data Path : Z:\HPCHEM1\BNA F\Data\BF112917\
Data File : BF100972.D
Acq On : 29 Nov 2017 11:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 08:24:45 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 15:21:02 2017
Response via : Initial Calibration

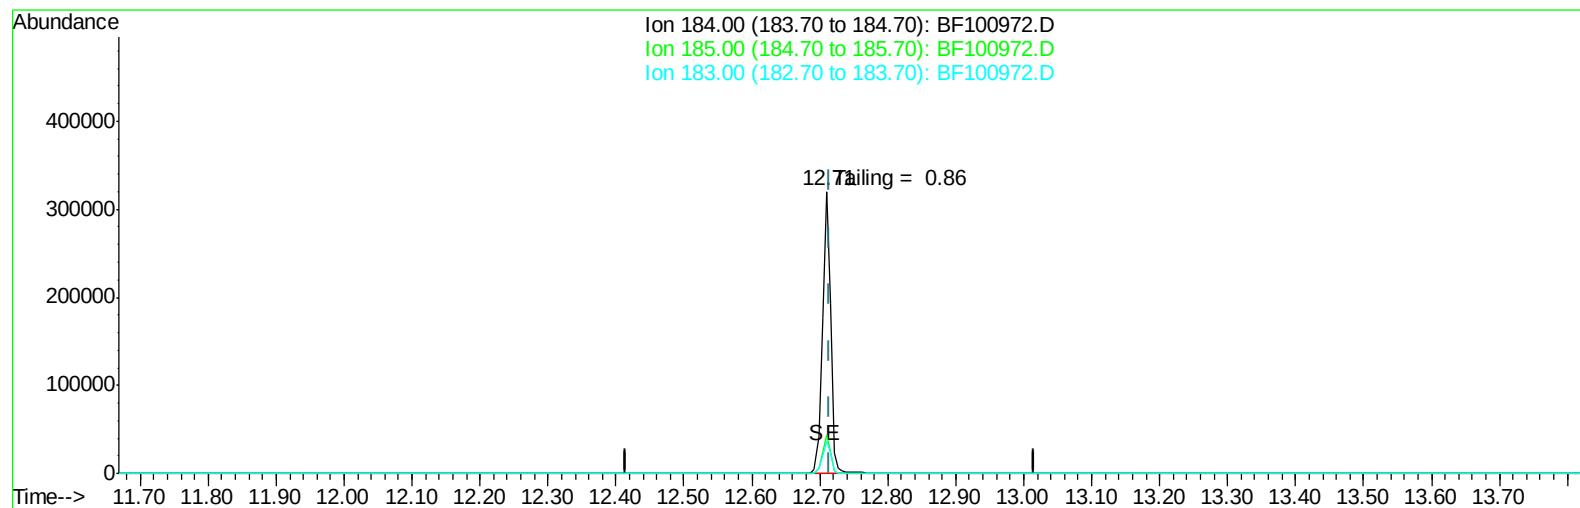

TIC: BF100972.D

(76) Benzidine



12.710min (-0.006) 0.00ng

response 274769

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.73
183.00	11.60	11.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF112917\
Data File : BF100972.D
Acq On : 29 Nov 2017 11:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 08:24:45 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 15:21:02 2017
Response via : Initial Calibration

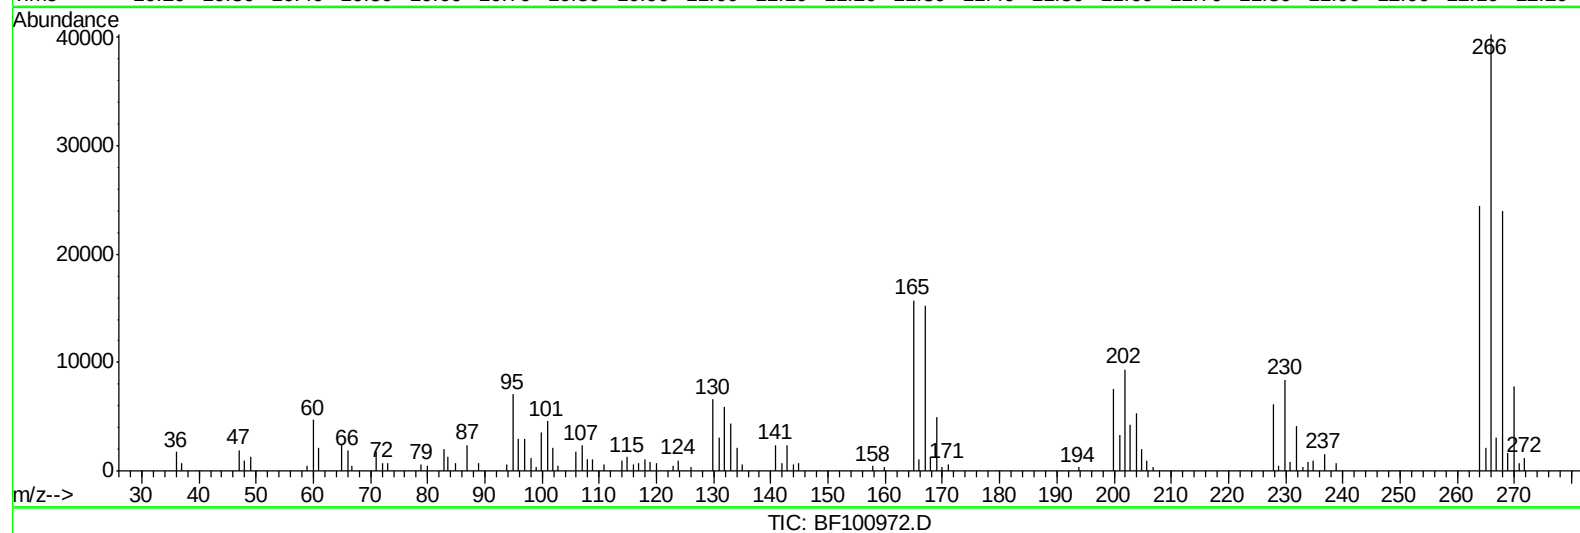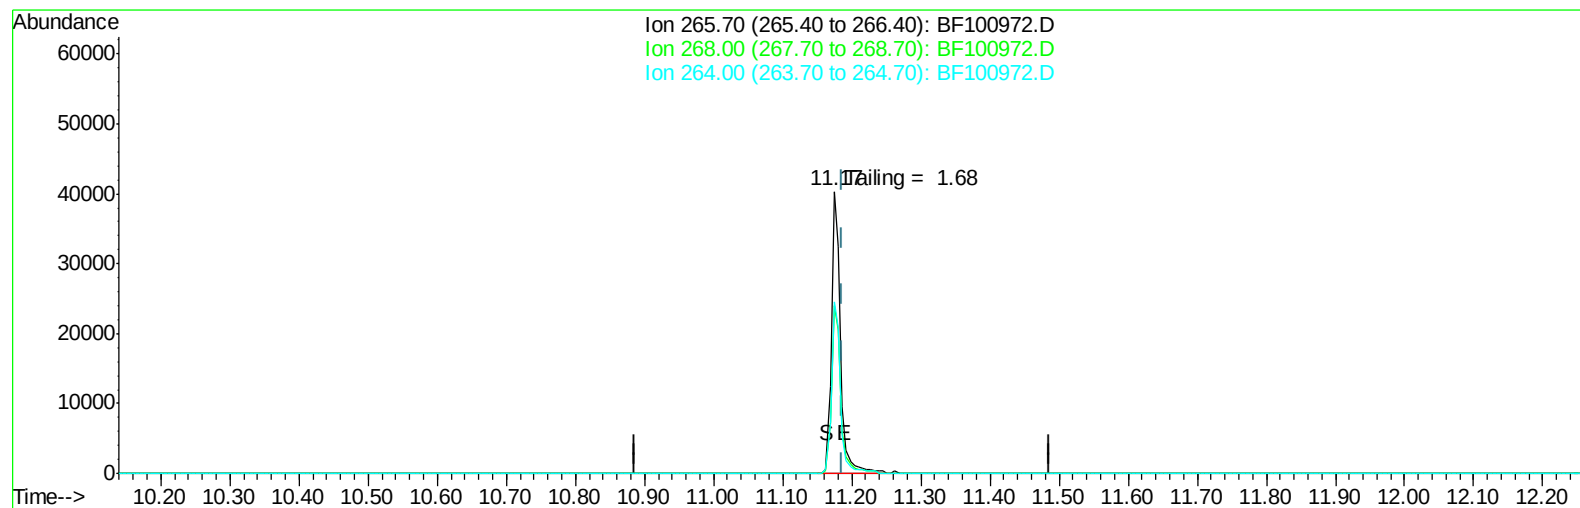

(69) Pentachlorophenol (C)

11.174min (-0.012) 0.00ng

response 37158

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.53
264.00	61.90	60.80
0.00	0.00	0.00