
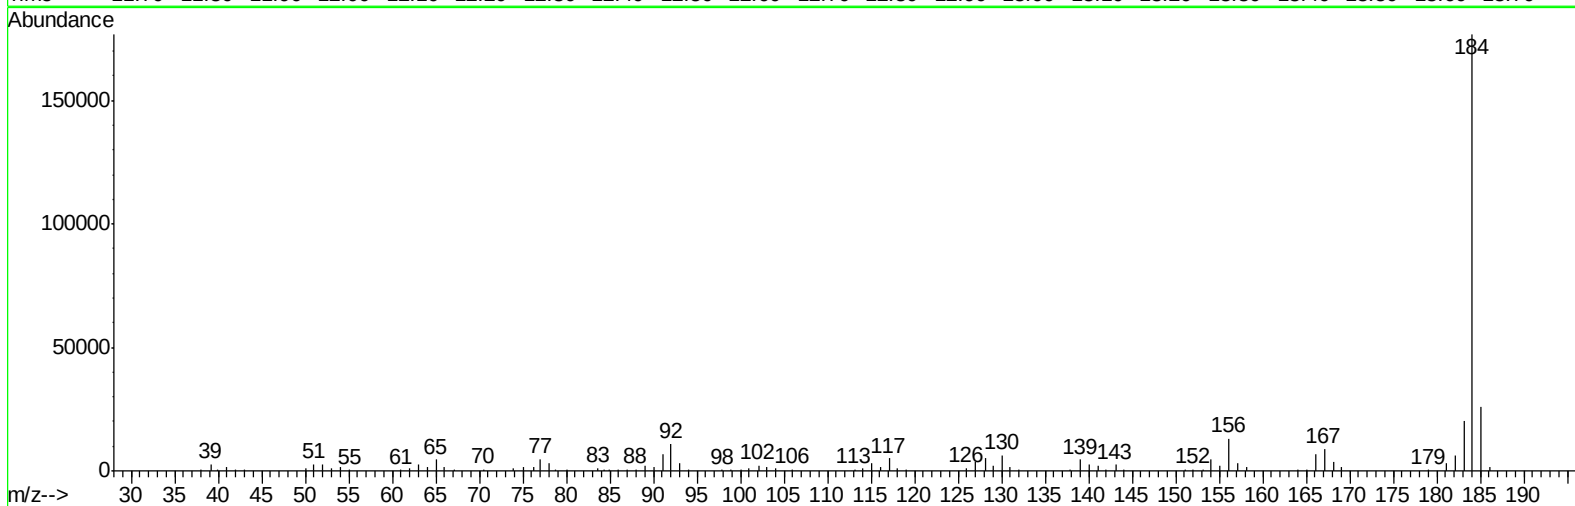


Data Path : Z:\HPCHEM1\BNA F\Data\BF112917\
Data File : BF100997.D
Acq On : 30 Nov 2017 00:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 08:25:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 15:21:02 2017
Response via : Initial Calibration

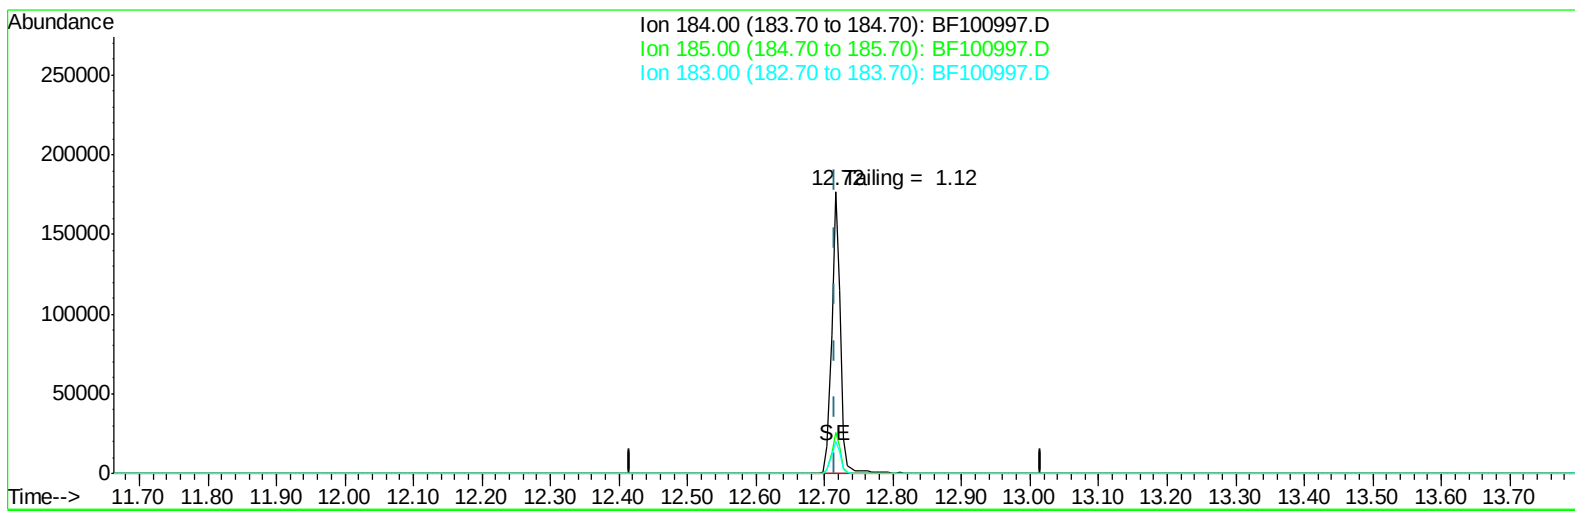

TIC: BF100997.D

(76) Benzidine



12.716min (-0.000) 0.00ng

response 154013

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.77
183.00	11.60	11.55
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF112917\
Data File : BF100997.D
Acq On : 30 Nov 2017 00:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 08:25:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 15:21:02 2017
Response via : Initial Calibration

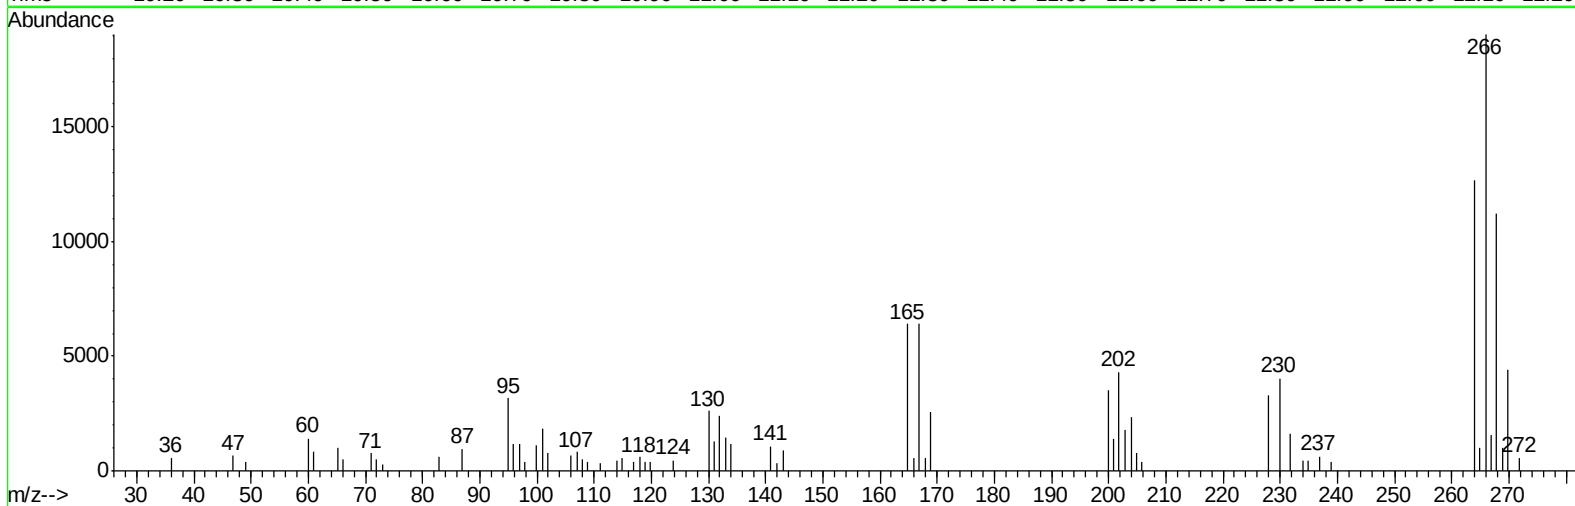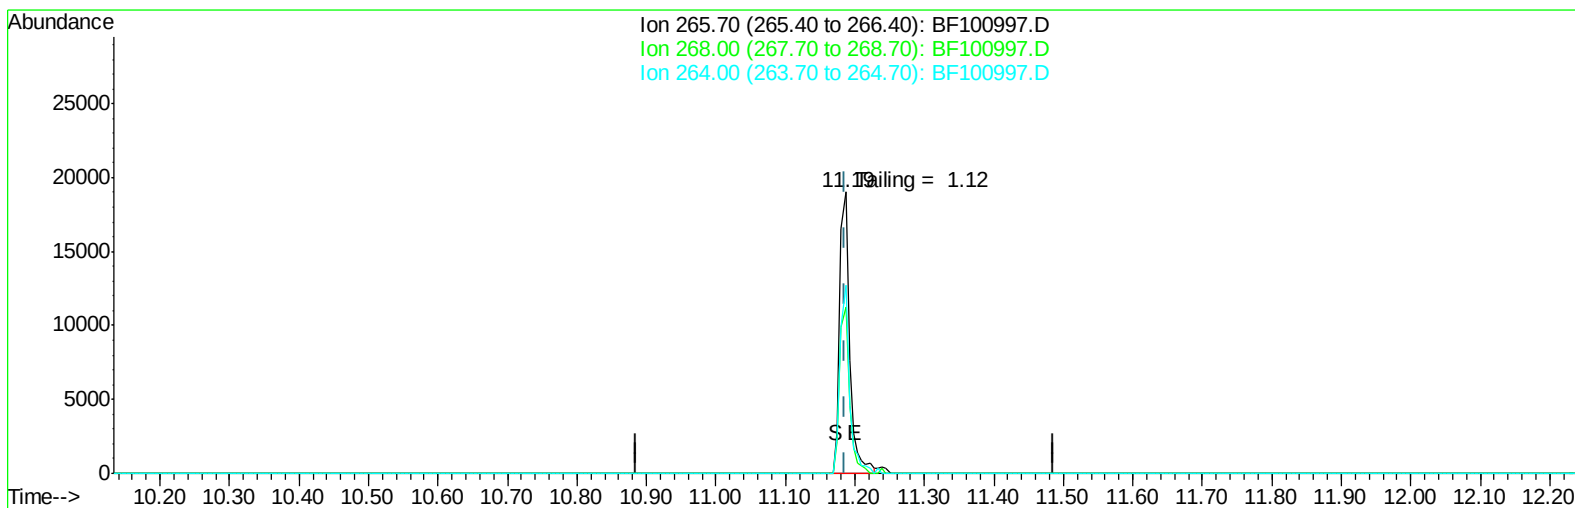

TIC: BF100997.D

(69) Pentachlorophenol (C)

11.186min (-0.000) 0.00ng

response 18690

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.90
264.00	61.90	66.66
0.00	0.00	0.00