


Data Path : Z:\HPCHEM1\BNA F\Data\BF112917\
 Data File : BF100972.D
 Acq On : 29 Nov 2017 11:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 28 15:21:02 2017

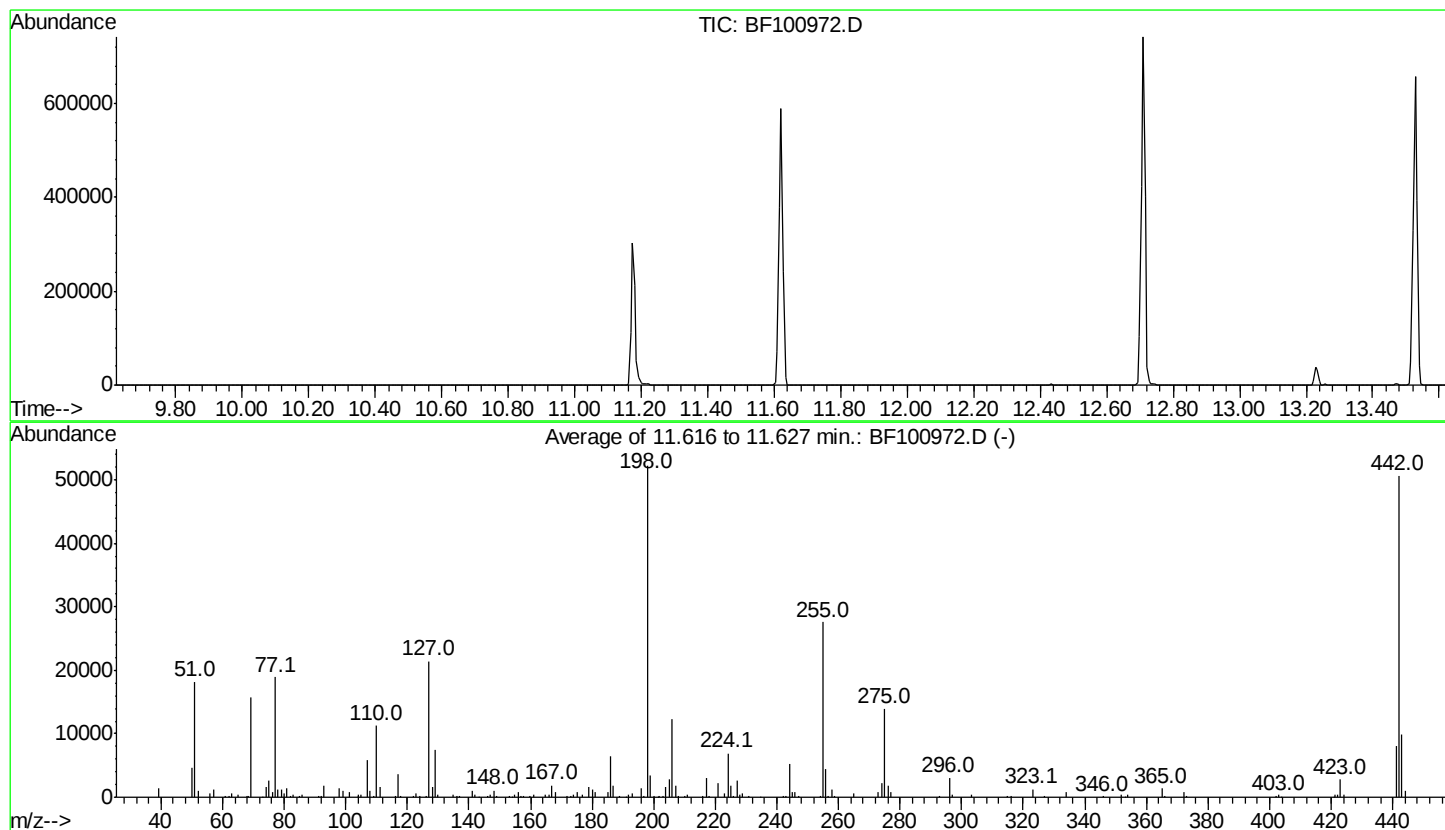

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	18162	PASS
68	69	0.00	2	0.9	148	PASS
69	198	0.00	100	30.1	15737	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.1	21446	PASS
197	198	0.00	2	0.2	121	PASS
198	198	100	100	100.0	52226	PASS
199	198	5	9	6.6	3455	PASS
275	198	10	60	26.8	13997	PASS
365	198	1	100	2.7	1409	PASS
441	443	0.01	100	81.4	8049	PASS
442	198	50	100	96.9	50624	PASS
443	442	15	24	19.5	9890	PASS