


Data Path : Z:\HPCHEM1\BNA F\Data\BF112917\
 Data File : BF100997.D
 Acq On : 30 Nov 2017 00:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 28 15:21:02 2017

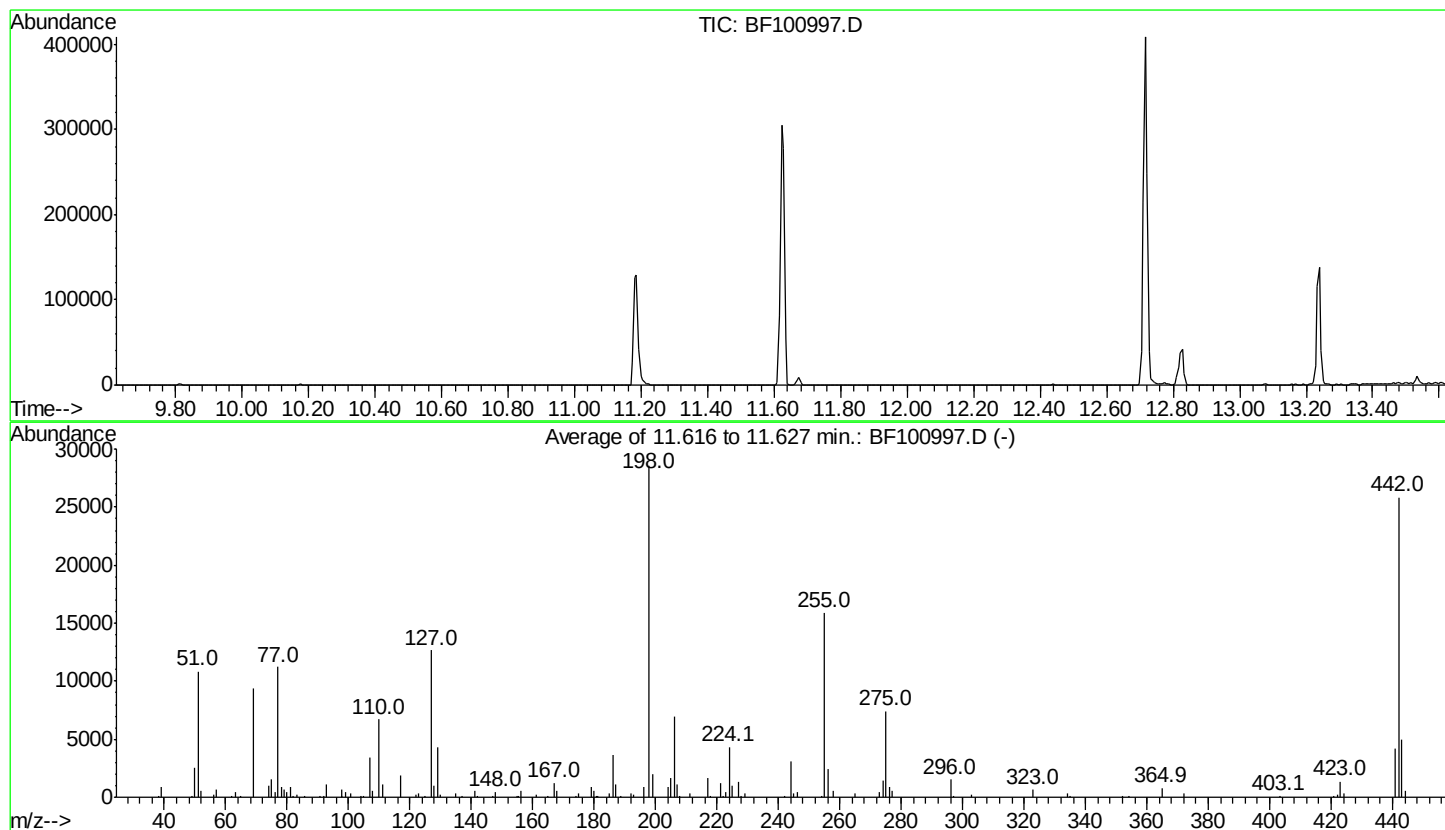

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	10863	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.0	9422	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.3	12659	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28573	PASS
199	198	5	9	6.8	1937	PASS
275	198	10	60	25.9	7414	PASS
365	198	1	100	2.8	813	PASS
441	443	0.01	100	85.4	4231	PASS
442	198	50	100	90.5	25867	PASS
443	442	15	24	19.2	4957	PASS