


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112922\
 Data File : BF131450.D
 Acq On : 29 Nov 2022 09:07
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 00:18:36 2022

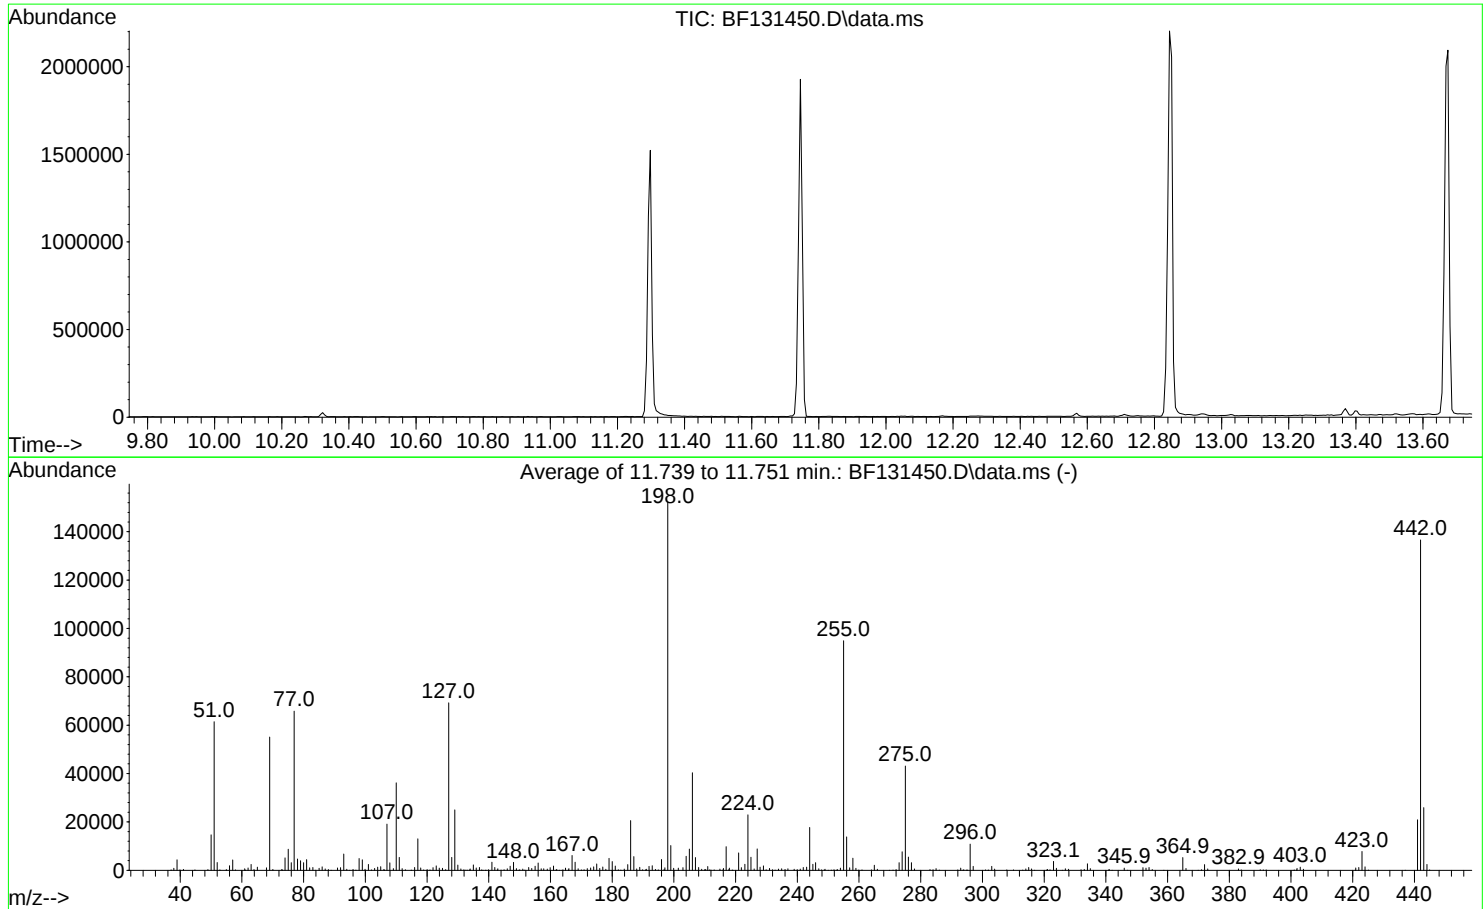




AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	61403	PASS
68	69	0.00	2	1.8	1004	PASS
69	198	0.00	100	36.2	55078	PASS
70	69	0.00	2	0.6	342	PASS
127	198	10	80	45.5	69272	PASS
197	198	0.00	2	0.7	1014	PASS
198	198	100	100	100.0	152112	PASS
199	198	5	9	6.7	10220	PASS
275	198	10	60	28.3	43093	PASS
365	198	1	100	3.5	5273	PASS
441	198	0.01	100	13.7	20899	PASS
442	442	50	100	100.0	136581	PASS
443	442	15	24	19.0	25900	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112922\
 Data File : BF131450.D
 Acq On : 29 Nov 2022 09:07
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 30 05:06:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 00:18:36 2022
 Response via : Initial Calibration

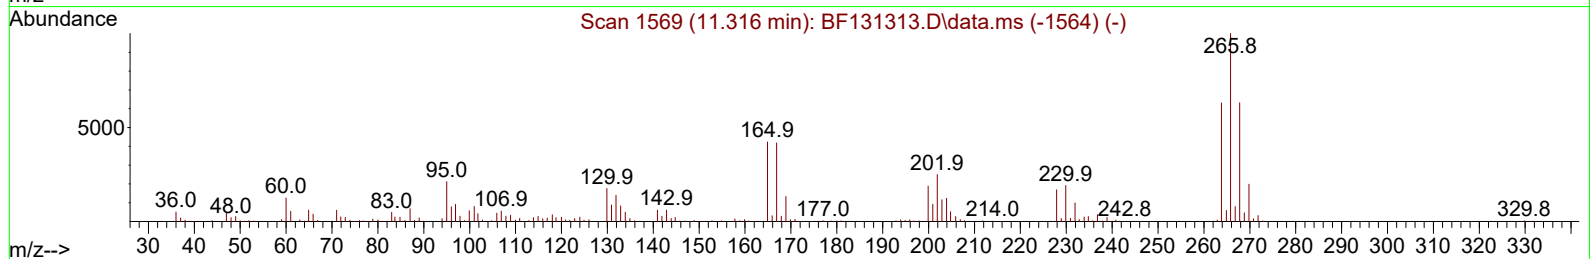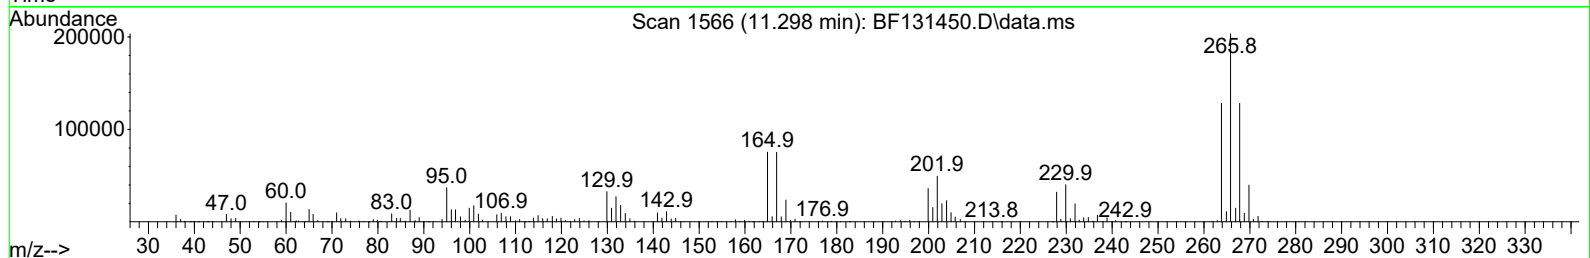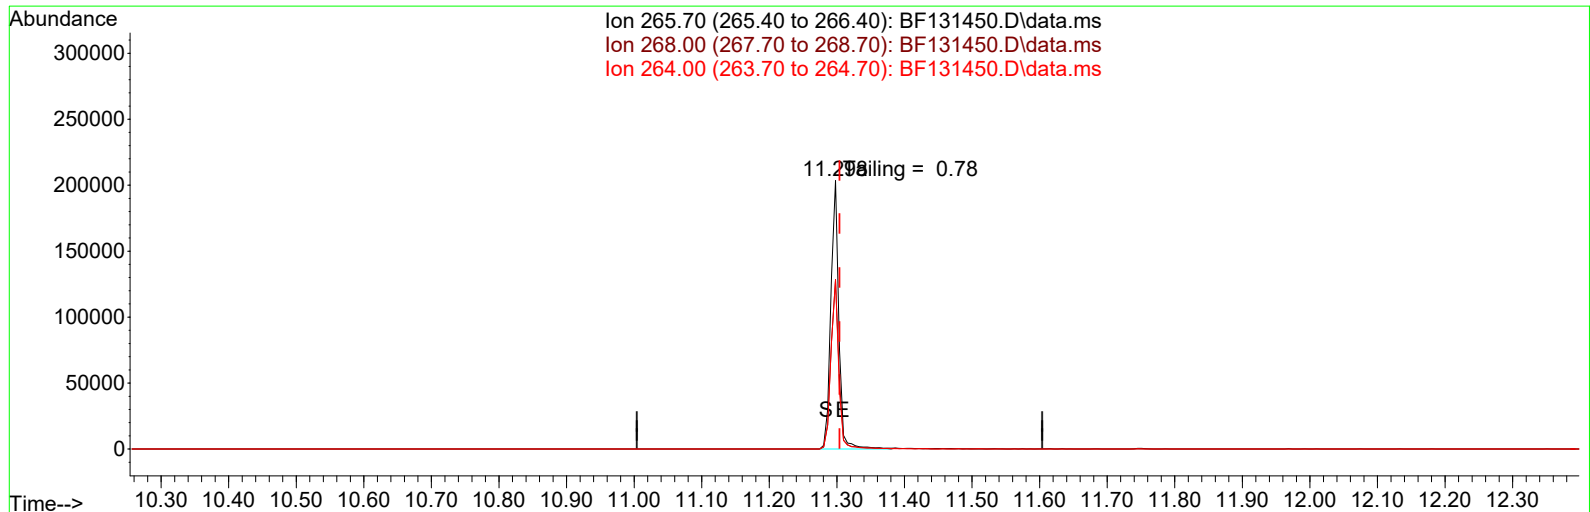

TIC: BF131450.D\data.ms

(70) Pentachlorophenol (C)

11.298min (-0.006) 33167.77 ng




response 167639

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	63.04
264.00	63.00	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112922\
Data File : BF131450.D
Acq On : 29 Nov 2022 09:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 30 05:06:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 00:18:36 2022
Response via : Initial Calibration

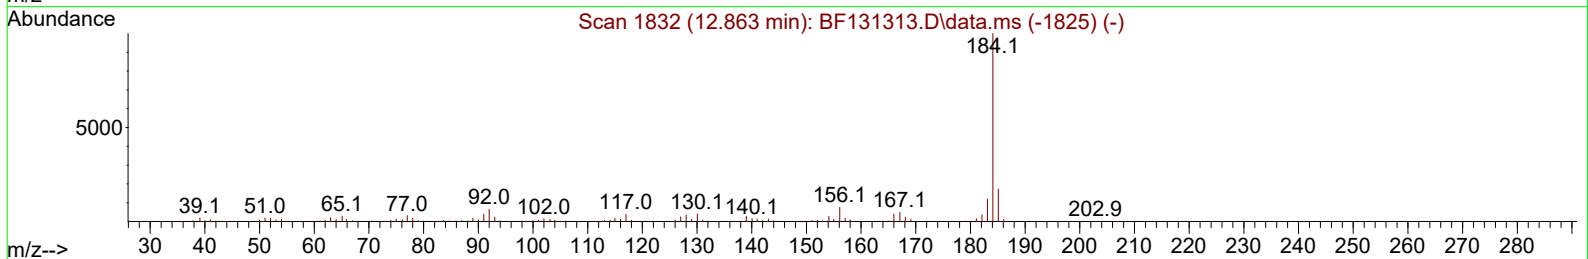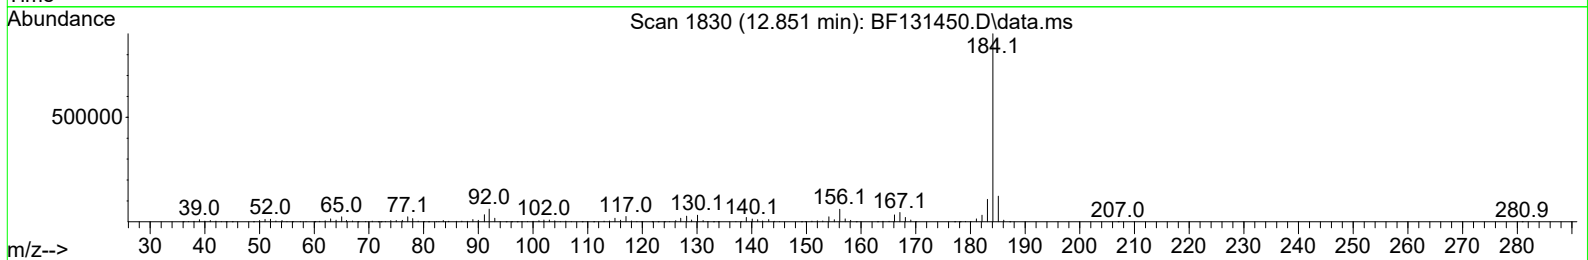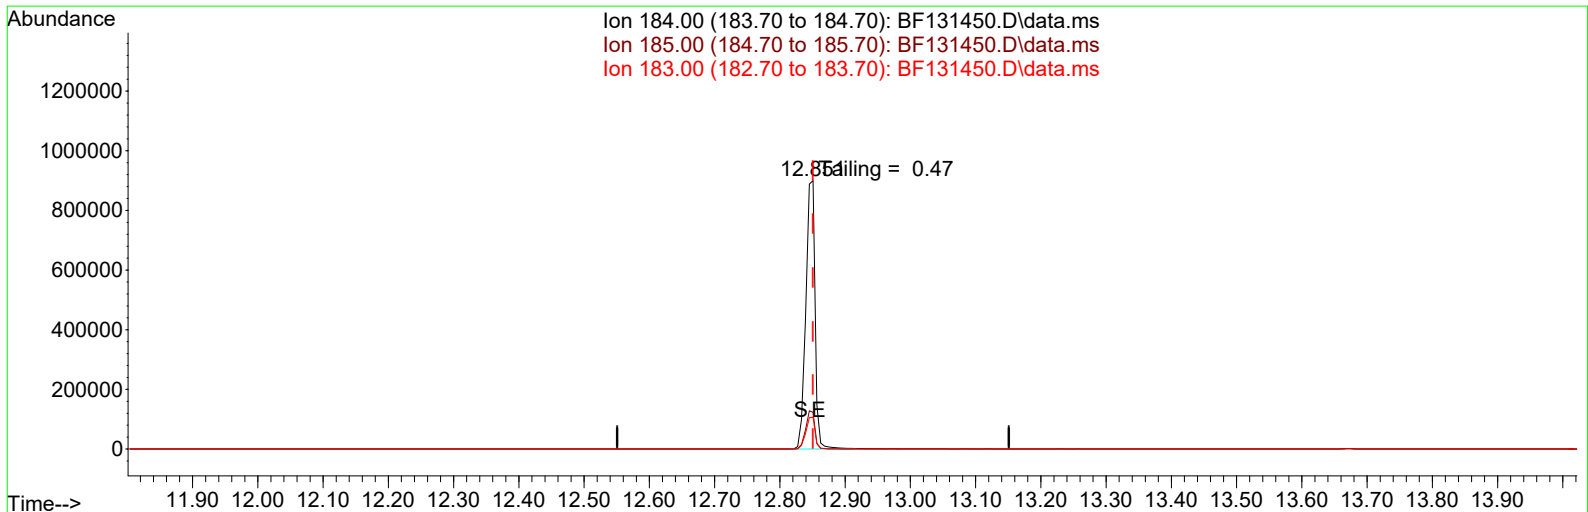

TIC: BF131450.D\data.ms

(77) Benzidine

12.851min (-0.000) 0.00 ng

response 898972

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	13.65#
183.00	12.00	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/29/2022	BNA_F	<u>BF131450.D</u>
Compound Name	Response	Retention Time
DDT	406650	13.674
DDD	10442	13.368
DDE	875	13.027
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11317	417967	2.71

Instrument :
BNA_F
ClientSampleId :
DFTPP