
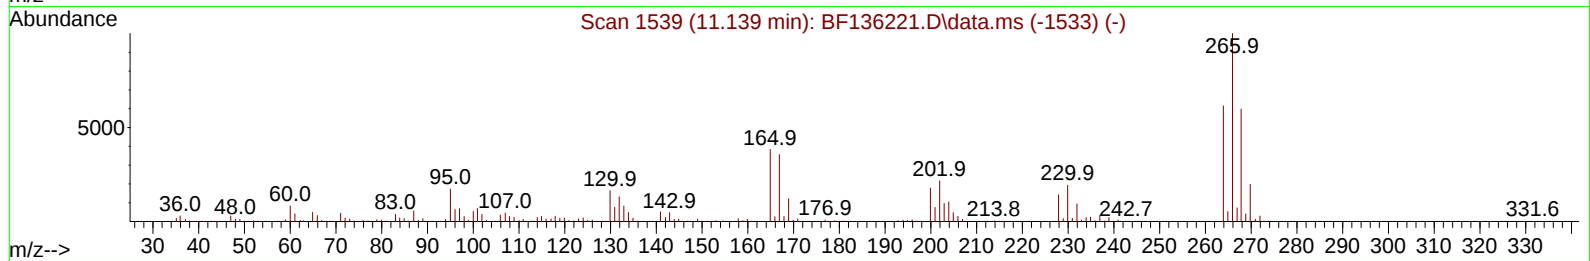
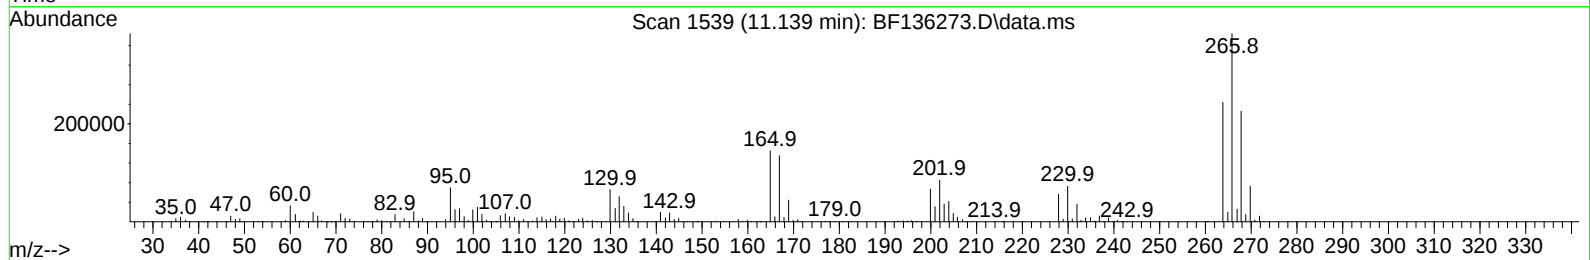


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136273.D
Acq On : 29 Nov 2023 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 11:37:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

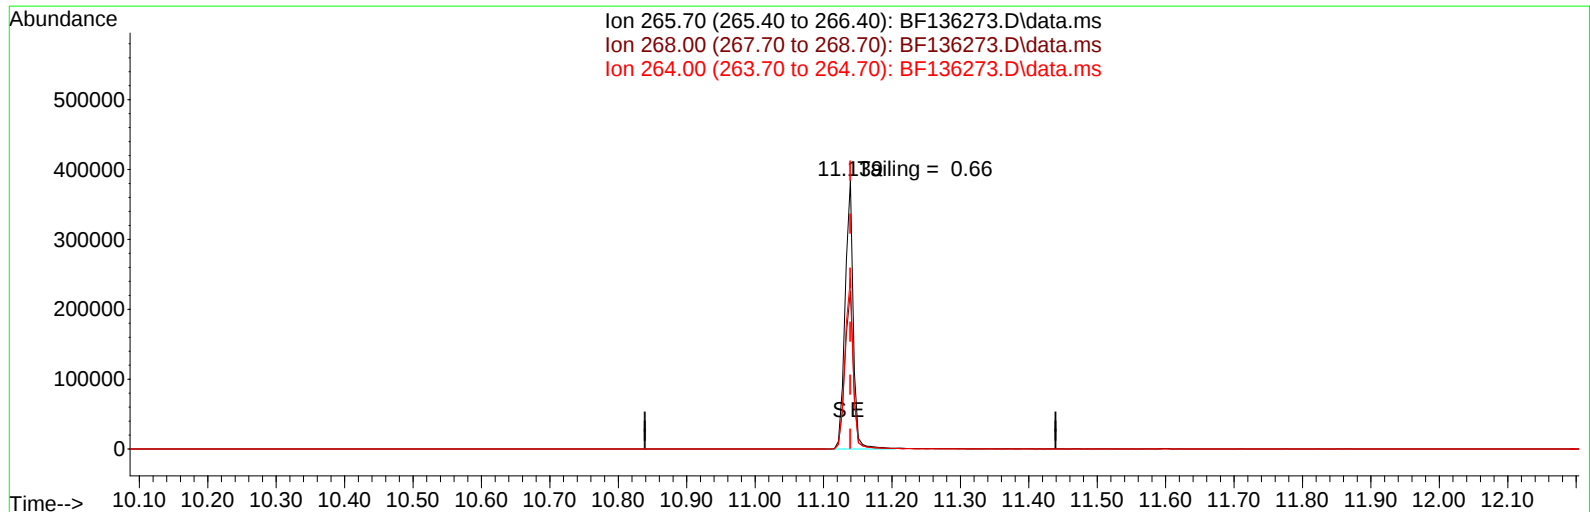

TIC: BF136273.D\data.ms

(70) Pentachlorophenol (C)




11.139min (+ 0.000) 91611.79 ng

response 319543

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	58.83
264.00	61.40	63.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136273.D
Acq On : 29 Nov 2023 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 11:37:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

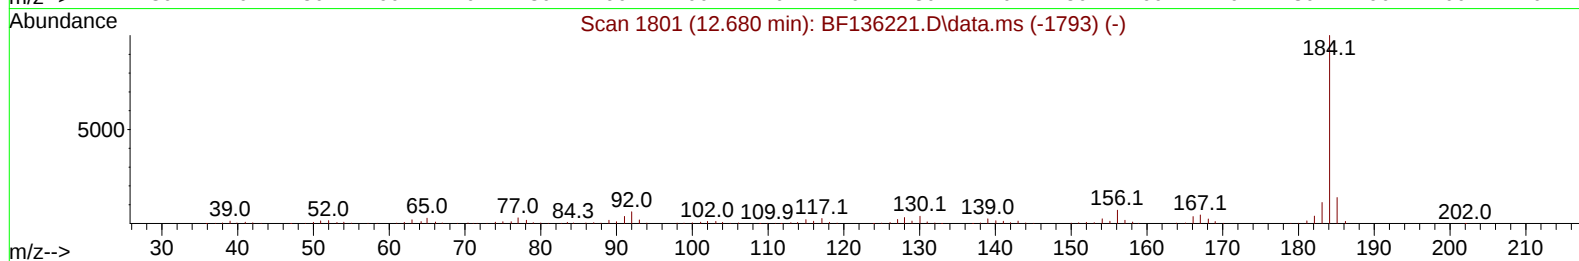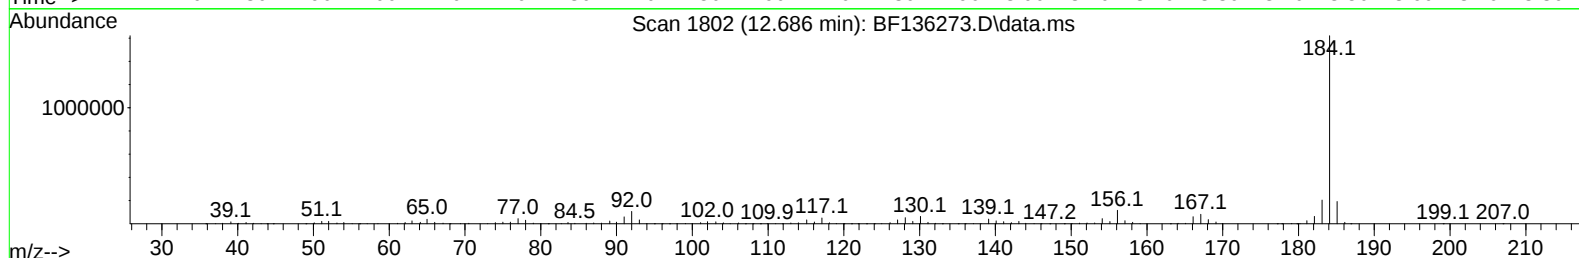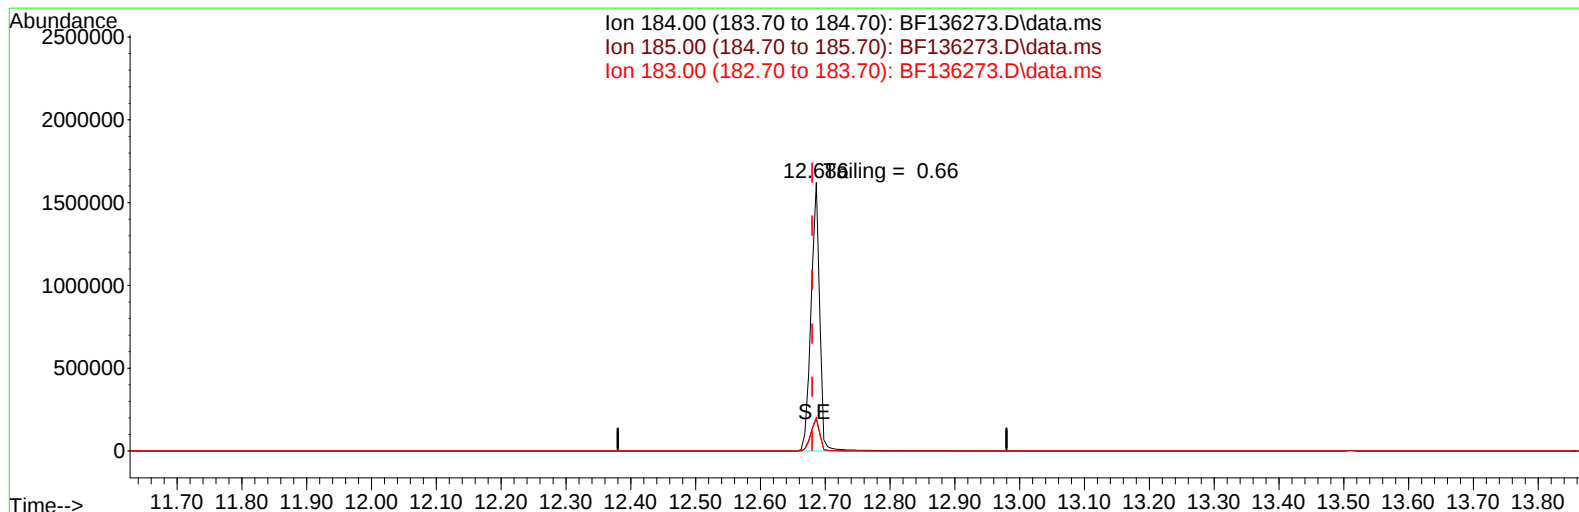

TIC: BF136273.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 163648.17 ng

response 1506451

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	11.85
183.00	11.20	12.63
0.00	0.00	0.00