

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136275.D
Acq On : 29 Nov 2023 10:42
Operator : CG\JU
Sample : PB156824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156824BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.187	12	17	22	rVB	75429	102431	1.45%	0.273%
2	5.457	567	573	576	rBV	4948772	5001849	70.57%	13.310%
3	6.446	734	741	744	rBV	4199958	4903006	69.17%	13.047%
4	6.804	798	802	805	rBV	1192997	897751	12.67%	2.389%
5	7.369	891	898	901	rBV	2993195	3118791	44.00%	8.299%
6	8.081	1014	1019	1022	rBV	1411870	1239215	17.48%	3.297%
7	9.163	1197	1203	1206	rBV	6752611	6571426	92.71%	17.486%
8	9.839	1312	1318	1321	rBV	1824136	1455005	20.53%	3.872%
9	10.634	1445	1453	1456	rBV	3897885	3839702	54.17%	10.217%
10	11.333	1568	1572	1575	rBV	1841031	1525771	21.53%	4.060%
11	12.939	1839	1845	1847	rBV	6901813	7088124	100.00%	18.861%
12	13.986	2018	2023	2034	rBV	1257461	1123606	15.85%	2.990%
13	15.468	2270	2275	2281	rBV	580221	714266	10.08%	1.901%




Sum of corrected areas: 37580943

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136275.D
Acq On : 29 Nov 2023 10:42
Operator : CG\JU
Sample : PB156824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156824BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

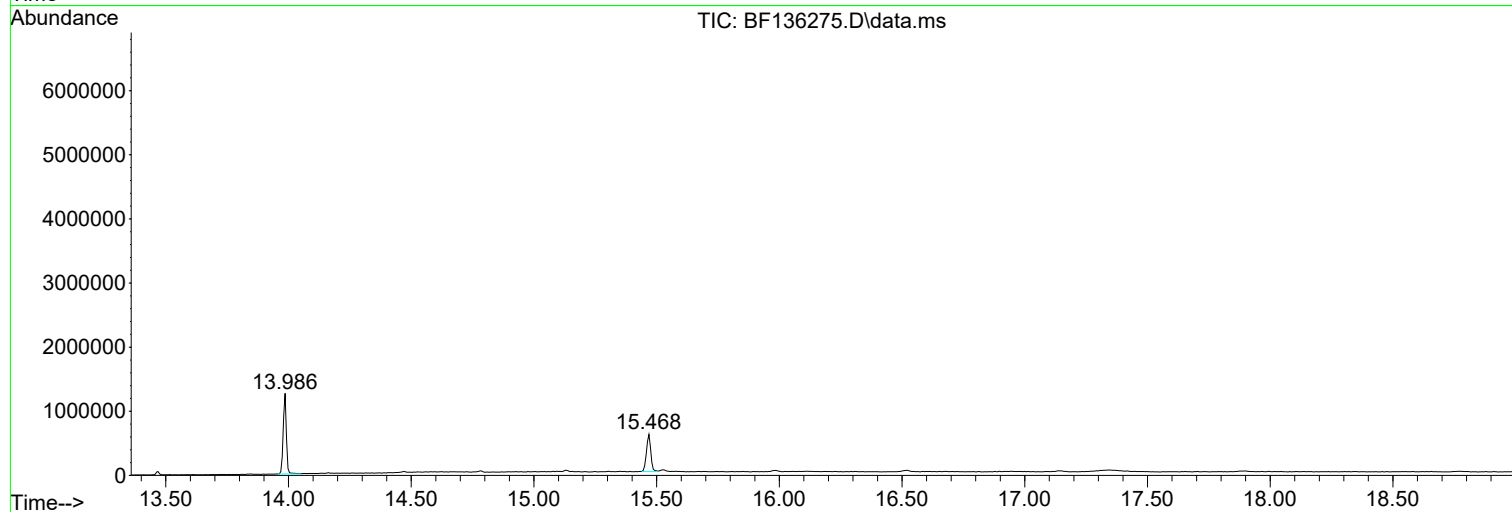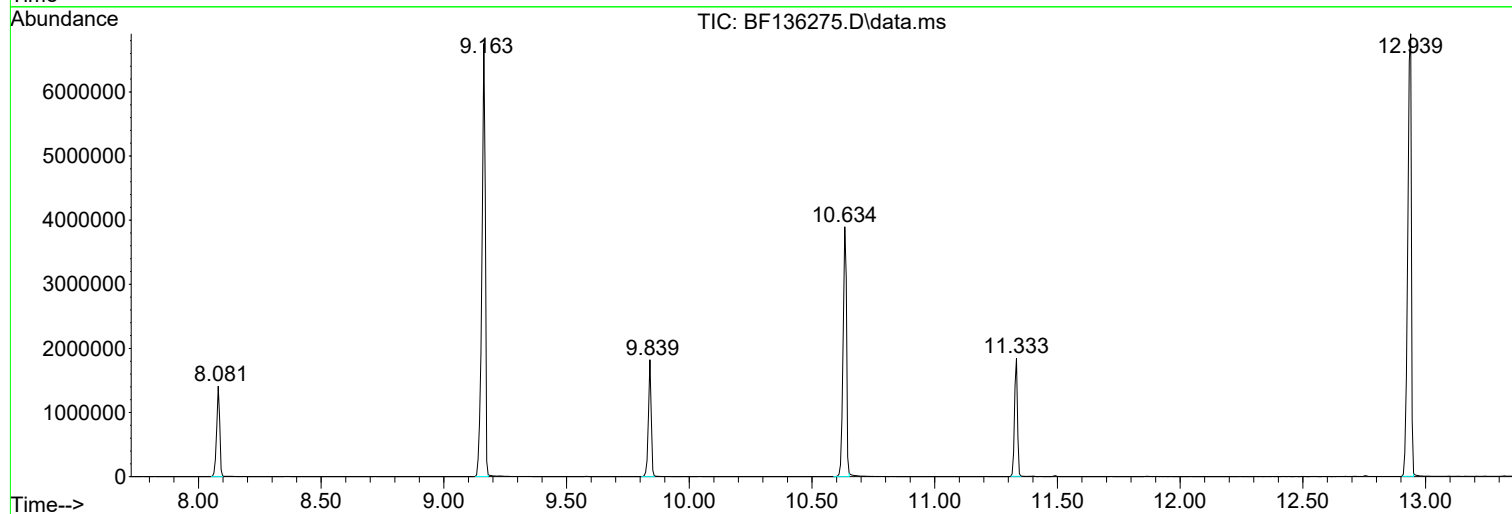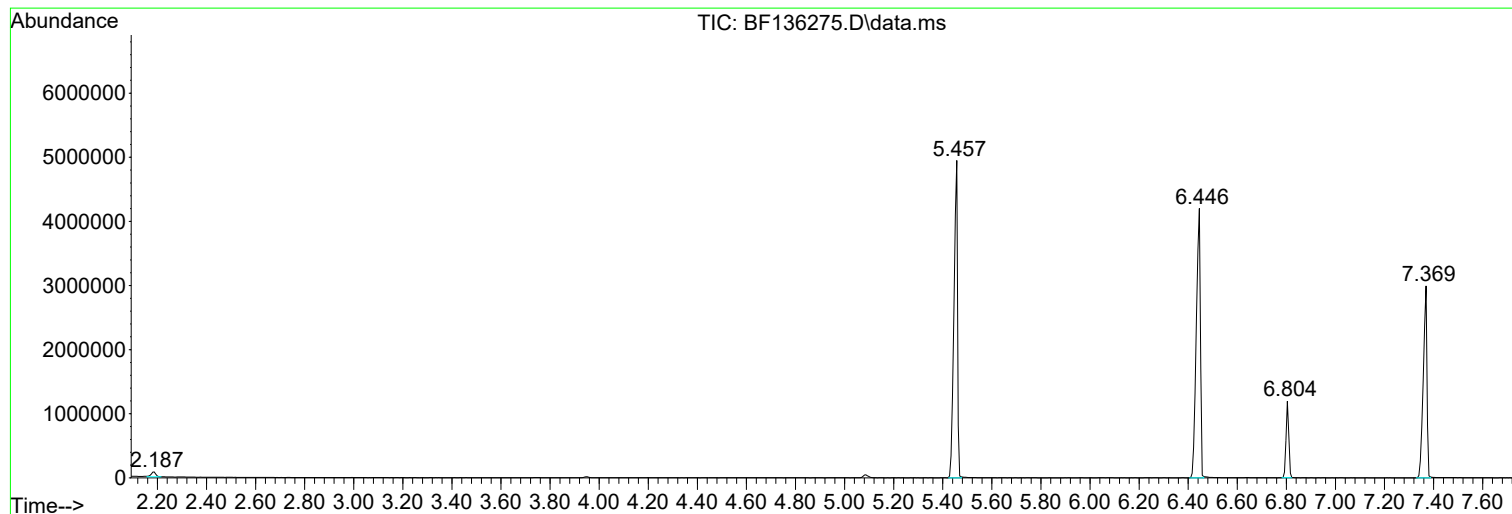

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136275.D
Acq On : 29 Nov 2023 10:42
Operator : CG\JU
Sample : PB156824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156824BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.187	2.28 ng	102431	1,4-Dichlorobenzene-d4	6.804

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	38
4			2,5-Dimethyl-4-hydroxy-3-hexanone	144	C8H16O2	000815-77-0	37
5			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	37

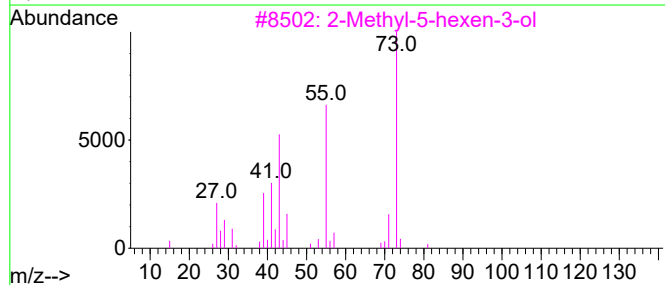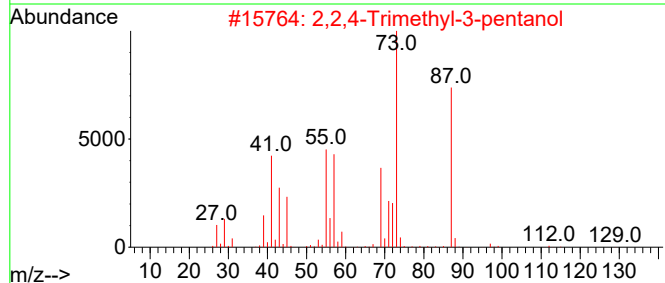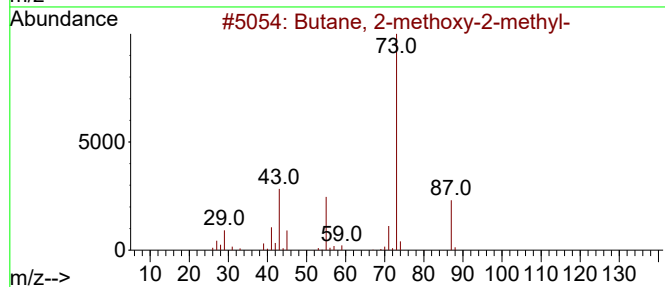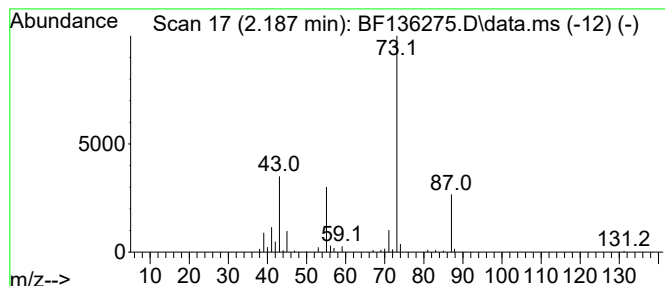

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136275.D
Acq On : 29 Nov 2023 10:42
Operator : CG\JU
Sample : PB156824BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156824BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.187	2.3	ng	102431	1	6.804	897751	20.0