

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
 Data File : BF136277.D
 Acq On : 29 Nov 2023 11:46
 Operator : CG\JU
 Sample : PB157393BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157393BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.175	10	15	20	rVB	72373	99905	1.51%	0.283%
2	5.451	566	572	575	rBV	4254561	4743008	71.67%	13.428%
3	6.445	734	741	744	rBV	4235337	4603703	69.56%	13.033%
4	6.804	798	802	805	rBV	1150412	847311	12.80%	2.399%
5	7.369	891	898	901	rBV	2840496	2974712	44.95%	8.422%
6	8.080	1014	1019	1022	rBV	1380330	1171840	17.71%	3.318%
7	9.163	1197	1203	1206	rBV	6763033	6192382	93.56%	17.531%
8	9.839	1312	1318	1321	rBV	1658144	1391456	21.02%	3.939%
9	10.633	1446	1453	1456	rBV	3862781	3650155	55.15%	10.334%
10	11.333	1568	1572	1575	rBV	1614688	1437504	21.72%	4.070%
11	12.933	1839	1844	1847	rBV	6683002	6618269	100.00%	18.737%
12	13.980	2018	2022	2030	rBV	974184	964016	14.57%	2.729%
13	15.468	2269	2275	2281	rBV	478493	628415	9.50%	1.779%




Sum of corrected areas: 35322676

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136277.D
Acq On : 29 Nov 2023 11:46
Operator : CG\JU
Sample : PB157393BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157393BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

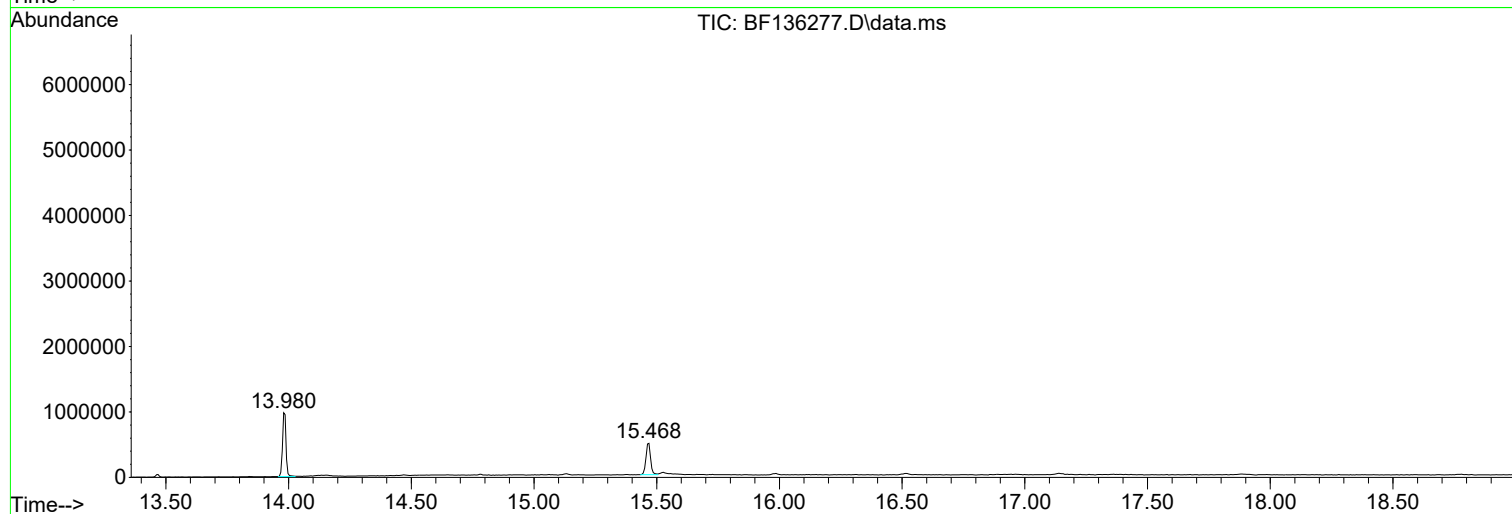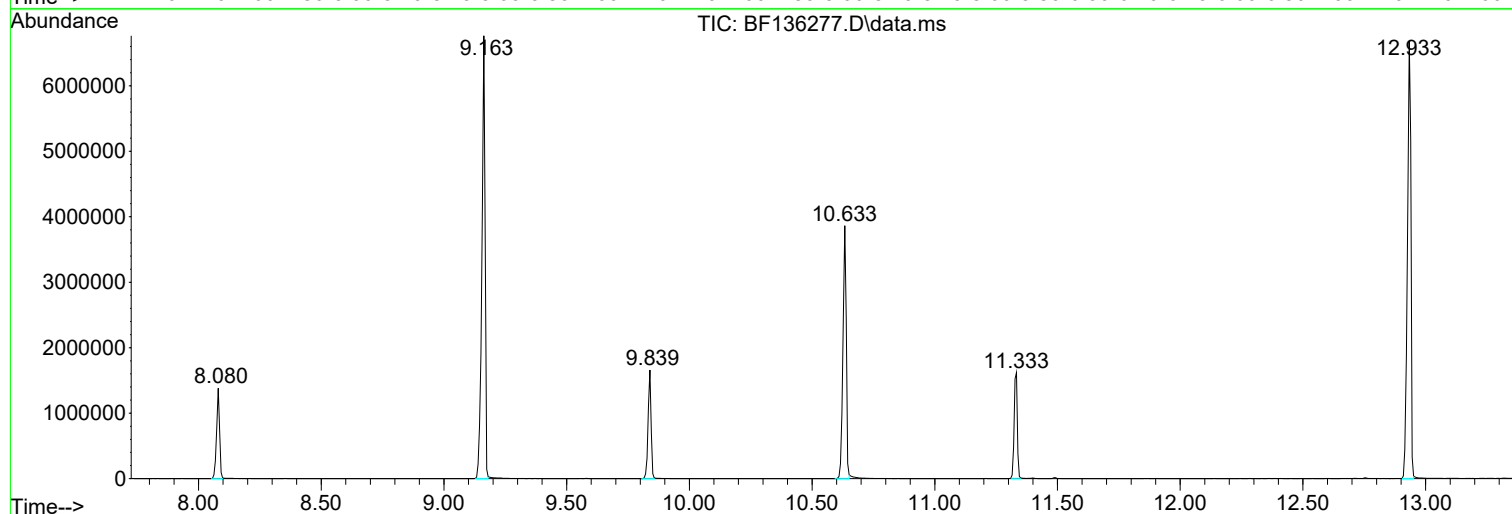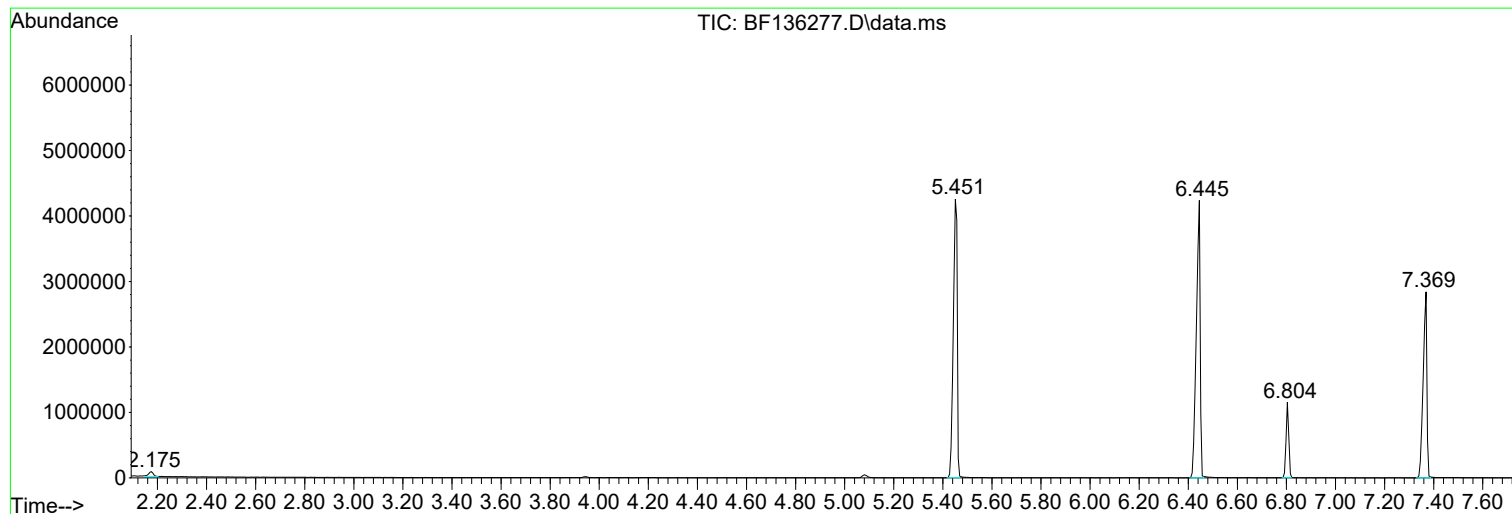

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136277.D
Acq On : 29 Nov 2023 11:46
Operator : CG\JU
Sample : PB157393BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157393BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.175	2.36 ng	99905	1,4-Dichlorobenzene-d4	6.804

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
2			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23
3			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	23
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

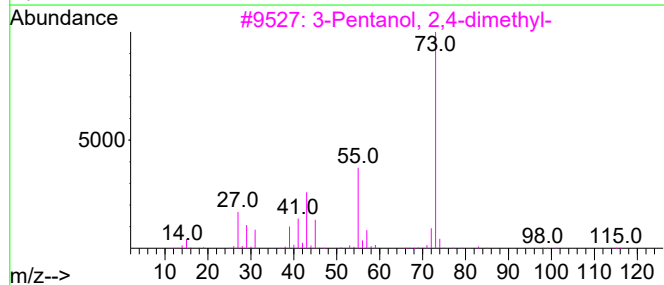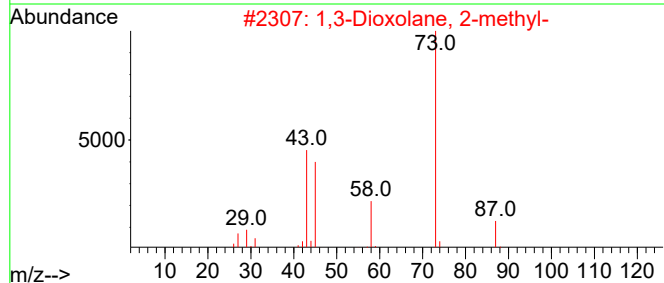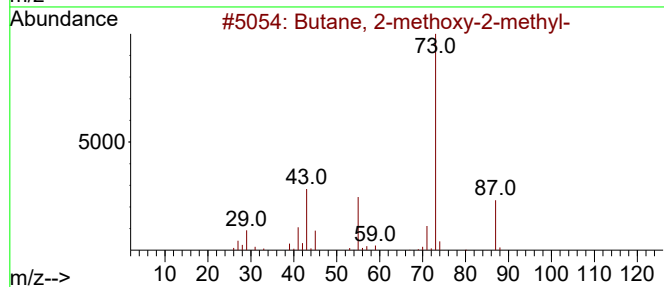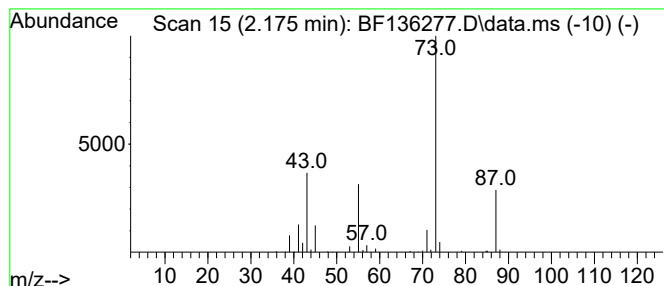

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136277.D
Acq On : 29 Nov 2023 11:46
Operator : CG\JU
Sample : PB157393BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157393BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.175	2.4	ng	99905	1	6.804	847311	20.0