

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
 Data File : BF136279.D
 Acq On : 29 Nov 2023 12:49
 Operator : CG\JU
 Sample : PB157160BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157160BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136279.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.175	11	15	20	rVB	75906	98819	1.50%	0.280%
2	5.451	567	572	575	rBV	4219000	4759083	72.05%	13.470%
3	6.446	734	741	744	rBV	4210909	4619346	69.94%	13.075%
4	6.804	798	802	805	rBV	1141628	844404	12.78%	2.390%
5	7.369	891	898	901	rBV	2839582	3000125	45.42%	8.492%
6	8.081	1014	1019	1022	rBV	1352413	1160395	17.57%	3.284%
7	9.163	1197	1203	1206	rBV	6756584	6206076	93.96%	17.566%
8	9.839	1312	1318	1321	rBV	1707878	1395339	21.13%	3.949%
9	10.633	1446	1453	1456	rBV	3898126	3572550	54.09%	10.112%
10	11.328	1567	1571	1575	rBV	1648761	1466589	22.20%	4.151%
11	12.933	1839	1844	1847	rBV	6894008	6605037	100.00%	18.695%
12	13.980	2018	2022	2032	rBV	1021188	959118	14.52%	2.715%
13	15.468	2269	2275	2281	rBV	478394	643440	9.74%	1.821%




Sum of corrected areas: 35330321

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136279.D
Acq On : 29 Nov 2023 12:49
Operator : CG\JU
Sample : PB157160BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157160BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

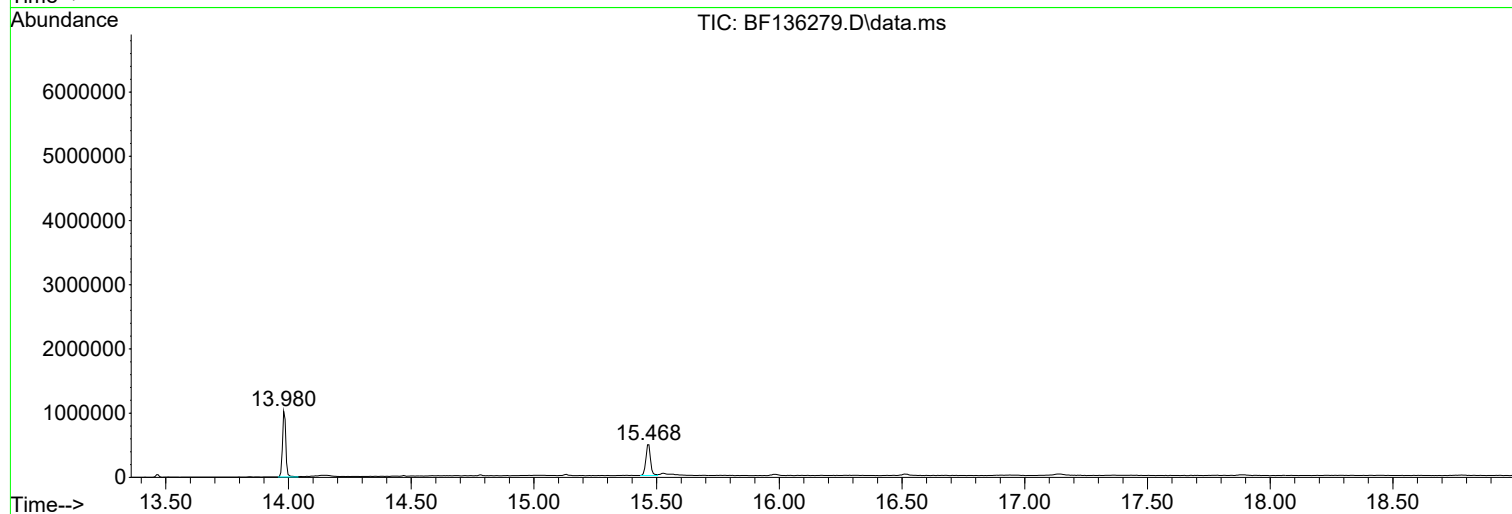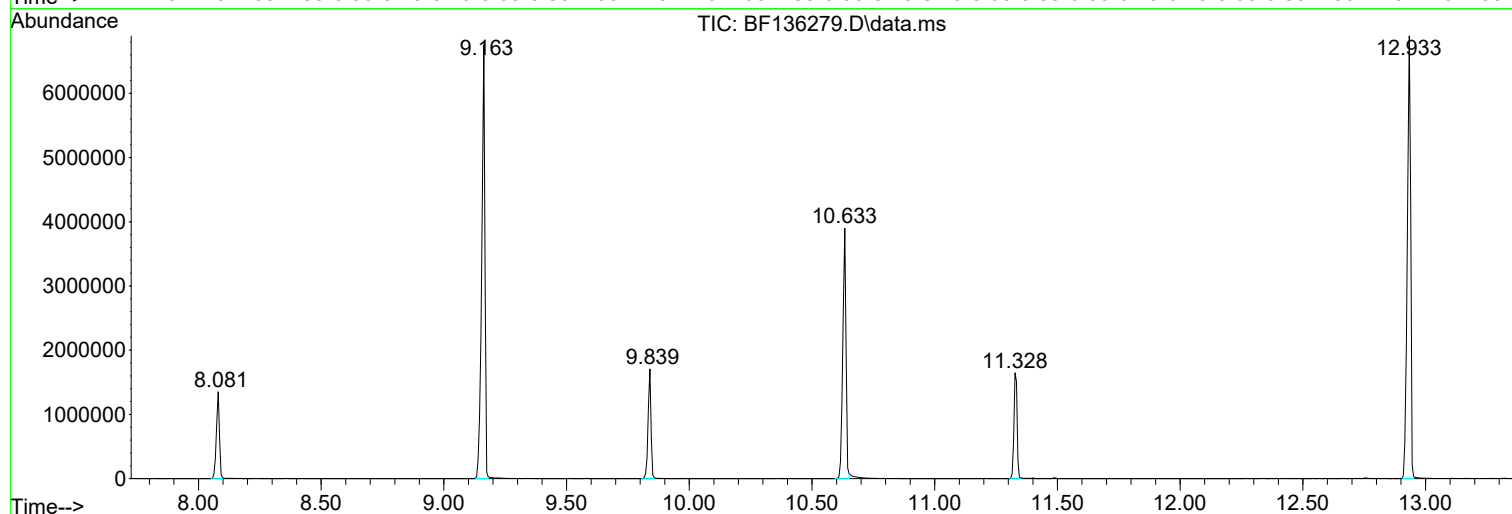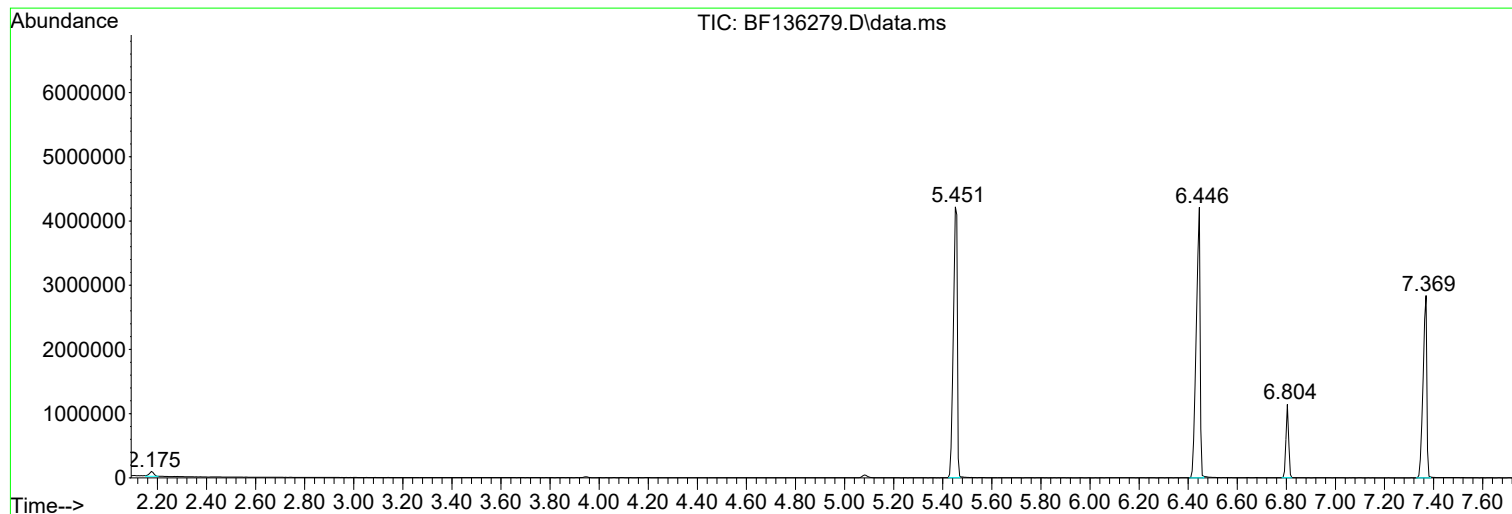

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136279.D
Acq On : 29 Nov 2023 12:49
Operator : CG\JU
Sample : PB157160BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157160BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.175	2.34 ng	98819	1,4-Dichlorobenzene-d4	6.804

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3		3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	12
4		Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	12
5		3-Methoxy-3-methylbutyl acetate	160	C8H16O3	1010430-01-2	12

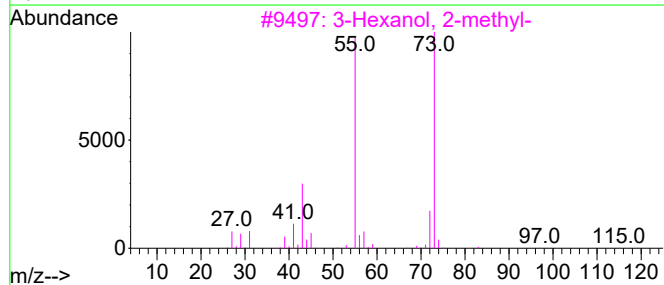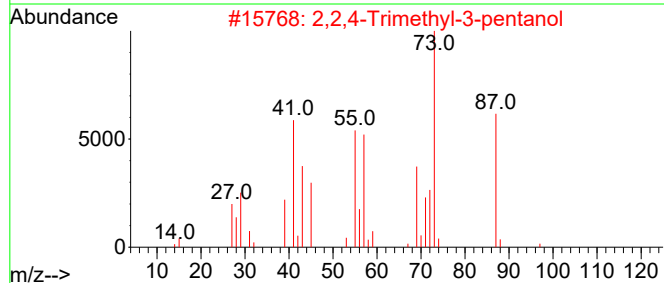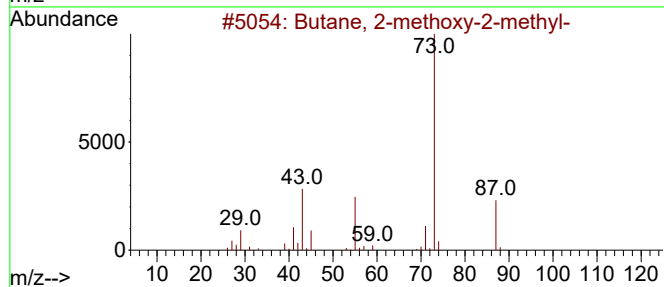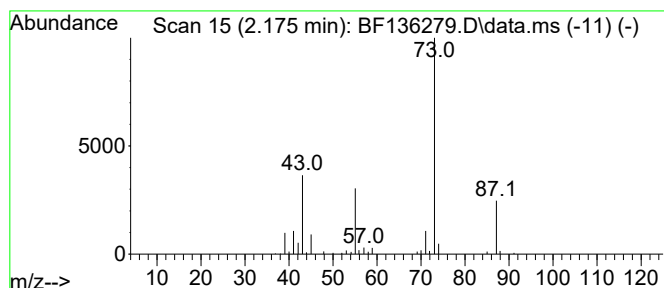

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136279.D
Acq On : 29 Nov 2023 12:49
Operator : CG\JU
Sample : PB157160BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157160BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.175	2.3	ng	98819	1	6.804	844404	20.0