

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136287.D
Acq On : 29 Nov 2023 17:04
Operator : CG\JU
Sample : PB157073BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157073BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.445	566	571	574	rBV	3038688	2757479	49.21%	10.195%
2	6.439	734	740	742	rBV	2557767	2712267	48.40%	10.027%
3	6.804	798	802	805	rBV	971948	759444	13.55%	2.808%
4	7.363	891	897	900	rBV	2456297	2720475	48.55%	10.058%
5	8.081	1014	1019	1022	rBV	1153614	1041908	18.59%	3.852%
6	9.163	1196	1203	1206	rBV	6303994	5603377	100.00%	20.716%
7	9.839	1312	1318	1321	rBV	1420593	1243410	22.19%	4.597%
8	10.627	1448	1452	1455	rBV	2340910	2027635	36.19%	7.496%
9	11.327	1567	1571	1575	rBV	1615503	1291366	23.05%	4.774%
10	12.933	1839	1844	1847	rBV	5777439	5582967	99.64%	20.641%
11	13.980	2018	2022	2032	rBV	830381	727634	12.99%	2.690%
12	15.462	2268	2274	2283	rBV	445925	580358	10.36%	2.146%




Sum of corrected areas: 27048320

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136287.D
Acq On : 29 Nov 2023 17:04
Operator : CG\JU
Sample : PB157073BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157073BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

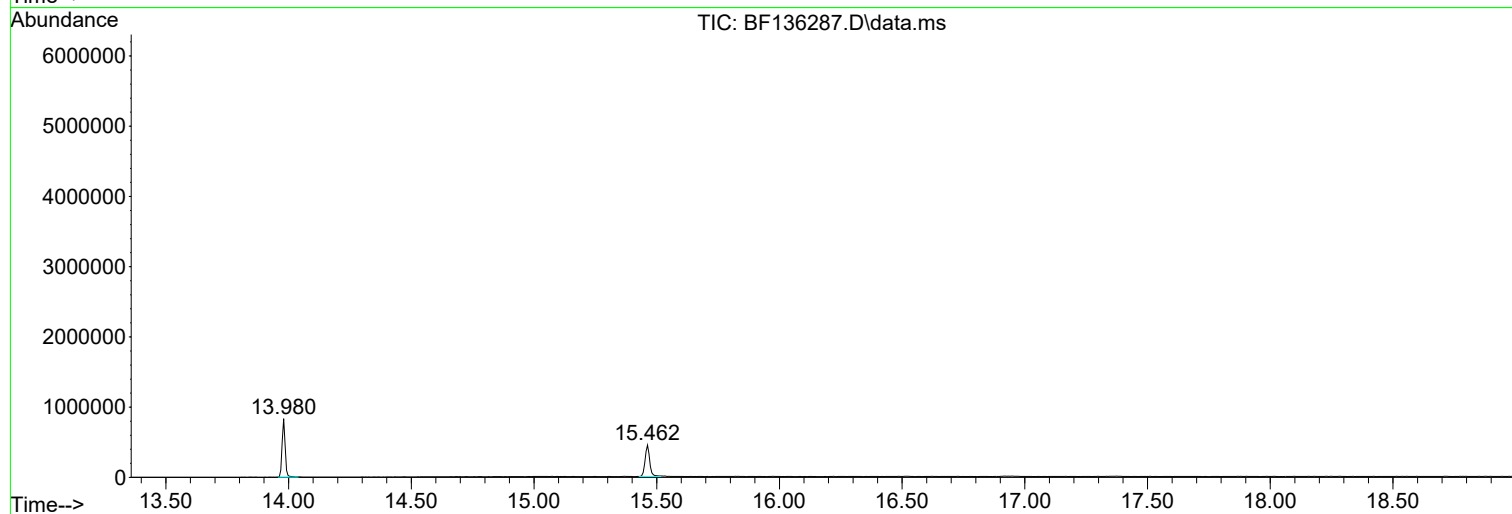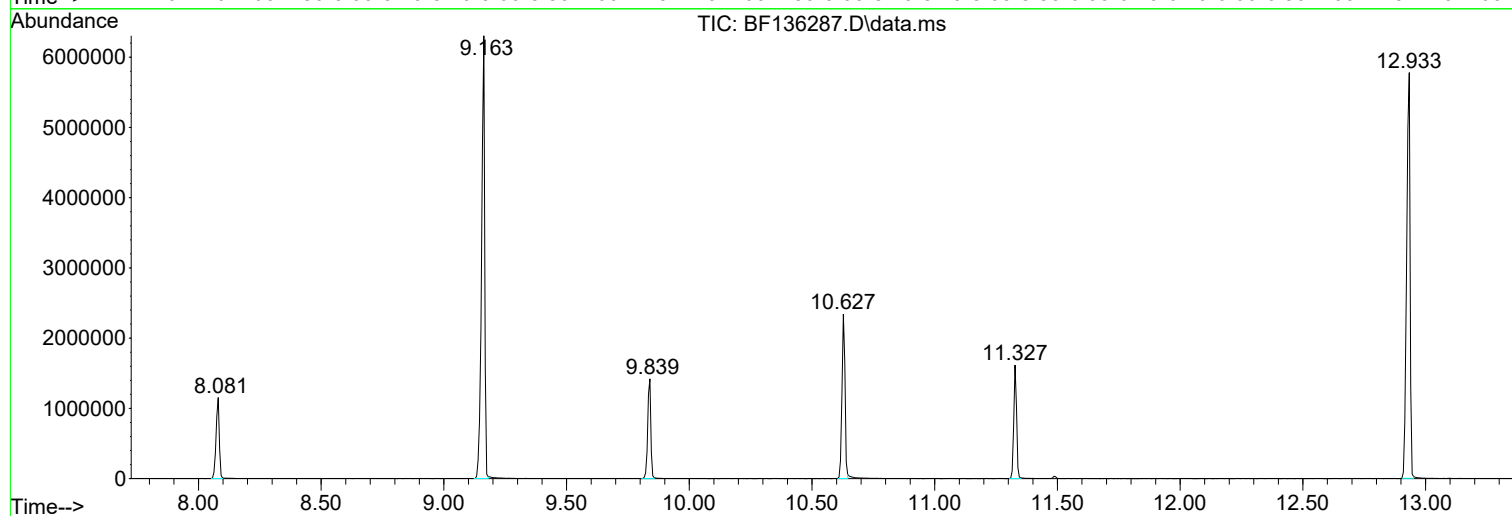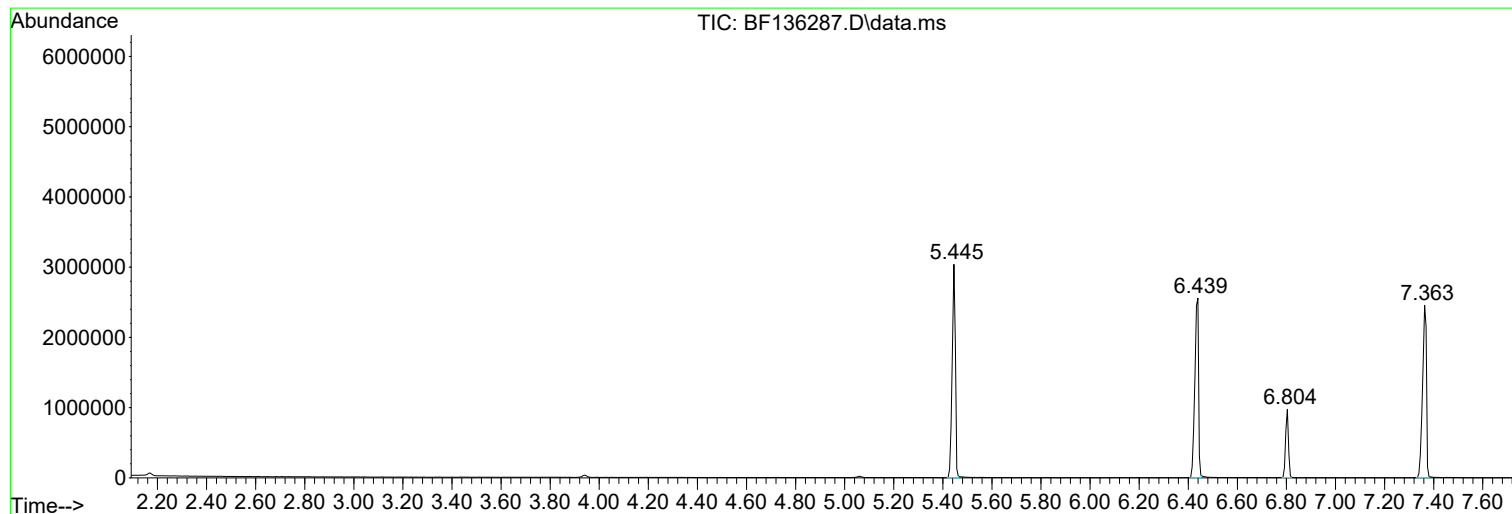

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136287.D
Acq On : 29 Nov 2023 17:04
Operator : CG\JU
Sample : PB157073BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157073BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136287.D
Acq On : 29 Nov 2023 17:04
Operator : CG\JU
Sample : PB157073BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157073BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------