
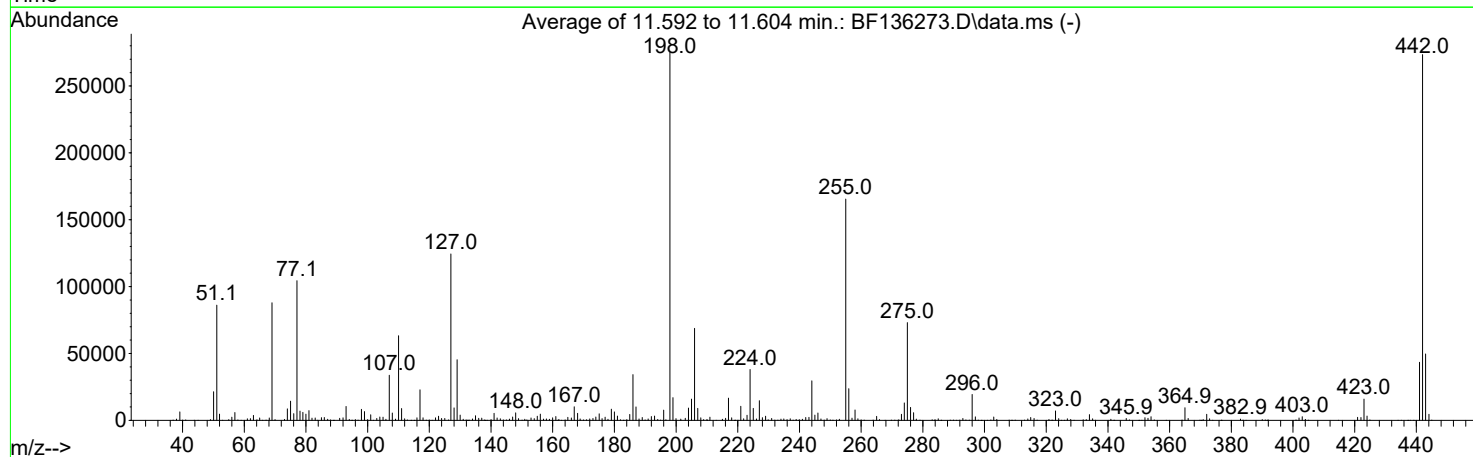


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136273.D
Acq On : 29 Nov 2023 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 28 03:04:20 2023

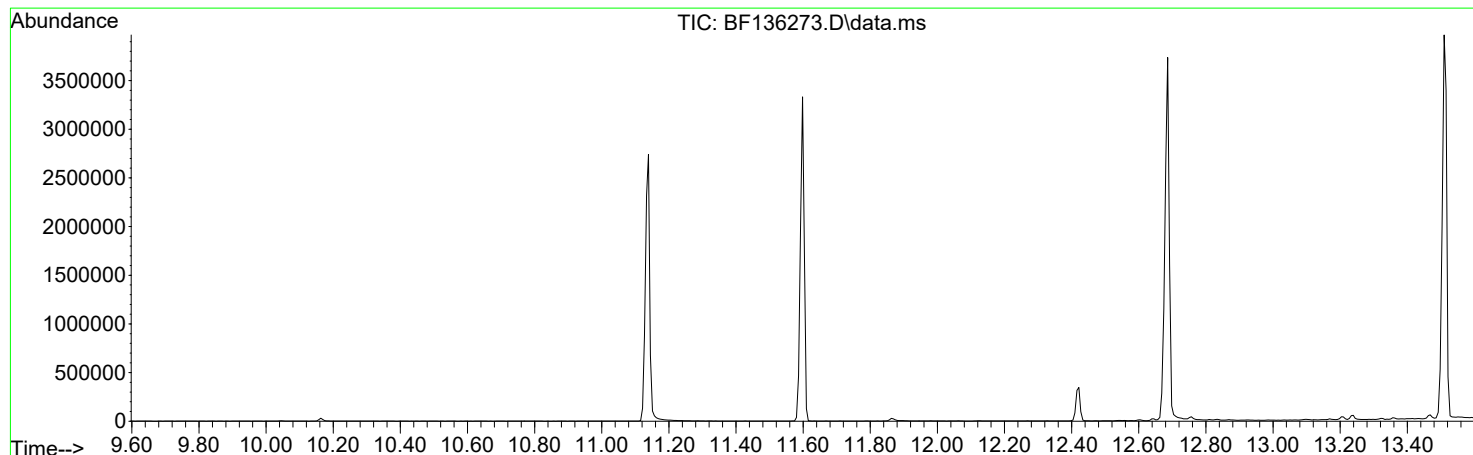

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	86152	PASS
68	69	0.00	2	2.0	1751	PASS
69	198	0.00	100	32.0	87981	PASS
70	69	0.00	2	0.7	644	PASS
127	198	10	80	45.3	124456	PASS
197	198	0.00	2	0.2	481	PASS
198	198	100	100	100.0	275029	PASS
199	198	5	9	6.2	16967	PASS
275	198	10	60	26.6	73117	PASS
365	198	1	100	3.5	9515	PASS
441	198	0.01	100	15.8	43387	PASS
442	442	50	100	100.0	273419	PASS
443	442	15	24	18.2	49640	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/29/2023	BNA_F	<u>BF136273.D</u>
Compound Name	Response	Retention Time
DDT	796946	13.51
DDD	12670	13.239
DDE	664	12.869
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13334	810280	1.65

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136273.D
Acq On : 29 Nov 2023 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 29 11:37:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

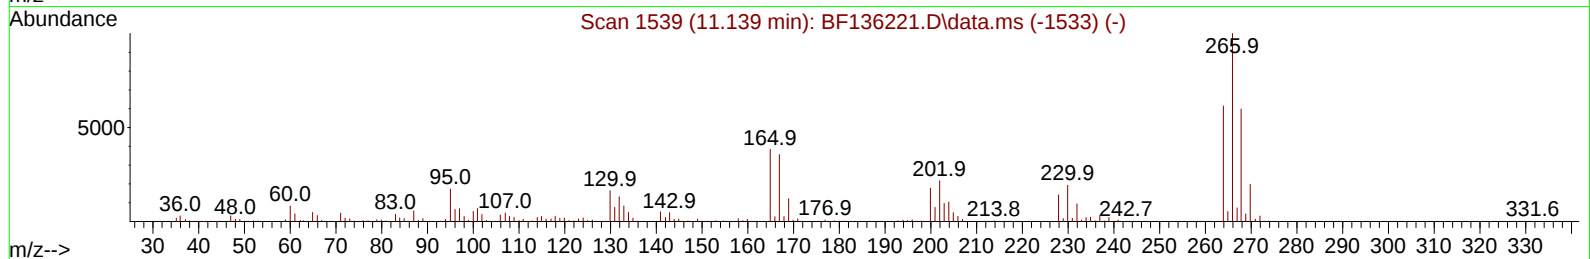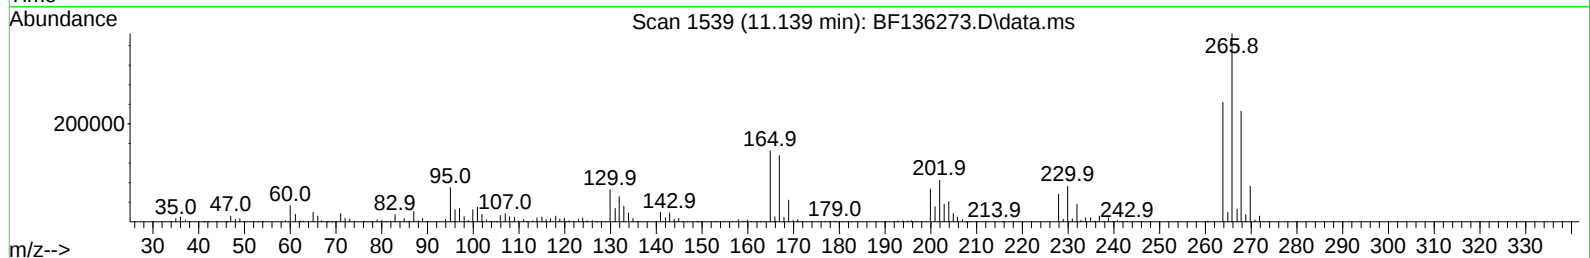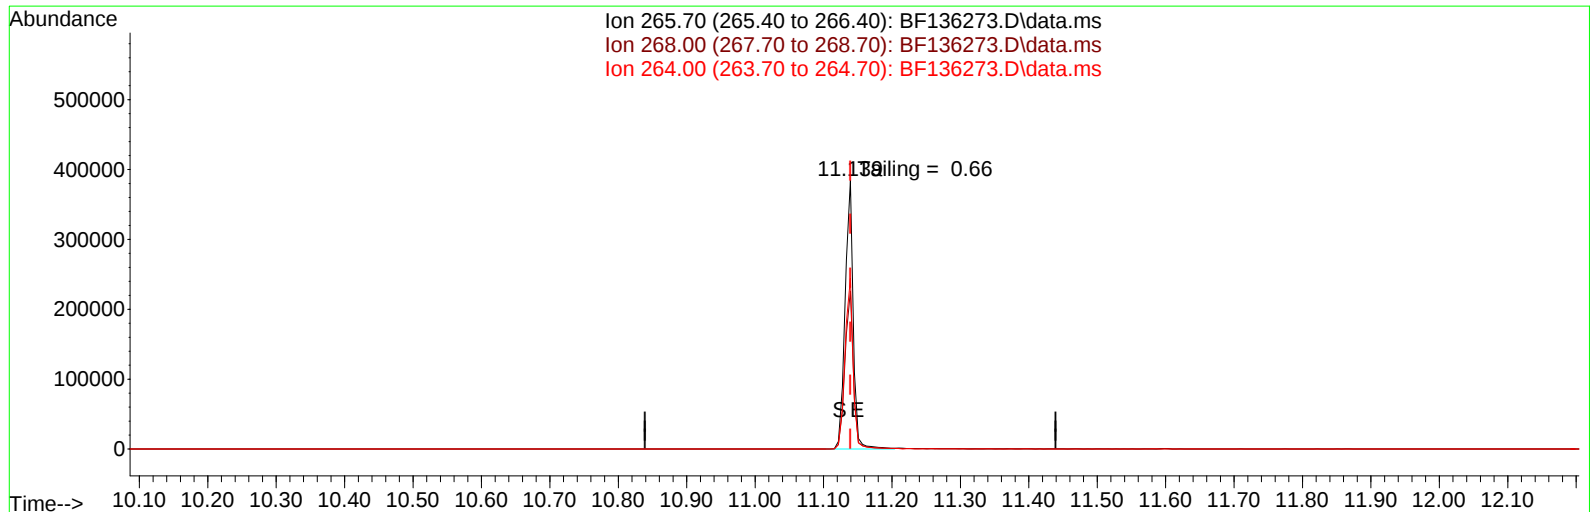

TIC: BF136273.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.000) 91611.79 ng

response 319543

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	58.83
264.00	61.40	63.50
0.00	0.00	0.00

