


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136282.D
Acq On : 29 Nov 2023 14:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 28 03:04:20 2023

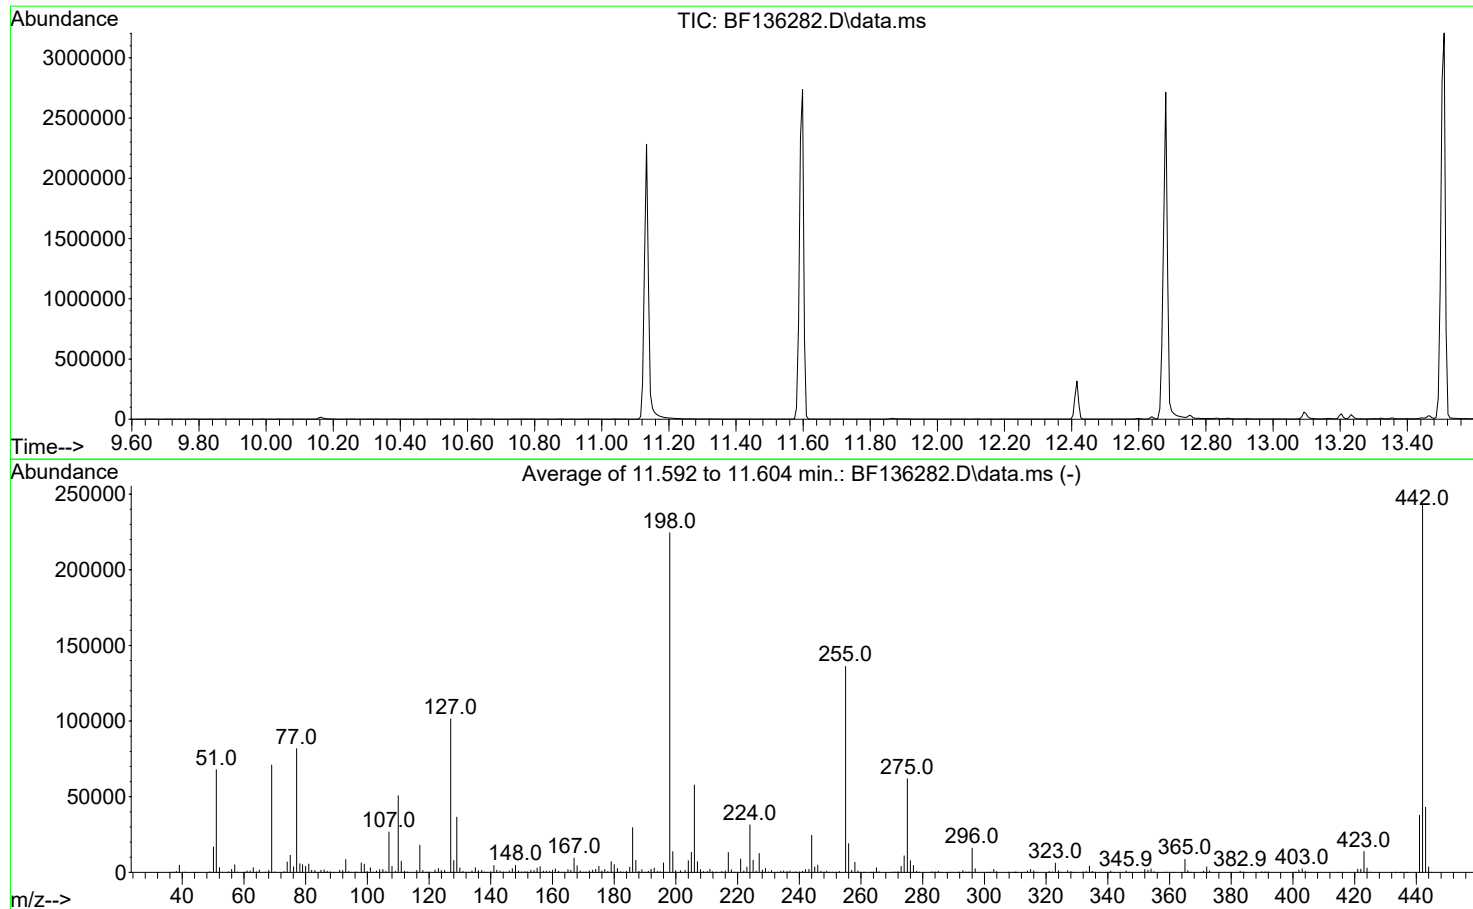

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	67899	PASS
68	69	0.00	2	1.9	1325	PASS
69	198	0.00	100	31.6	70959	PASS
70	69	0.00	2	0.5	351	PASS
127	198	10	80	45.2	101424	PASS
197	198	0.00	2	0.1	140	PASS
198	198	100	100	100.0	224387	PASS
199	198	5	9	6.1	13778	PASS
275	198	10	60	27.6	61853	PASS
365	198	1	100	3.8	8610	PASS
441	198	0.01	100	16.8	37776	PASS
442	442	50	100	100.0	243136	PASS
443	442	15	24	17.7	43059	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/29/2023	BNA_F	<u>BF136282.D</u>
Compound Name	Response	Retention Time
DDT	627833	13.51
DDD	12896	13.204
DDE	1039	12.869
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13935	641768	2.17

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
 Data File : BF136282.D
 Acq On : 29 Nov 2023 14:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 29 14:49:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 28 03:04:20 2023
 Response via : Initial Calibration

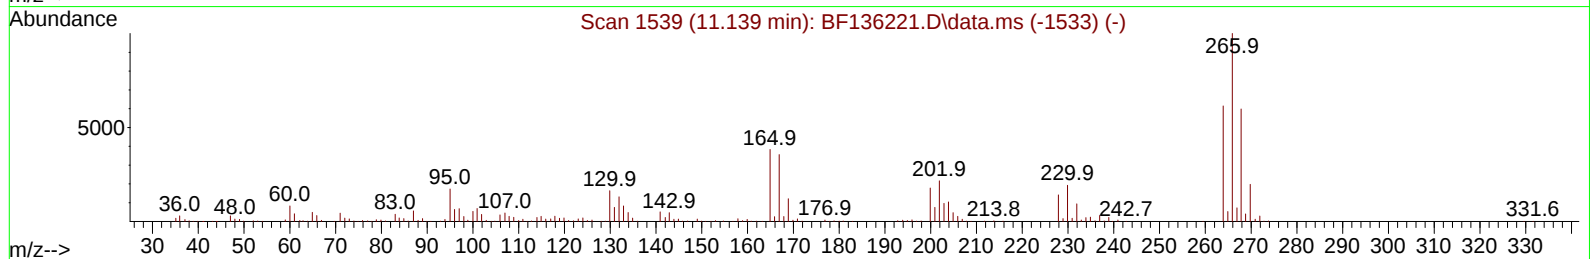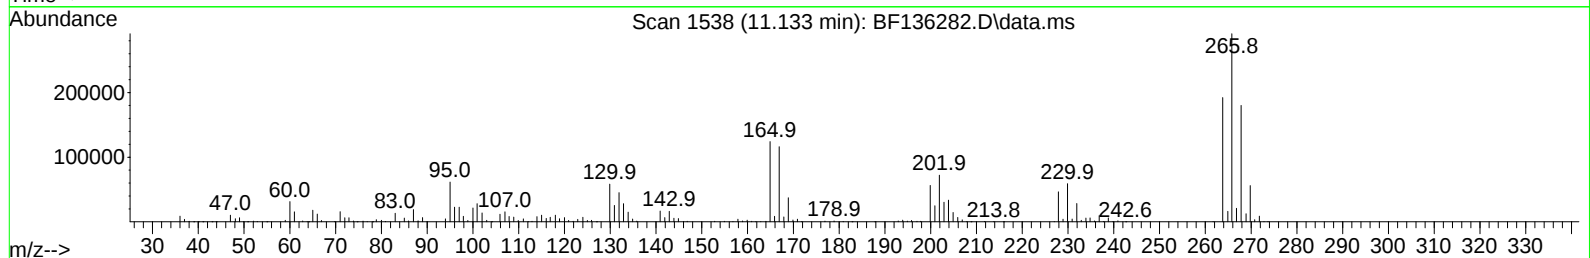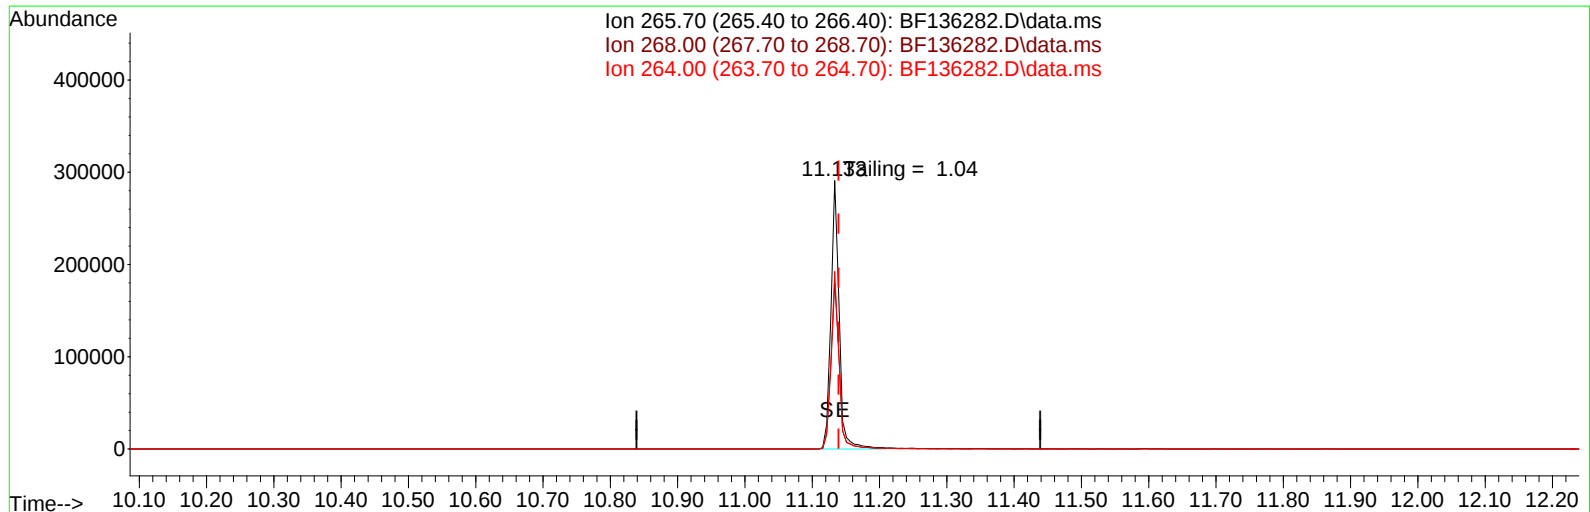

TIC: BF136282.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.006) 63080.57 ng




response 250839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	61.86
264.00	61.40	66.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112923\
Data File : BF136282.D
Acq On : 29 Nov 2023 14:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 29 14:49:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

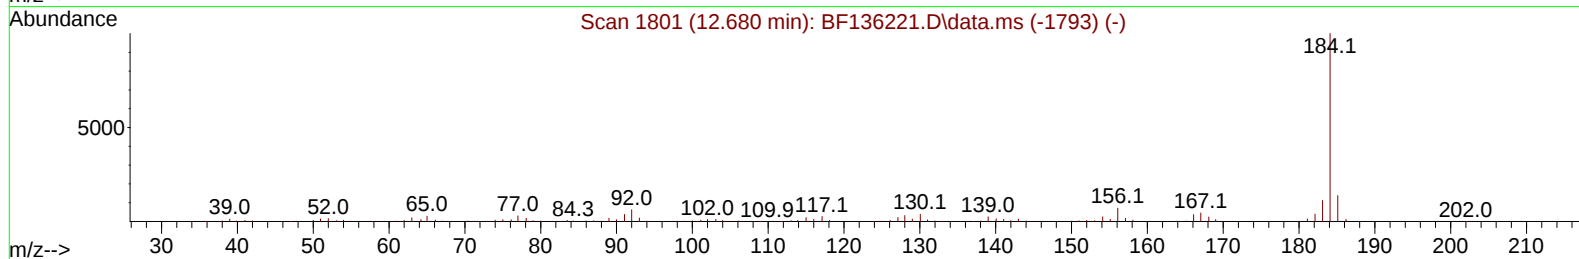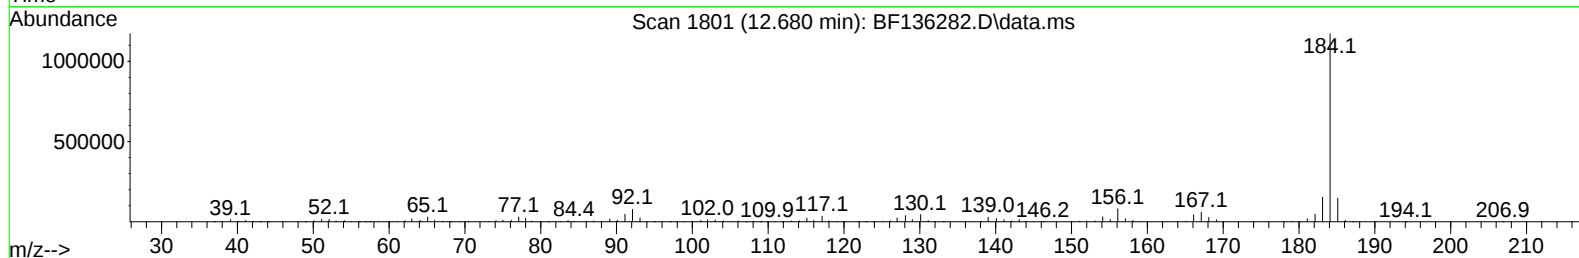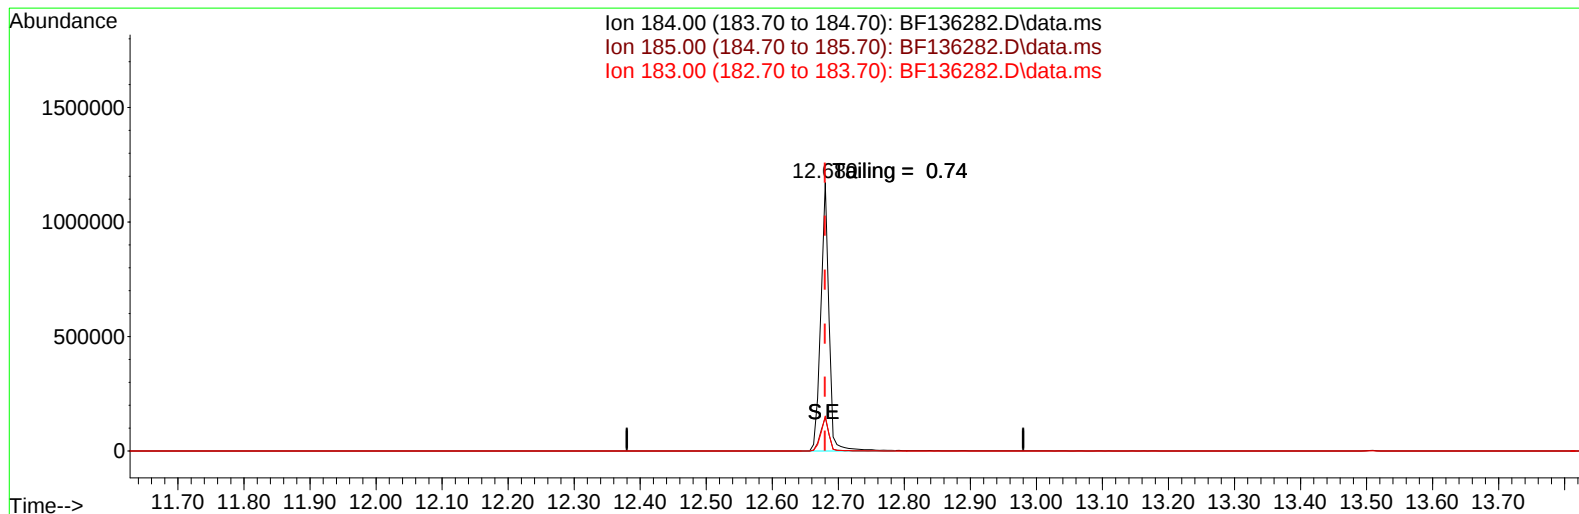

TIC: BF136282.D\data.ms

(77) Benzidine

12.680min (+ 0.000) 93245.01 ng

response 1022368

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	12.55
183.00	11.20	13.08
0.00	0.00	0.00