
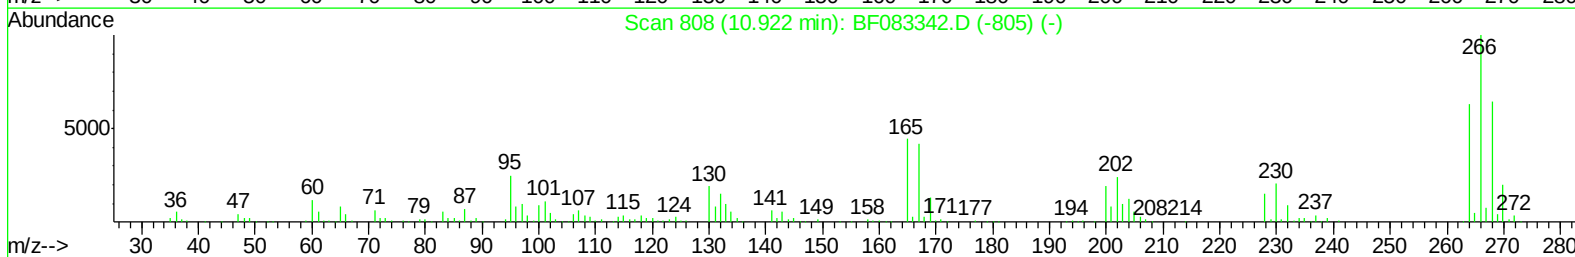
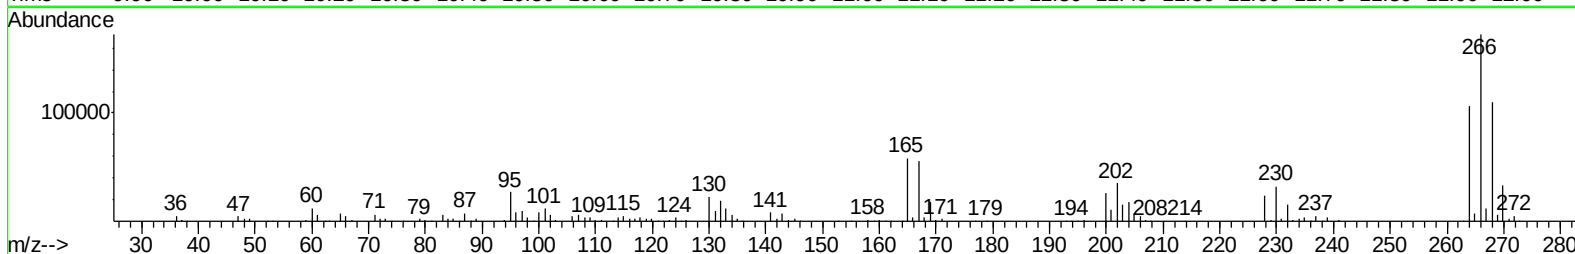


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF113015\
Data File : BF083338.D
Acq On : 30 Nov 2015 17:03
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 07:49:23 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 01 01:17:16 2015
Response via : Initial Calibration

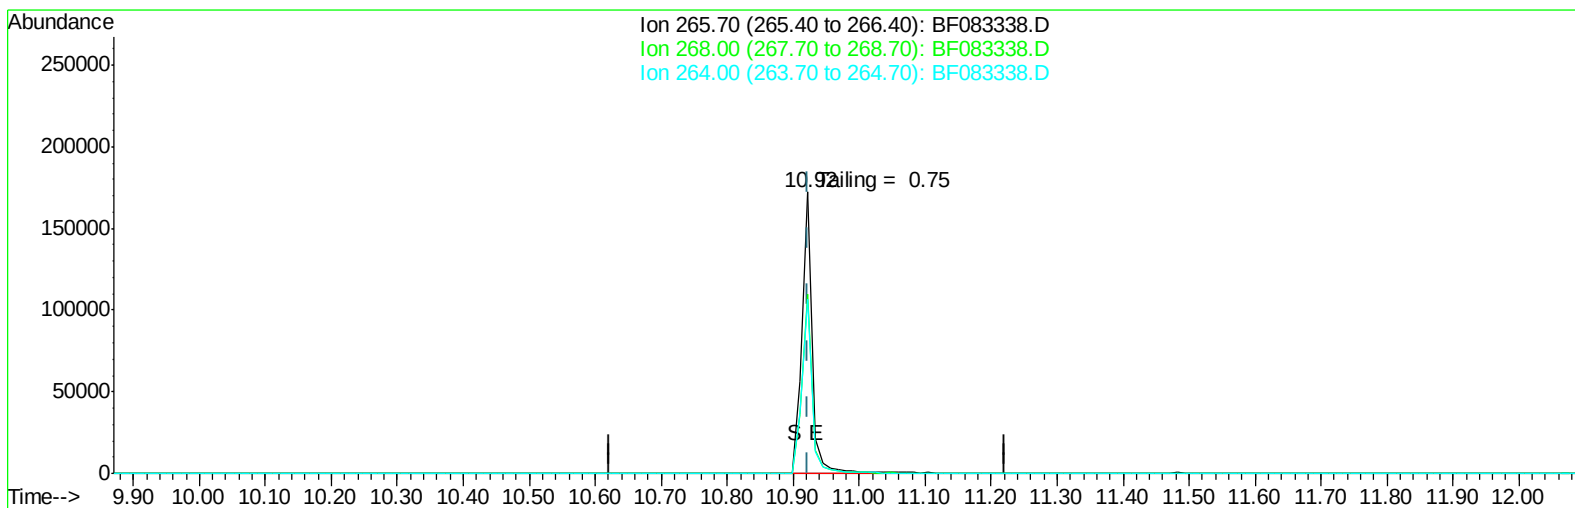

TIC: BF083338.D

(69) Pentachlorophenol (C)




10.922min (-0.000) 0.00ng

response 185290

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	63.78
264.00	63.00	61.82
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF113015\
Data File : BF083338.D
Acq On : 30 Nov 2015 17:03
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 07:49:23 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 01 01:17:16 2015
Response via : Initial Calibration

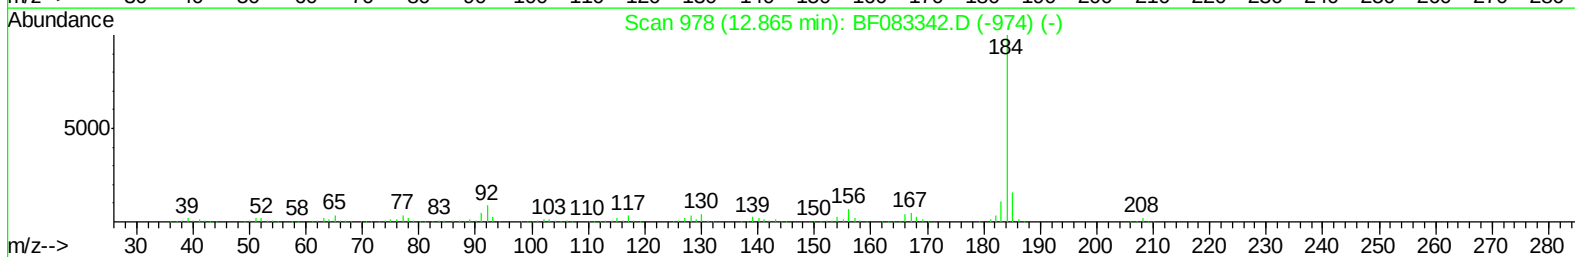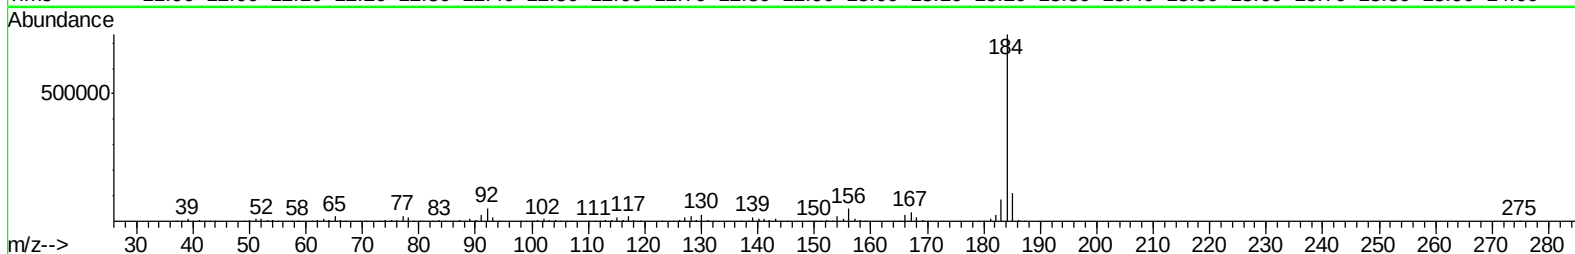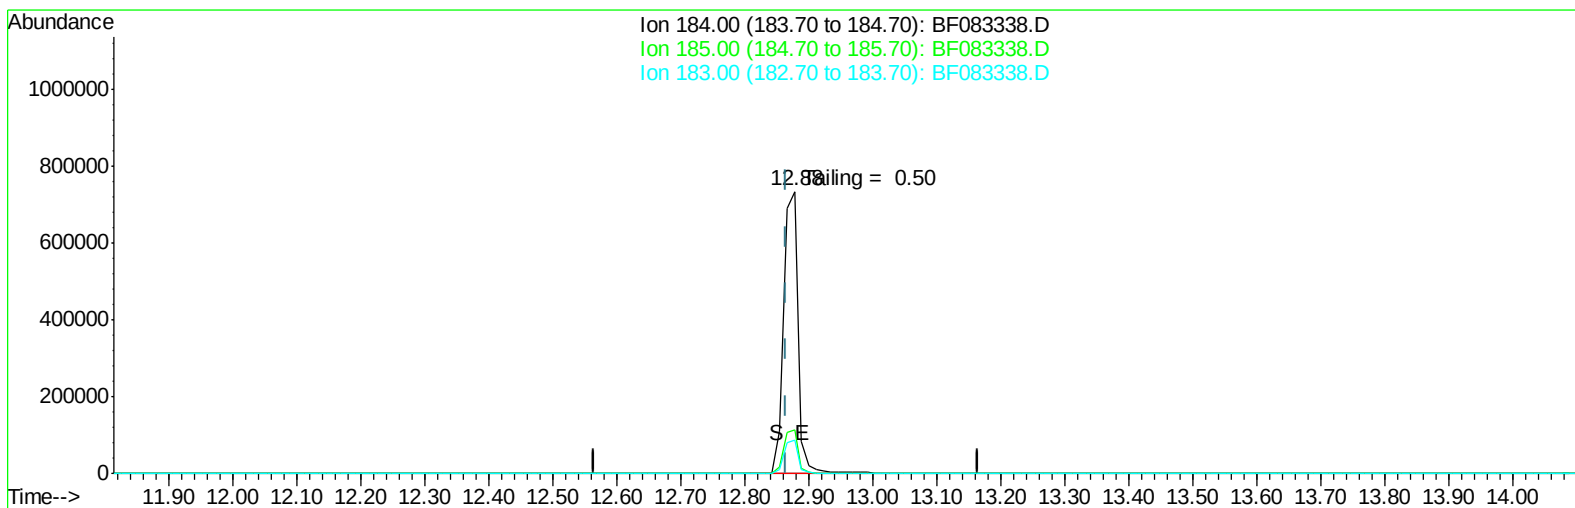

TIC: BF083338.D

(76) Benzidine

12.876min (+0.011) 167588.62ng

response 1158059

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	15.25
183.00	11.20	11.83
0.00	0.00	0.00