


Data Path : Z:\HPCHEM1\BNA_F\Data\BF113015\
 Data File : BF083338.D
 Acq On : 30 Nov 2015 17:03
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 01 01:17:16 2015

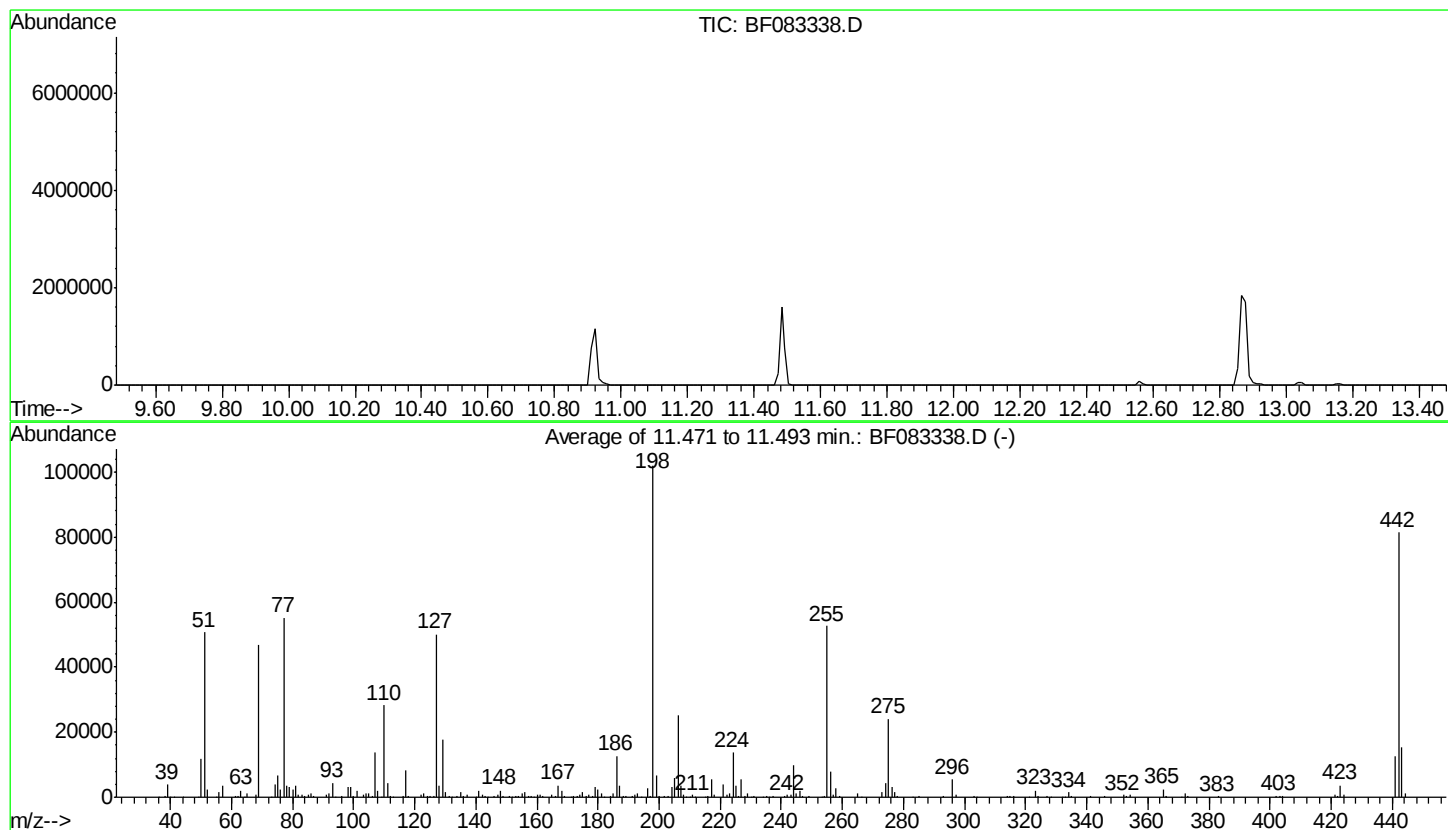

AutoFind: Scans 856, 857, 858; Background Corrected with Scan 852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.7	50640	PASS
68	69	0.00	2	1.8	846	PASS
69	198	0.00	100	45.9	46746	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.2	50098	PASS
197	198	0.00	2	0.5	552	PASS
198	198	100	100	100.0	101917	PASS
199	198	5	9	6.4	6504	PASS
275	198	10	60	23.7	24109	PASS
365	198	1	100	2.5	2509	PASS
441	442	0.01	24	15.5	12612	PASS
442	198	50	100	79.8	81304	PASS
443	442	15	24	19.0	15488	PASS