


Data Path : Z:\HPCHEM1\BNA F\Data\BF113015\
 Data File : BF083359.D
 Acq On : 1 Dec 2015 3:44
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 01 01:17:16 2015

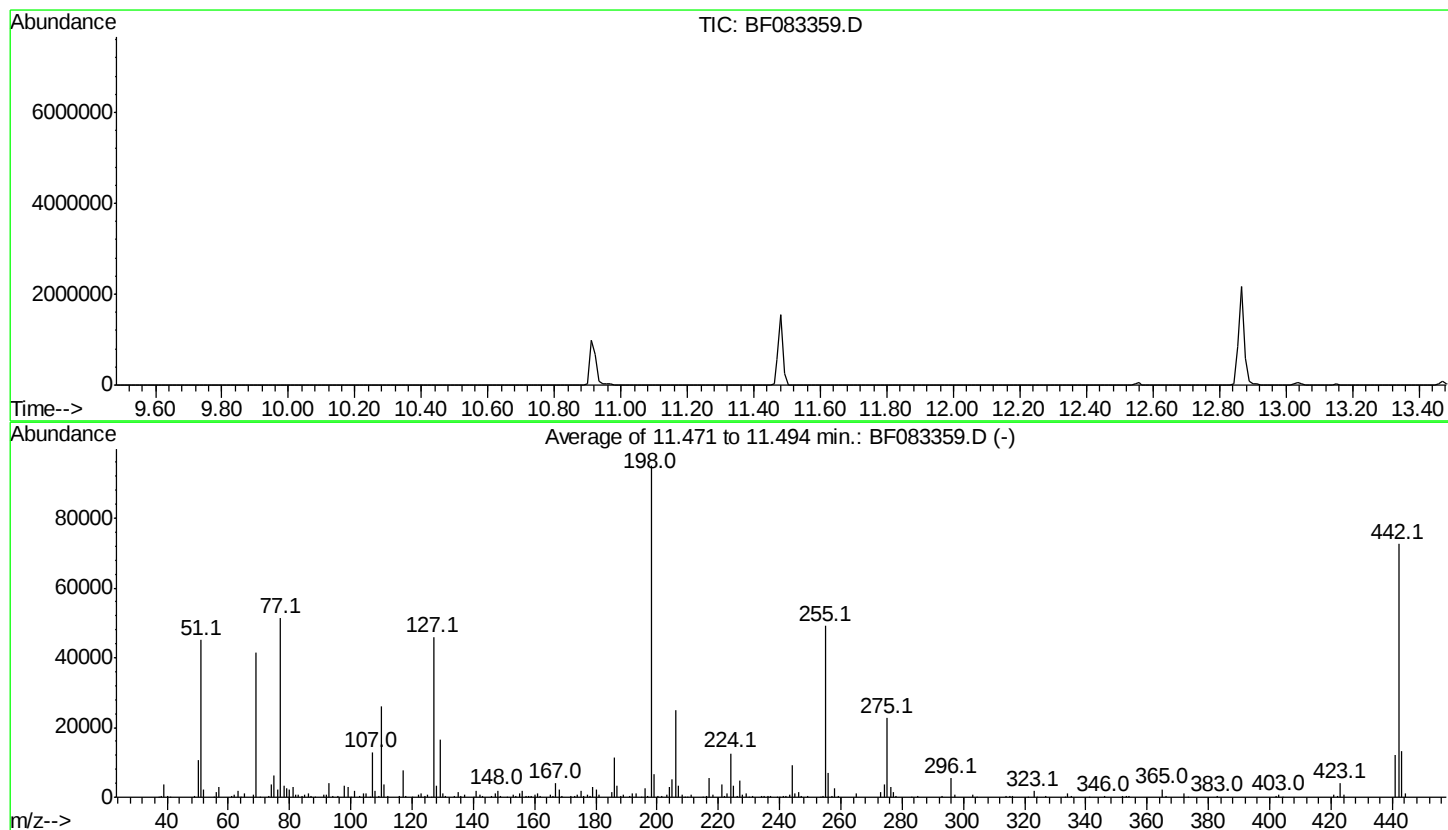

AutoFind: Scans 856, 857, 858; Background Corrected with Scan 852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	45072	PASS
68	69	0.00	2	1.6	655	PASS
69	198	0.00	100	43.6	41451	PASS
70	69	0.00	2	0.4	159	PASS
127	198	10	80	48.1	45742	PASS
197	198	0.00	2	0.5	479	PASS
198	198	100	100	100.0	95048	PASS
199	198	5	9	7.0	6627	PASS
275	198	10	60	23.9	22679	PASS
365	198	1	100	2.4	2308	PASS
441	442	0.01	24	16.5	12004	PASS
442	198	50	100	76.3	72559	PASS
443	442	15	24	18.2	13181	PASS