
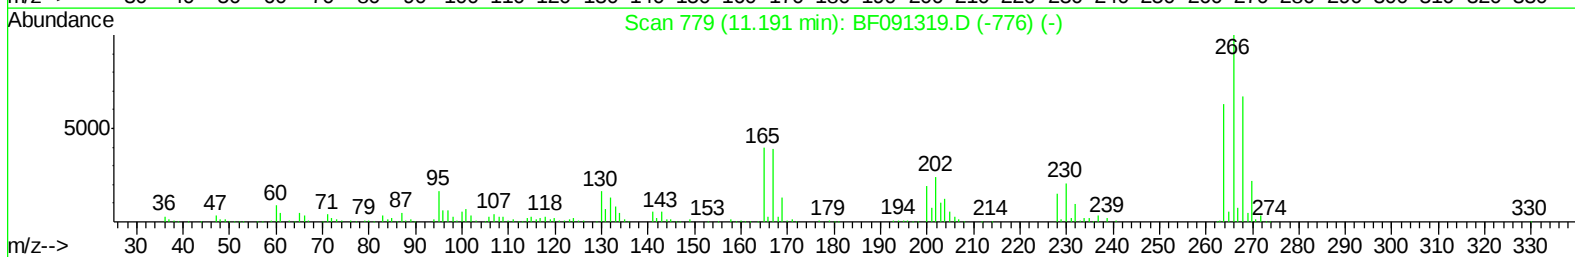
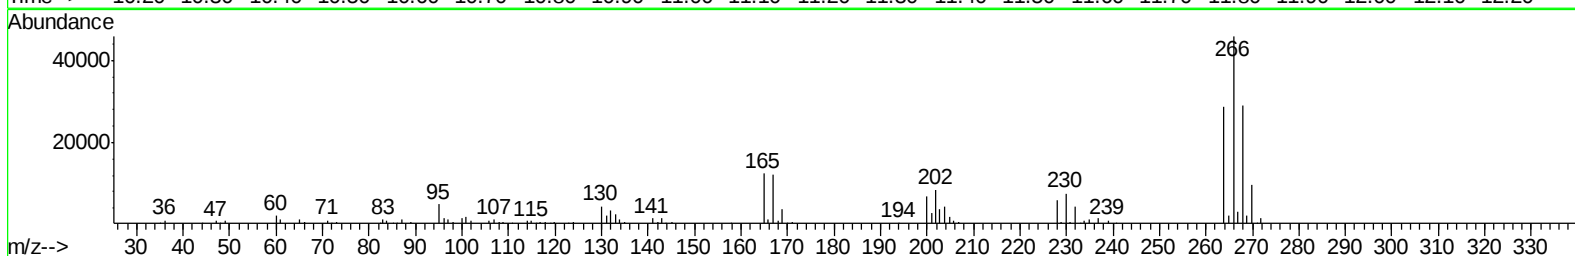


Data Path : Z:\HPCHEM1\BNA F\Data\BF113016\
Data File : BF091340.D
Acq On : 30 Nov 2016 8:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 18:05:48 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

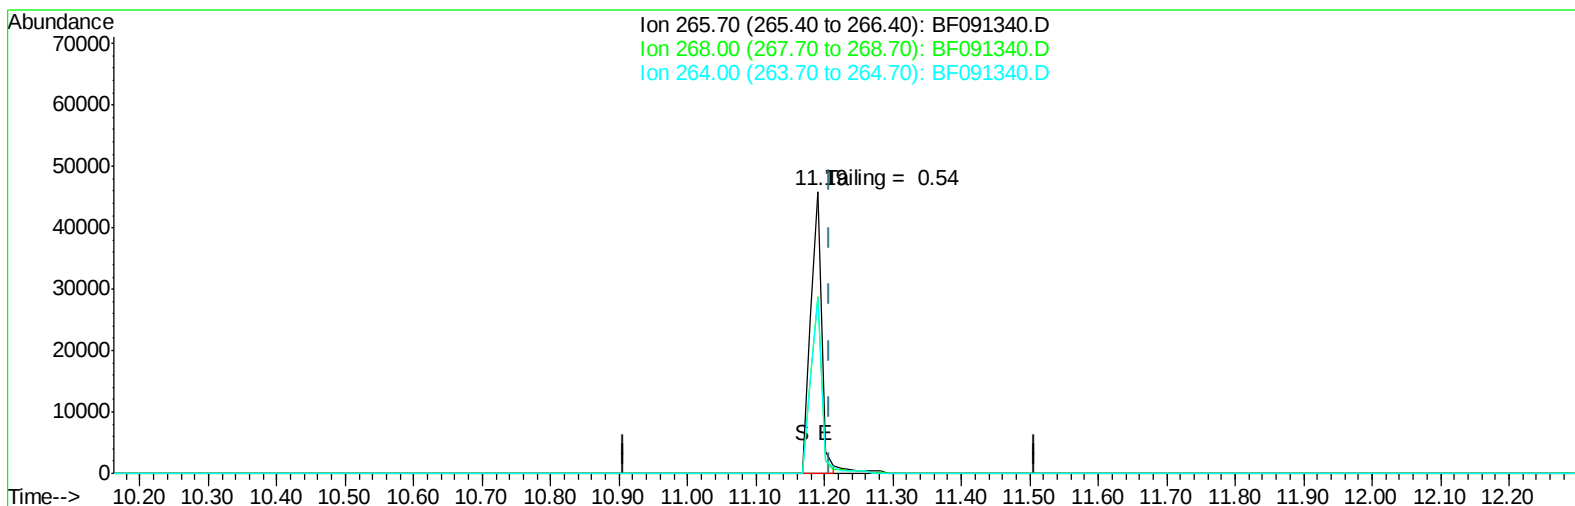

TIC: BF091340.D

(69) Pentachlorophenol (C)




11.191min (-0.017) 7438.88ng

response 54018

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	62.94
264.00	60.20	62.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF113016\
Data File : BF091340.D
Acq On : 30 Nov 2016 8:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 30 18:05:48 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

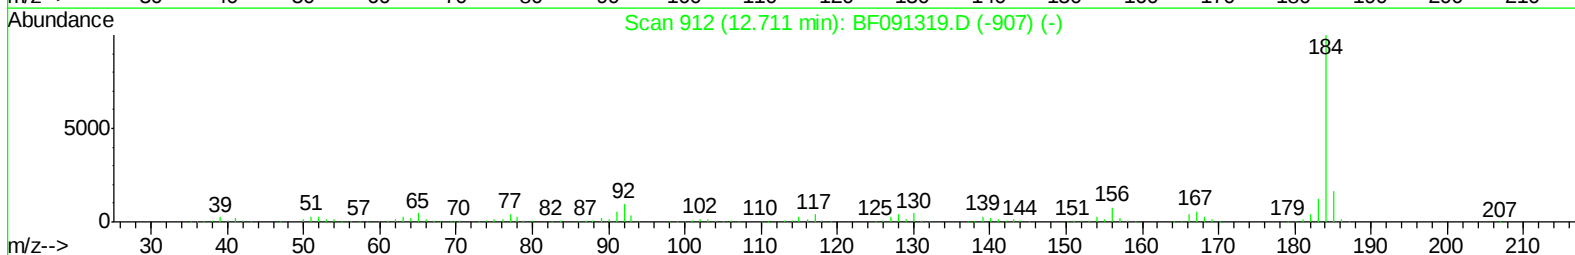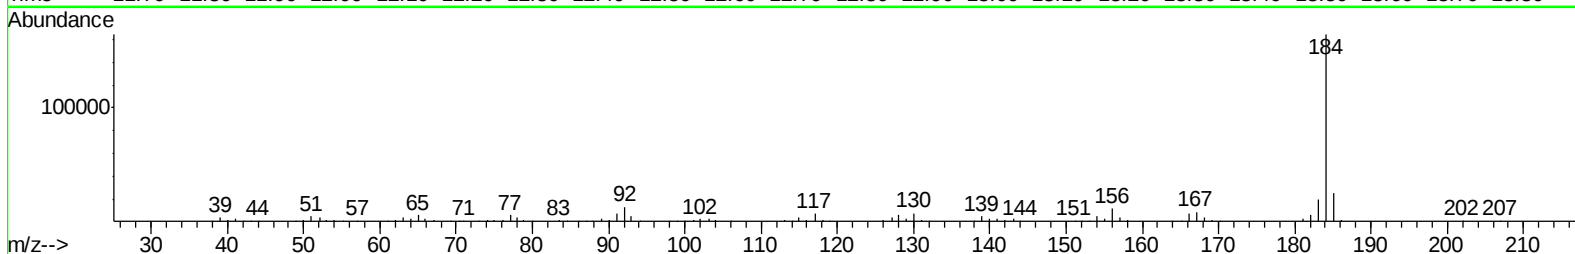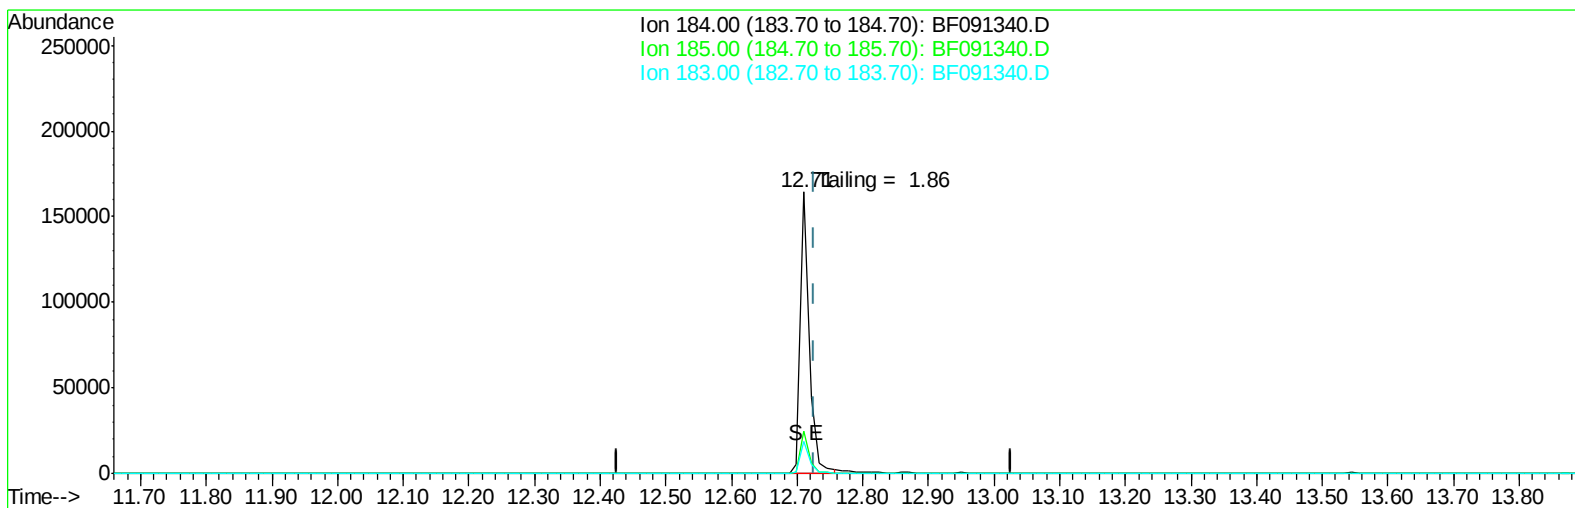

TIC: BF091340.D

(76) Benzidine

12.711min (-0.016) 96.29ng

response 159886

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	15.03
183.00	11.10	11.51
0.00	0.00	0.00