

Data Path : Z:\HPCHEM1\BNA F\DATA\BF113016\
 Data File : BF091367.D
 Acq On : 30 Nov 2016 21:10
 Operator : UM/SJ
 Sample : PB94960BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB94960BL

Quant Time: Dec 01 00:58:03 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 29 13:33:46 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	182676	20.00	ng	-0.02
21) Naphthalene-d8	8.15	136	777171	20.00	ng	-0.02
38) Acenaphthene-d10	9.90	164	384503	20.00	ng	-0.02
63) Phenanthrene-d10	11.38	188	606704	20.00	ng	-0.02
75) Chrysene-d12	14.01	240	441240	20.00	ng	-0.03
86) Perylene-d12	15.44	264	399267	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	691465	61.84	ng	0.00
7) Phenol-d6	6.48	99	875746	63.62	ng	-0.02
23) Nitrobenzene-d5	7.43	82	1061536	76.55	ng	-0.02
41) 2,4,6-Tribromophenol	10.69	330	205838	56.55	ng	-0.02
44) 2-Fluorobiphenyl	9.22	172	1648504	77.63	ng	-0.02
78) Terphenyl-d14	12.97	244	1436606	70.77	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF113016\
Data File : BF091367.D
Acq On : 30 Nov 2016 21:10
Operator : UM/SJ
Sample : PB94960BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94960BL

Quant Time: Dec 01 00:58:03 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 13:33:46 2016
Response via : Initial Calibration

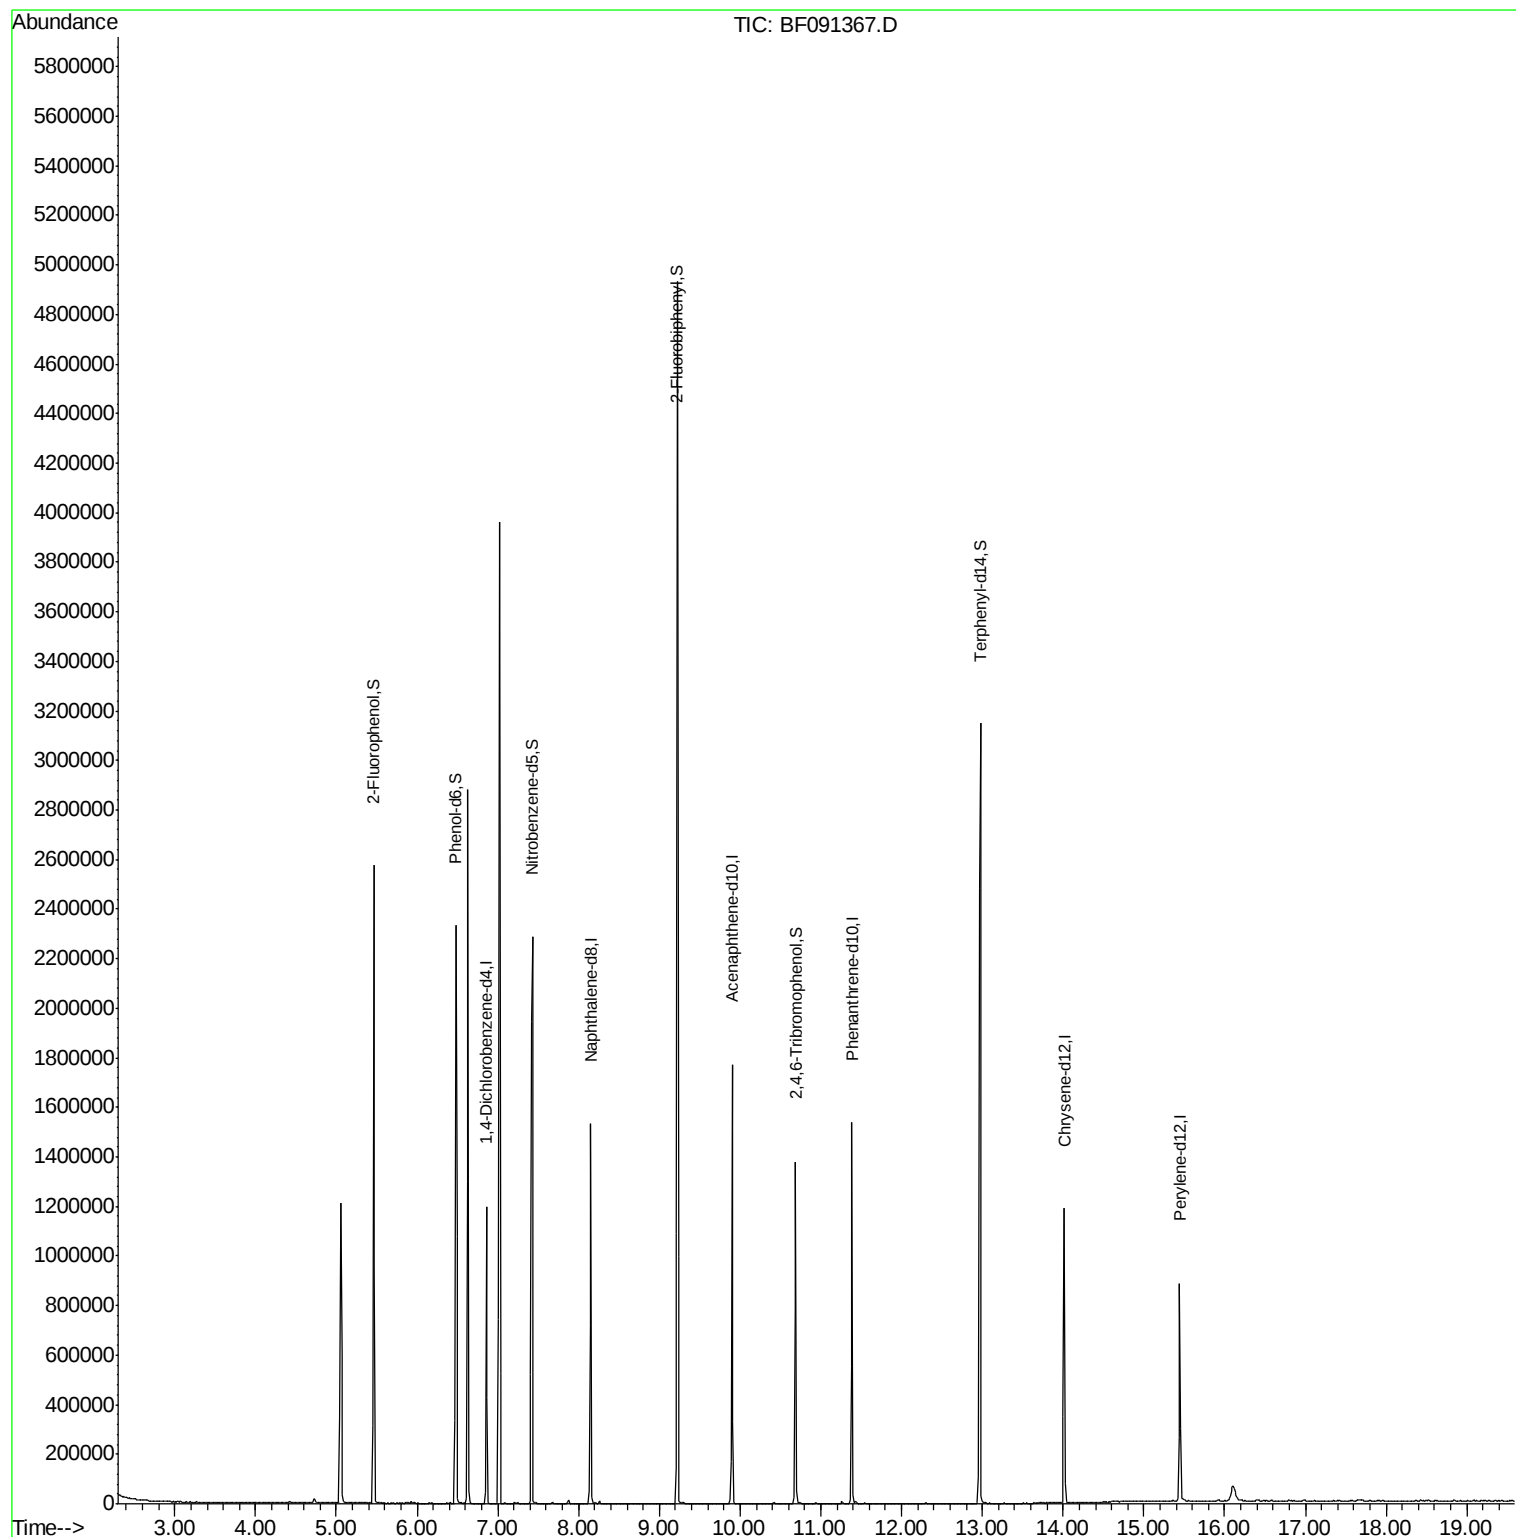

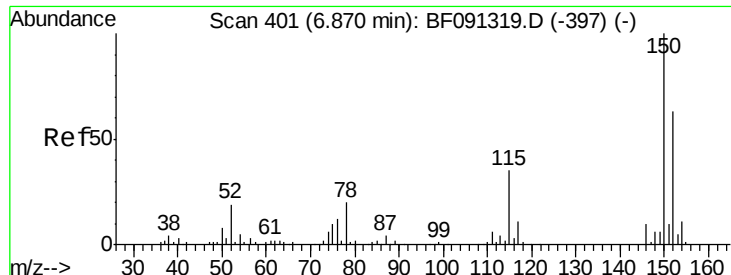

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.86 min Scan# 400

Delta R.T. -0.02 min

Lab File: BF091367.D

Acq: 30 Nov 2016 21:10

Instrument :

BNA_F

ClientSampleId :

PB94960BL


Tot Ion:152 Resp: 182676

Ion Ratio Lower Upper

152 100

150 157.1 122.5 183.7



115 68.9 51.8 77.8

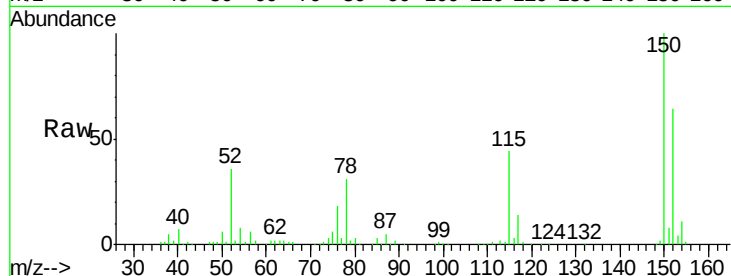

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

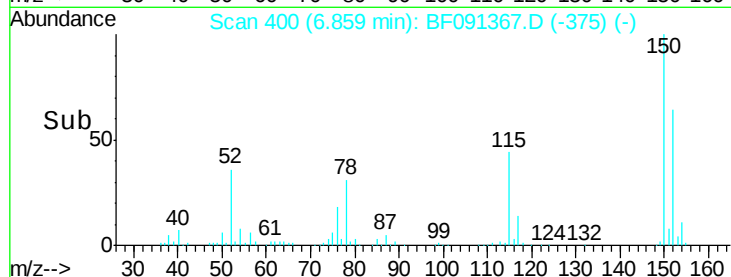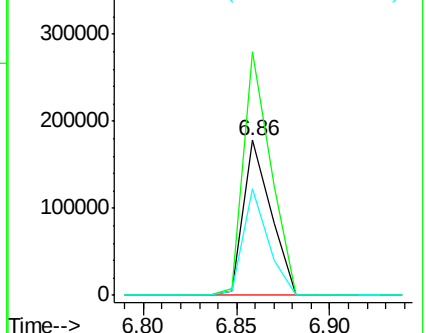

#5

2-Fluorophenol

Concen: 61.84 ng

RT: 5.46 min Scan# 278

Delta R.T. -0.00 min

Lab File: BF091367.D

Acq: 30 Nov 2016 21:10


Tgt Ion:112 Resp: 691465

Ion Ratio Lower Upper

112 100

64 76.8 61.5 92.3



63 41.3 33.3 49.9

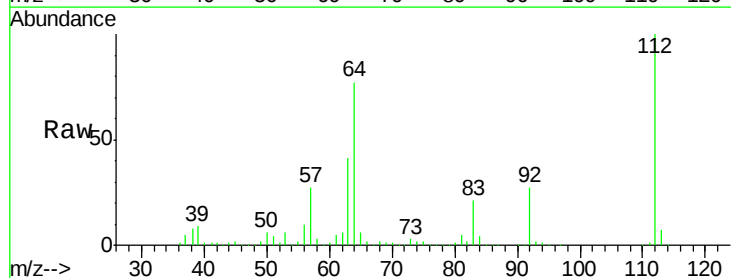


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

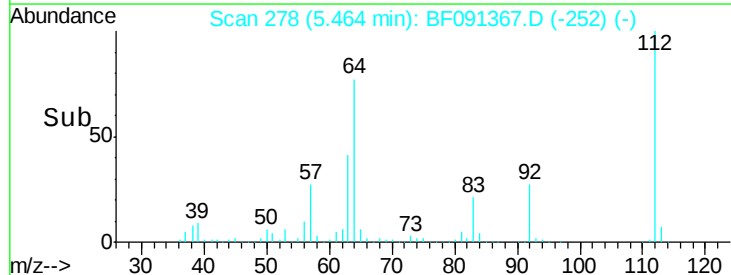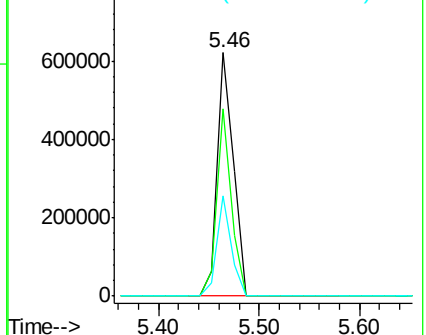

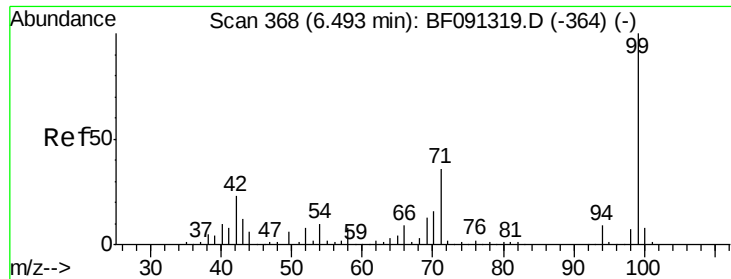

#7

Phenol-d6

Concen: 63.62 ng

RT: 6.48 min Scan# 367

Delta R.T. -0.02 min

Lab File: BF091367.D

Acq: 30 Nov 2016 21:10

Instrument :

BNA_F

ClientSampleId :

PB94960BL


Tot Ion: 99 Resp: 875746

Ion Ratio Lower Upper

99 100

42 26.0 20.6 31.0




71 37.3 29.9 44.9

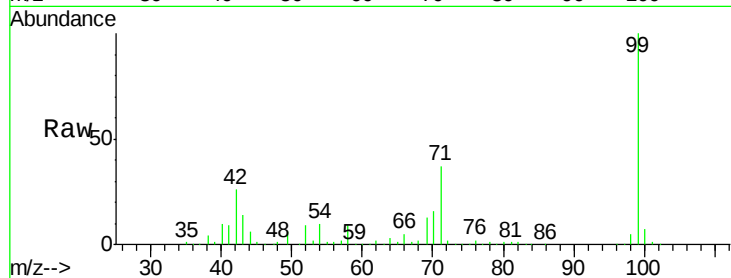

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

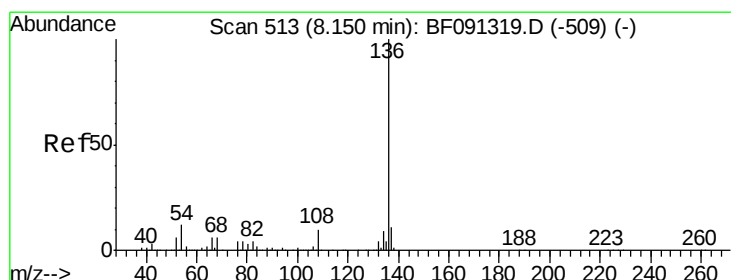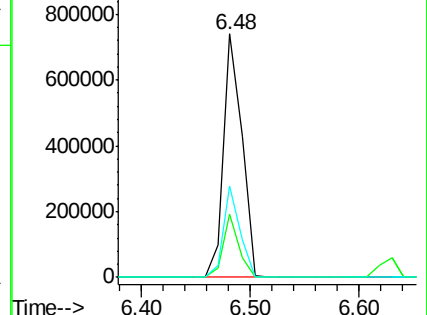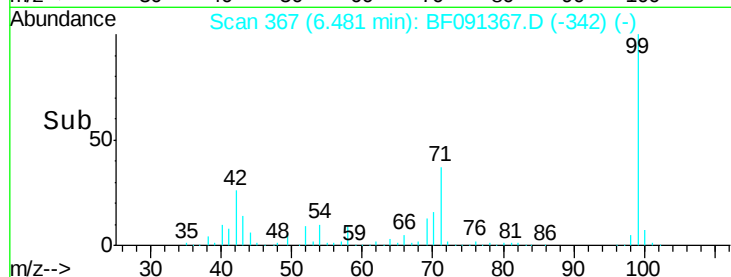

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.15 min Scan# 513

Delta R.T. -0.02 min

Lab File: BF091367.D

Acq: 30 Nov 2016 21:10

Tgt Ion: 136 Resp: 777171


Ion Ratio Lower Upper

136 100

137 11.0 9.1 13.7

54 9.0 9.1 13.7#

68 4.8 5.9 8.9#


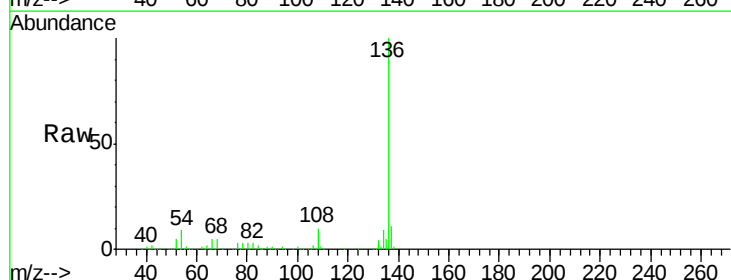


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

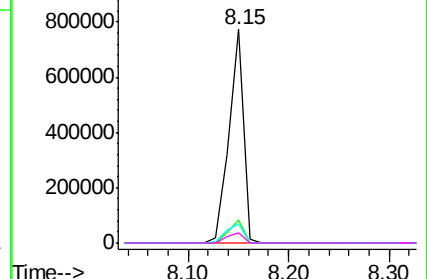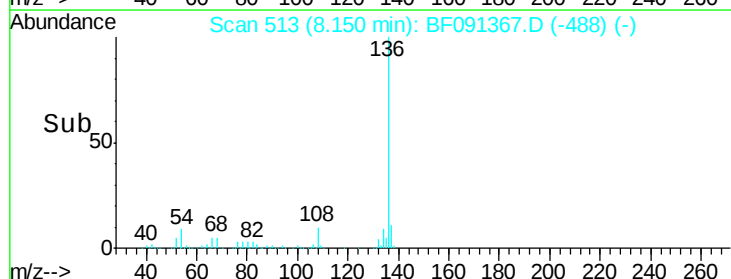







#23
 Nitrobenzene-d5
 Concen: 76.55 ng
 RT: 7.43 min Scan# 450
 Delta R.T. -0.02 min
 Lab File: BF091367.D
 Acq: 30 Nov 2016 21:10

Instrument :
 BNA_F
 ClientSampleId :
 PB94960BL

Tot Ion: 82 Resp: 1061536
 Ion Ratio Lower Upper
 82 100
 128 50.4 31.8 47.6#
 54 56.8 49.1 73.7

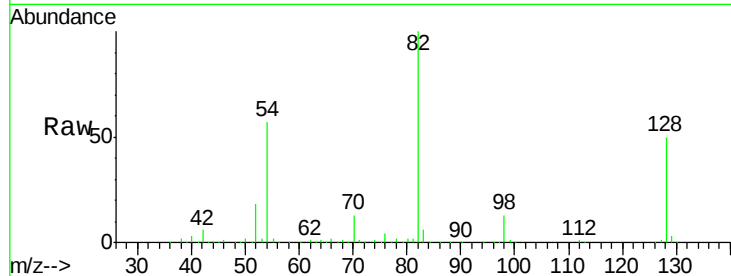


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

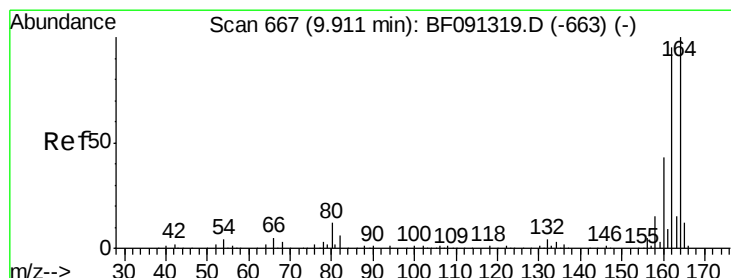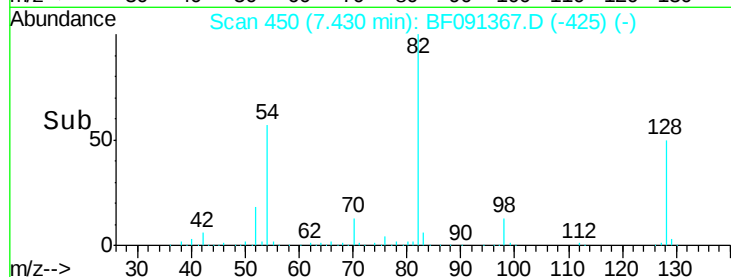
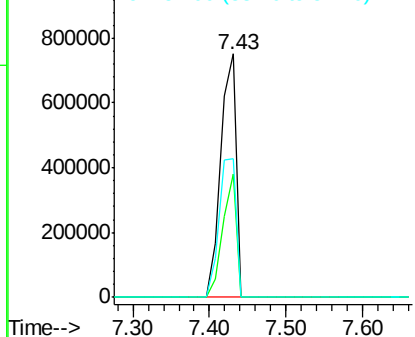



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.90 min Scan# 666
 Delta R.T. -0.02 min
 Lab File: BF091367.D
 Acq: 30 Nov 2016 21:10

Tgt Ion: 164 Resp: 384503
 Ion Ratio Lower Upper
 164 100
 162 96.9 82.6 124.0
 160 42.6 36.7 55.1

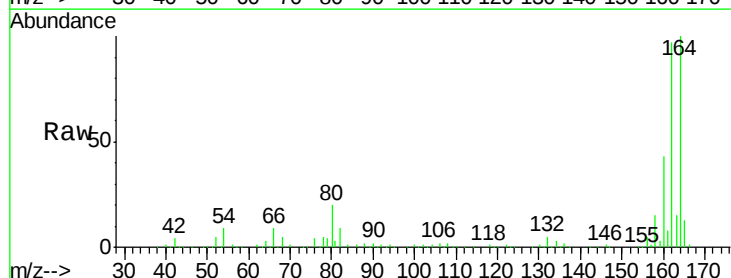

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

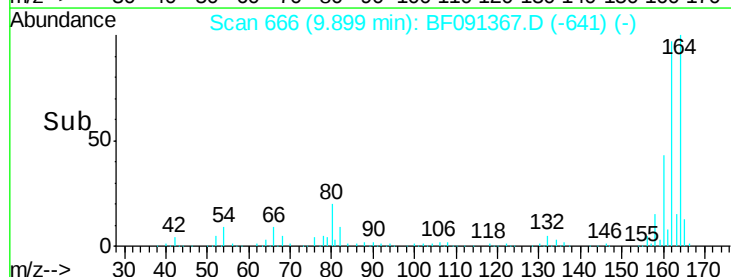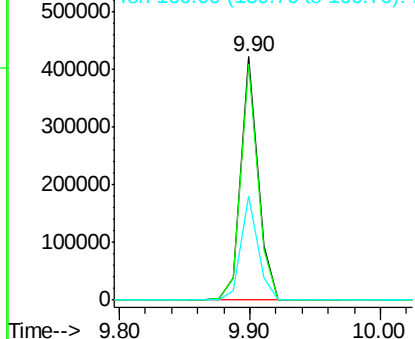

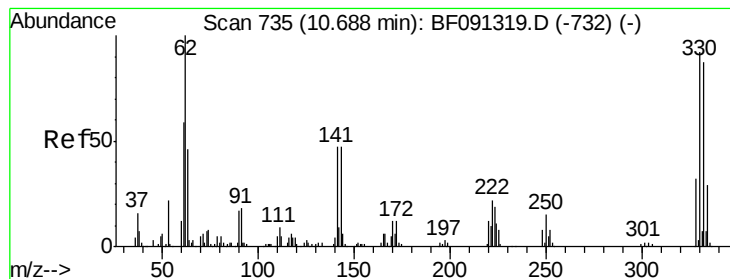

#41

2,4,6-Tribromophenol

Concen: 56.55 ng

RT: 10.69 min Scan# 735

Delta R.T. -0.02 min

Lab File: BF091367.D

Acq: 30 Nov 2016 21:10

Instrument :

BNA_F

ClientSampleId :

PB94960BL


Tot Ion:330 Resp: 205838

Ion Ratio Lower Upper

330 100

332 96.6 76.2 114.4




141 29.9 33.6 50.4#

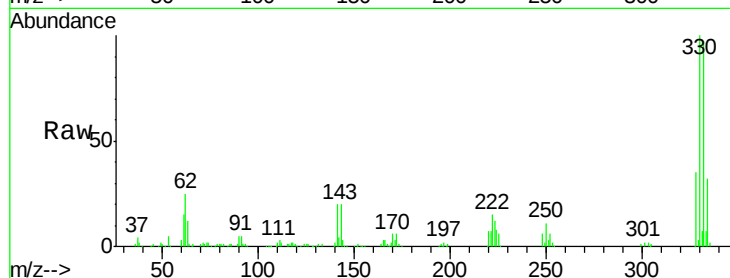

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

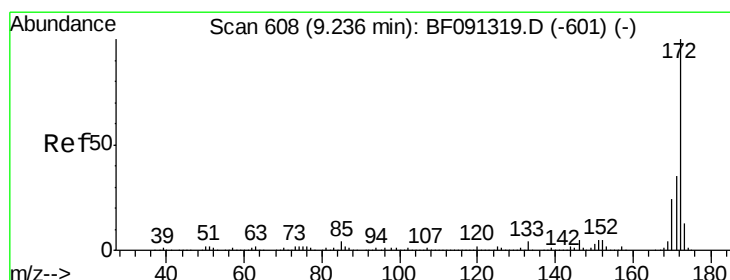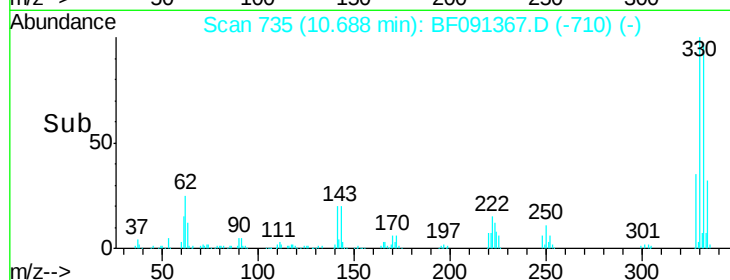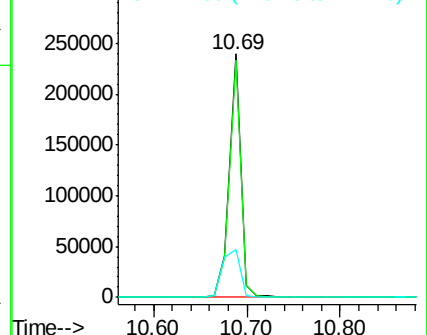

#44

2-Fluorobiphenyl

Concen: 77.63 ng

RT: 9.22 min Scan# 607

Delta R.T. -0.02 min

Lab File: BF091367.D

Acq: 30 Nov 2016 21:10


Tgt Ion:172 Resp: 1648504

Ion Ratio Lower Upper

172 100

171 36.4 29.4 44.0



170 24.4 19.7 29.5

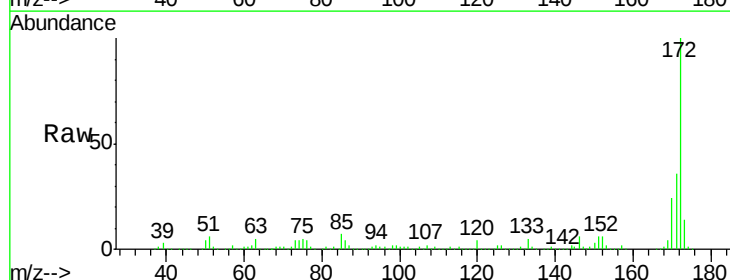


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

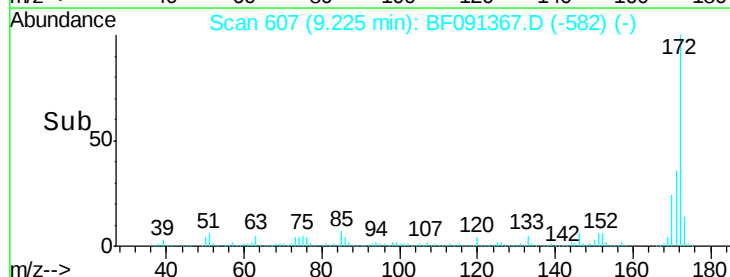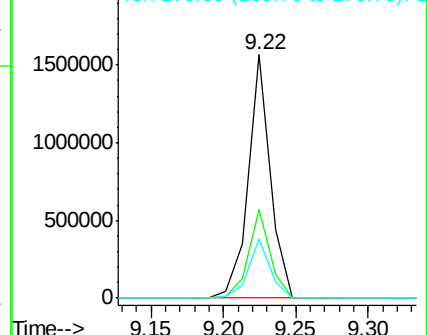

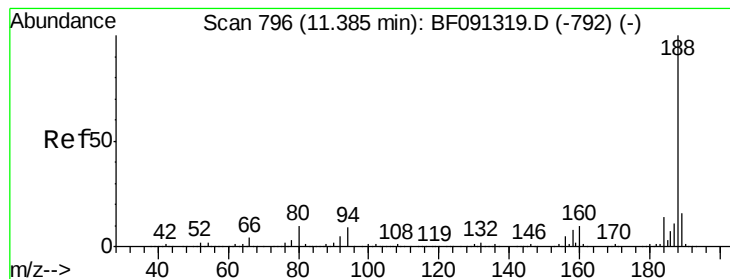

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.38 min Scan# 796

Delta R.T. -0.02 min

Lab File: BF091367.D

Acq: 30 Nov 2016 21:10

Instrument :

BNA_F

ClientSampleId :

PB94960BL


Tot Ion:188 Resp: 606704

Ion Ratio Lower Upper

188 100

94 7.0 9.2 13.8#




80 7.3 10.5 15.7#

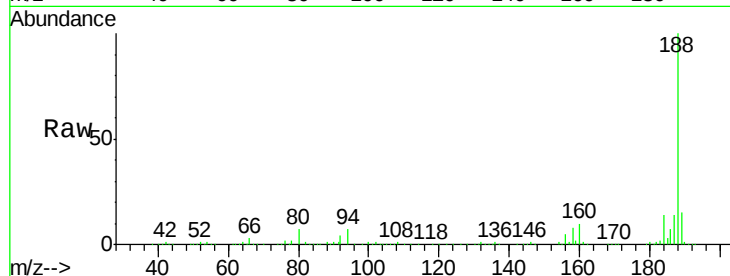

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

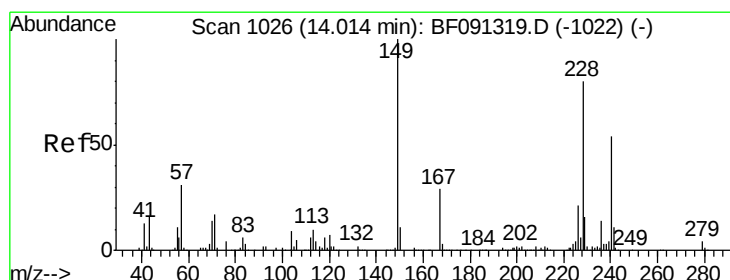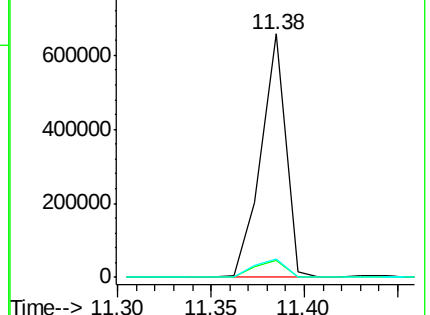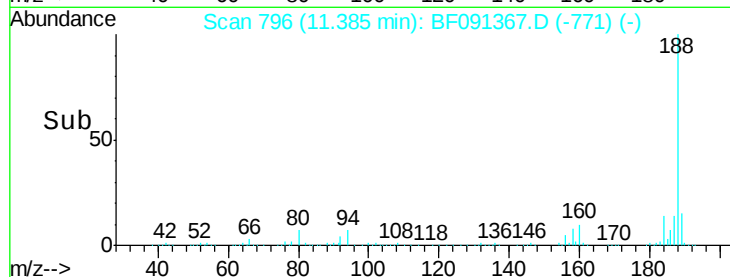

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.01 min Scan# 1026

Delta R.T. -0.03 min

Lab File: BF091367.D

Acq: 30 Nov 2016 21:10


Tgt Ion:240 Resp: 441240

Ion Ratio Lower Upper

240 100

120 8.3 12.1 18.1#



236 24.9 21.0 31.6

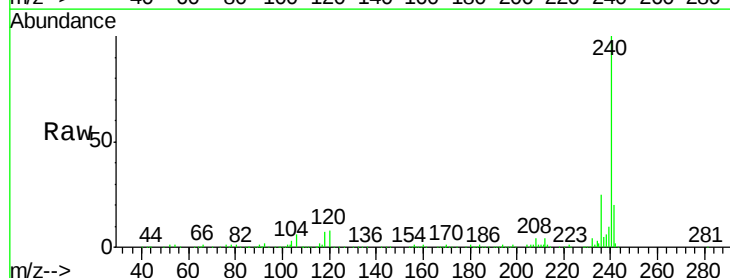

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



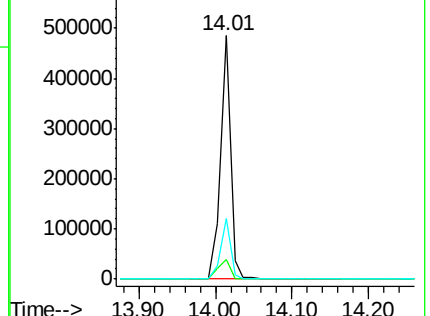
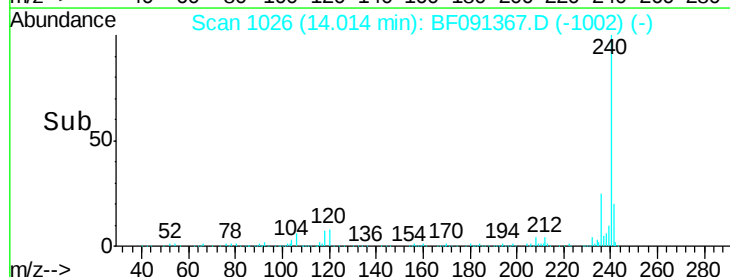




#78
 Terphenyl-d14
 Concen: 70.77 ng
 RT: 12.97 min Scan# 935
 Delta R.T. -0.02 min
 Lab File: BF091367.D
 Acq: 30 Nov 2016 21:10

Instrument :
 BNA_F
 ClientSampleId :
 PB94960BL

Tot Ion:244 Resp: 1436606
 Ion Ratio Lower Upper
 244 100
 212 6.3 6.5 9.7#
 122 5.6 9.5 14.3#

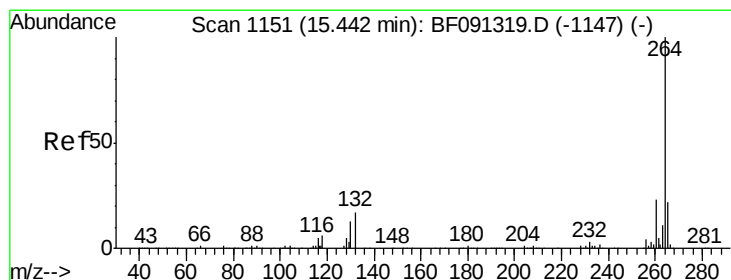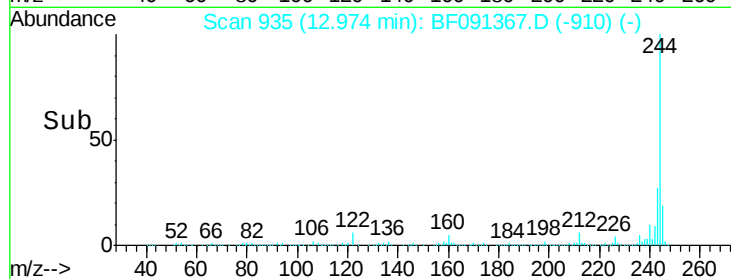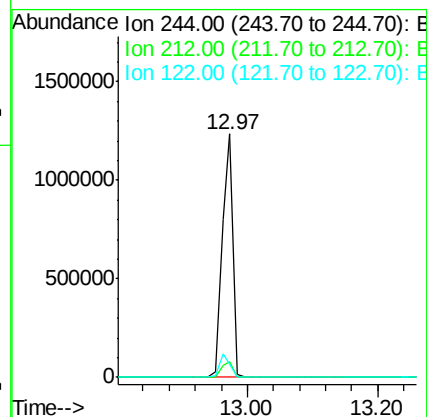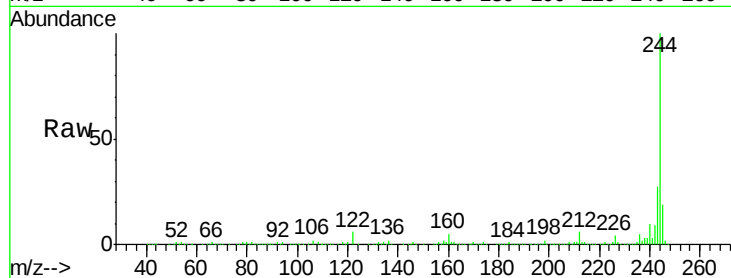

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.44 min Scan# 1151
 Delta R.T. -0.03 min
 Lab File: BF091367.D
 Acq: 30 Nov 2016 21:10

Tgt Ion:264 Resp: 399267
 Ion Ratio Lower Upper
 264 100
 260 23.5 18.8 28.2
 265 21.8 17.0 25.6

