

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF113016\
 Data File : BF091363.D
 Acq On : 30 Nov 2016 19:19
 Operator : UM/SJ
 Sample : H5779-03
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 112816-DSDC-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.041	238	241	243	rBV	382993	489631	8.71%	1.496%
2	5.453	275	277	280	rBV	1360505	1373936	24.45%	4.197%
3	6.481	365	367	369	rBV	1218806	1078299	19.19%	3.294%
4	6.630	377	380	382	rBV	2580882	2704424	48.13%	8.260%
5	6.859	398	400	403	rBV	1040029	1100478	19.58%	3.361%
6	7.019	411	414	417	rVB	4058216	3909095	69.56%	11.940%
7	7.430	447	450	452	rBV	3512795	3923141	69.81%	11.983%
8	8.150	510	513	515	rBV	1635372	1511920	26.91%	4.618%
9	9.225	604	607	610	rBV	4974294	5619344	100.00%	17.164%
10	9.613	639	641	644	rBV	70469	68250	1.21%	0.208%
11	9.899	664	666	669	rVB	1812374	1517778	27.01%	4.636%
12	10.688	732	735	737	rBV	1785284	1905033	33.90%	5.819%
13	10.813	744	746	751	rVB	56800	65253	1.16%	0.199%
14	11.385	793	796	798	rBV	1291702	1283056	22.83%	3.919%
15	11.911	840	842	848	rBV	71226	93138	1.66%	0.284%
16	12.699	909	911	918	rBV	73790	92827	1.65%	0.284%
17	12.974	932	935	937	rBV	3171820	4032724	71.77%	12.318%
18	14.014	1023	1026	1028	rBV	1062704	1027488	18.28%	3.138%
19	15.442	1148	1151	1154	rBV	778292	943537	16.79%	2.882%


Sum of corrected areas: 32739352

Data Path : Z:\HPCHEM1\BNA F\DATA\BF113016\
Data File : BF091363.D
Acq On : 30 Nov 2016 19:19
Operator : UM/SJ
Sample : H5779-03
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112816-DSDC-F-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

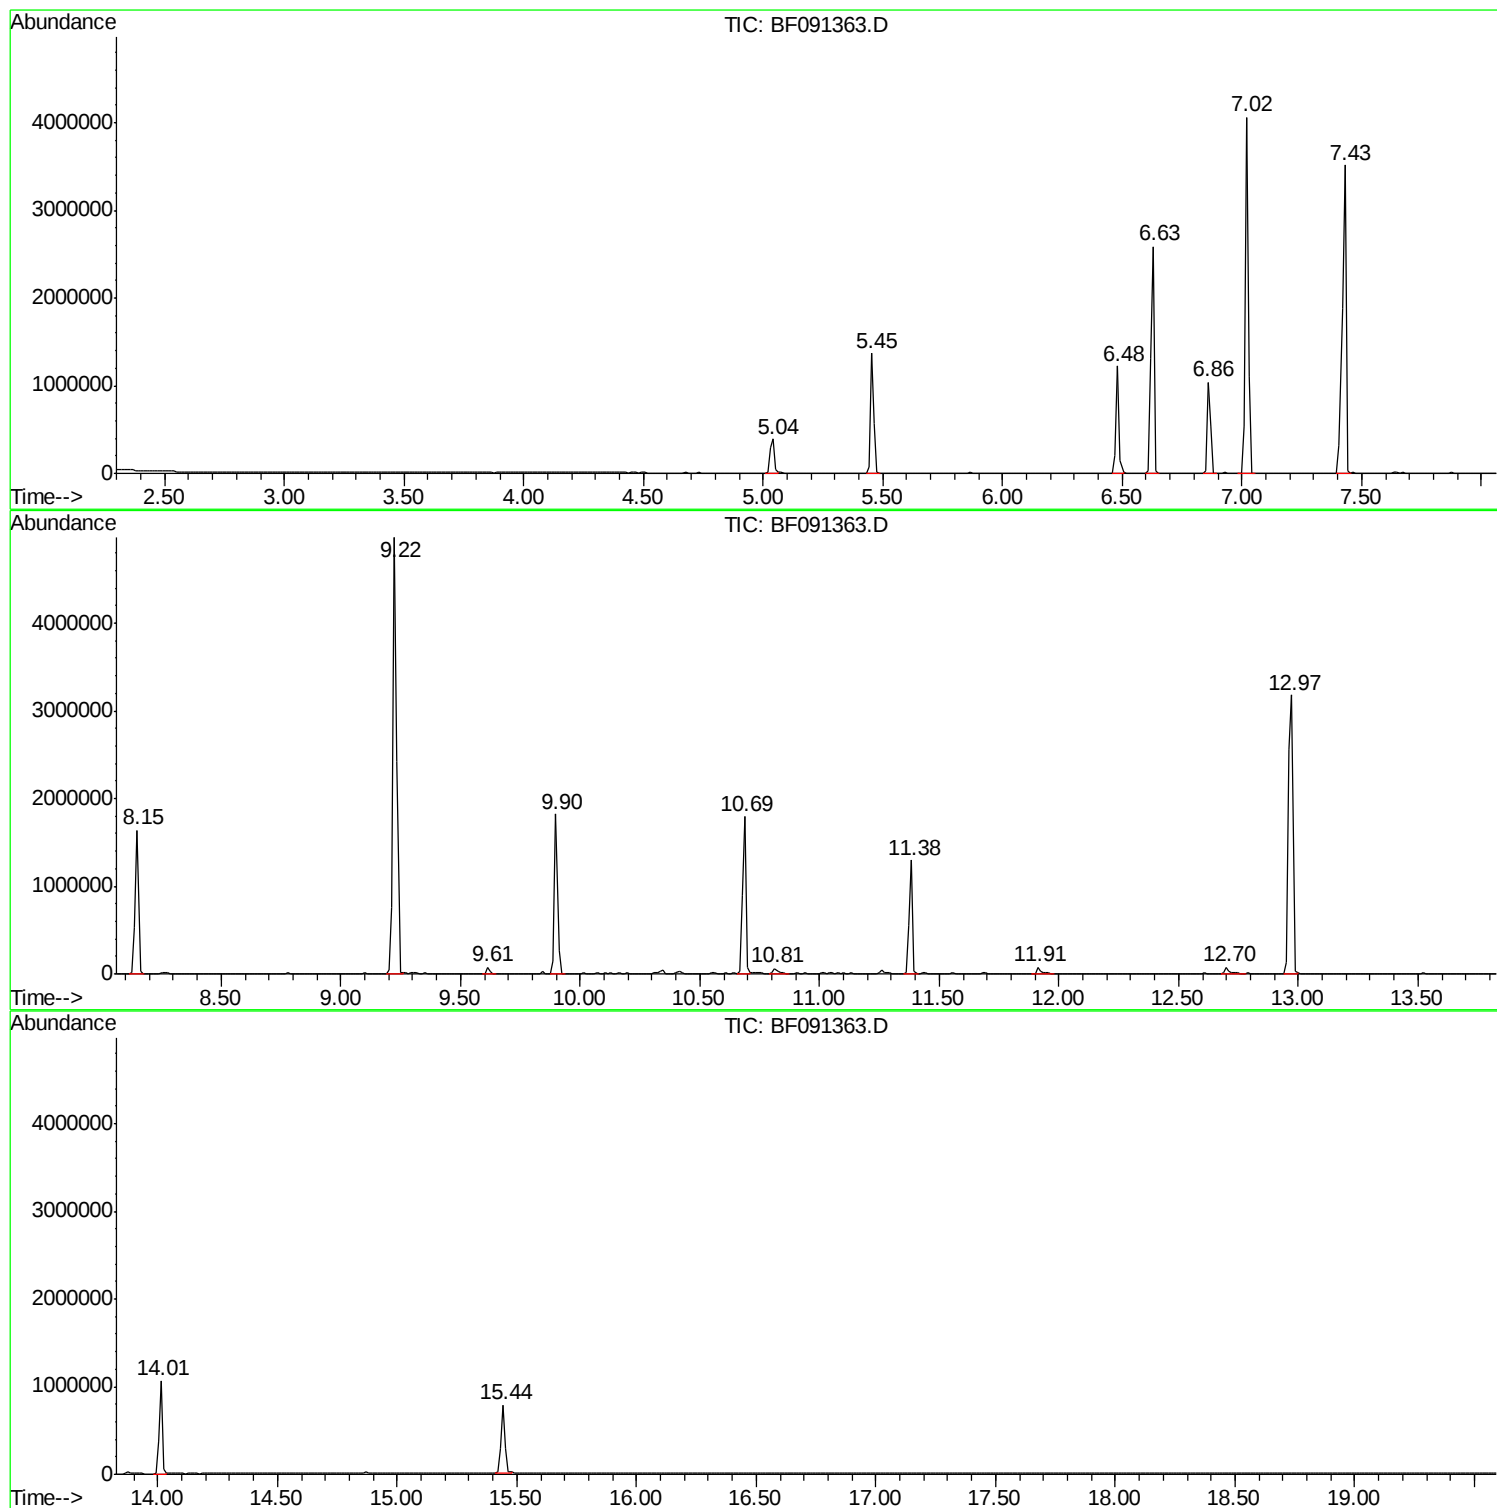

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF113016\
Data File : BF091363.D
Acq On : 30 Nov 2016 19:19
Operator : UM/SJ
Sample : H5779-03
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112816-DSDC-F-U-B










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.04	8.90 ng	489631	1,4-Dichlorobenzene-d4	6.86

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28
4			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
5			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16

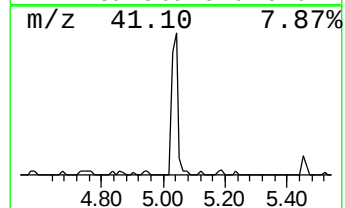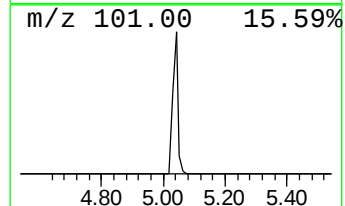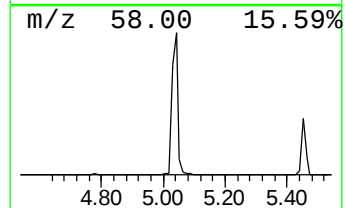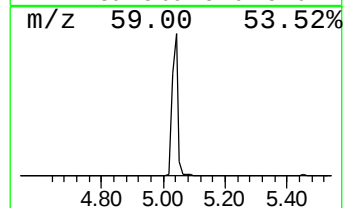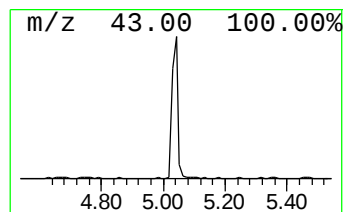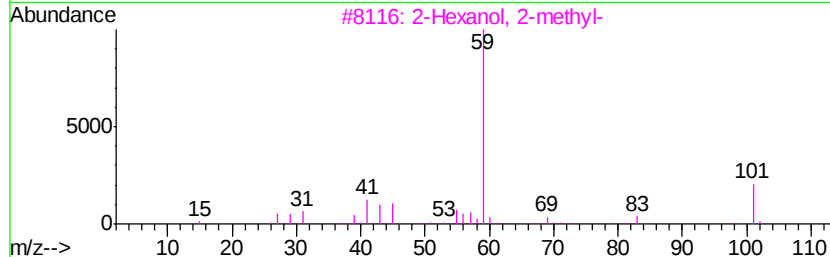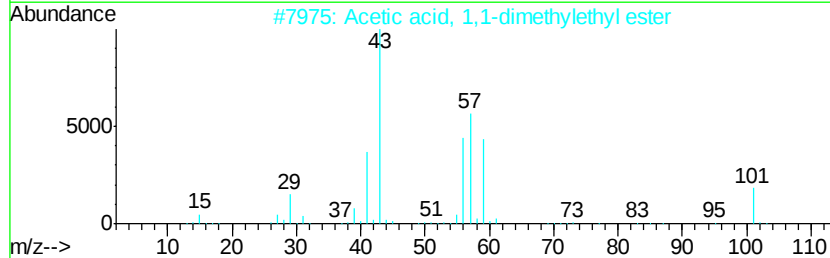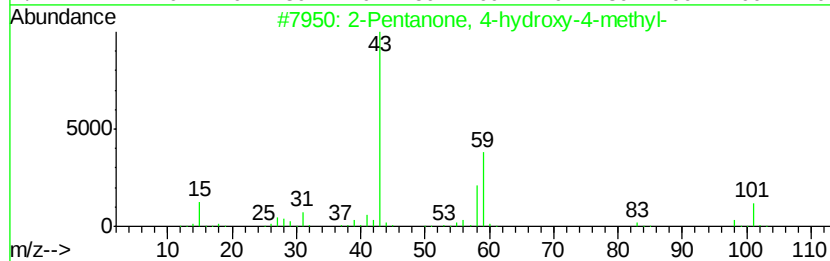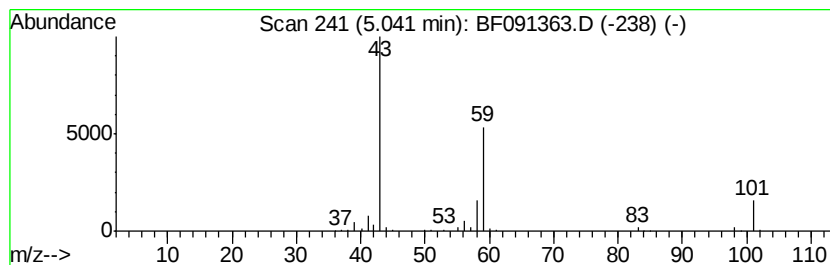

Data Path : Z:\HPCHEM1\BNA F\DATA\BF113016\
Data File : BF091363.D
Acq On : 30 Nov 2016 19:19
Operator : UM/SJ
Sample : H5779-03
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112816-DSDC-F-U-B










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.63 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.63	49.15 ng	2704420	1,4-Dichlorobenzene-d4	6.86

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	9
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9

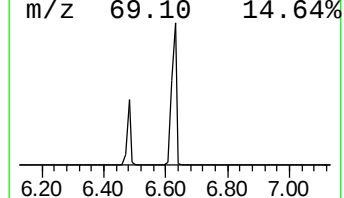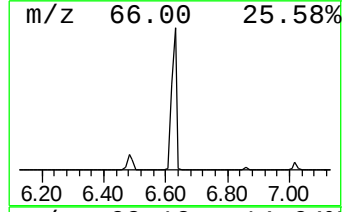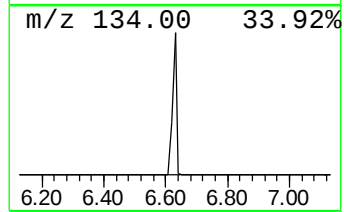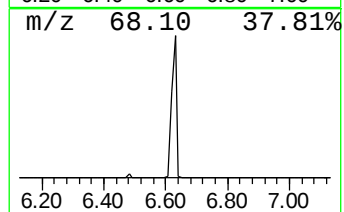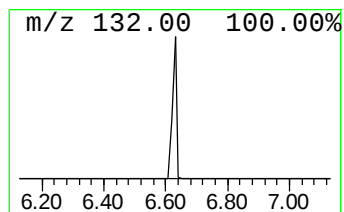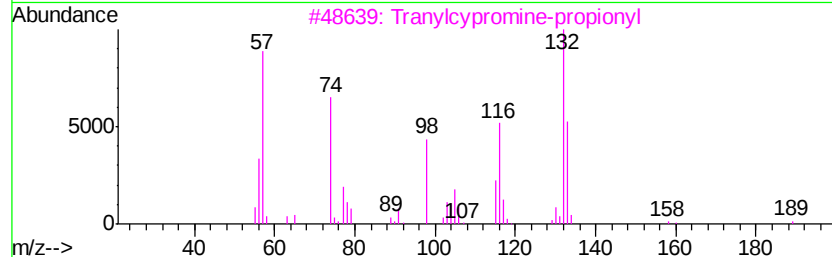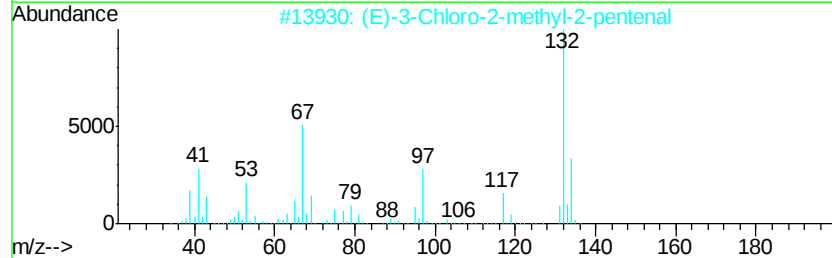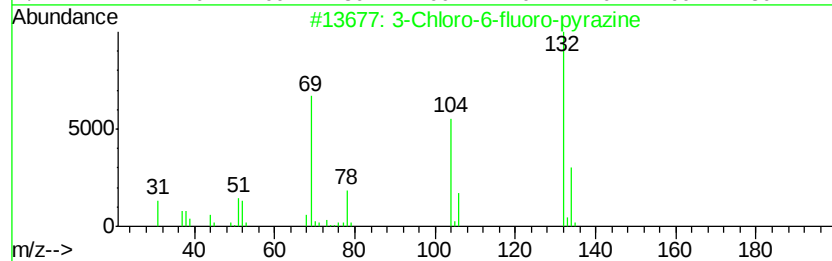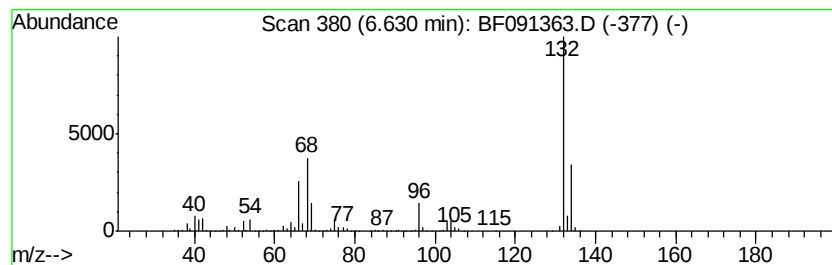

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF113016\
Data File : BF091363.D
Acq On : 30 Nov 2016 19:19
Operator : UM/SJ
Sample : H5779-03
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112816-DSDC-F-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.04	8.9	ng	489631	1	6.86	1100480	20.0
unknown6.63	6.63	49.1	ng	2704420	1	6.86	1100480	20.0