


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF113016\
Data File : BF091340.D
Acq On : 30 Nov 2016 8:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 29 13:33:46 2016

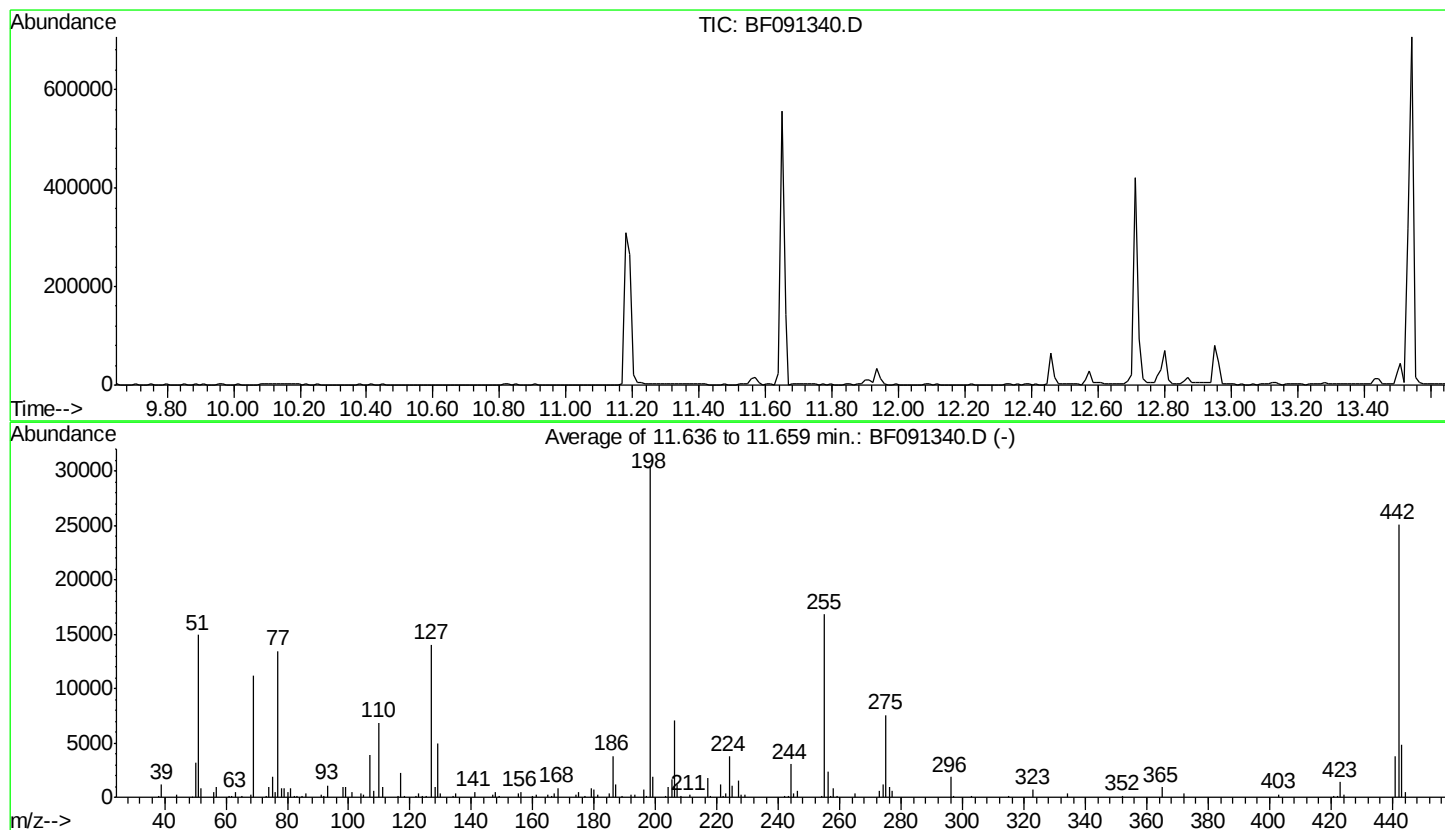

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.0	14938	PASS
68	69	0.00	2	1.8	196	PASS
69	198	0.00	100	36.5	11133	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.0	14019	PASS
197	198	0.00	2	0.6	174	PASS
198	198	100	100	100.0	30503	PASS
199	198	5	9	6.0	1843	PASS
275	198	10	60	24.8	7550	PASS
365	198	1	100	3.1	931	PASS
441	442	0.01	24	15.2	3813	PASS
442	198	50	100	82.2	25074	PASS
443	442	15	24	19.2	4816	PASS