


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF113016\
 Data File : BF091365.D
 Acq On : 30 Nov 2016 20:15
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 29 13:33:46 2016

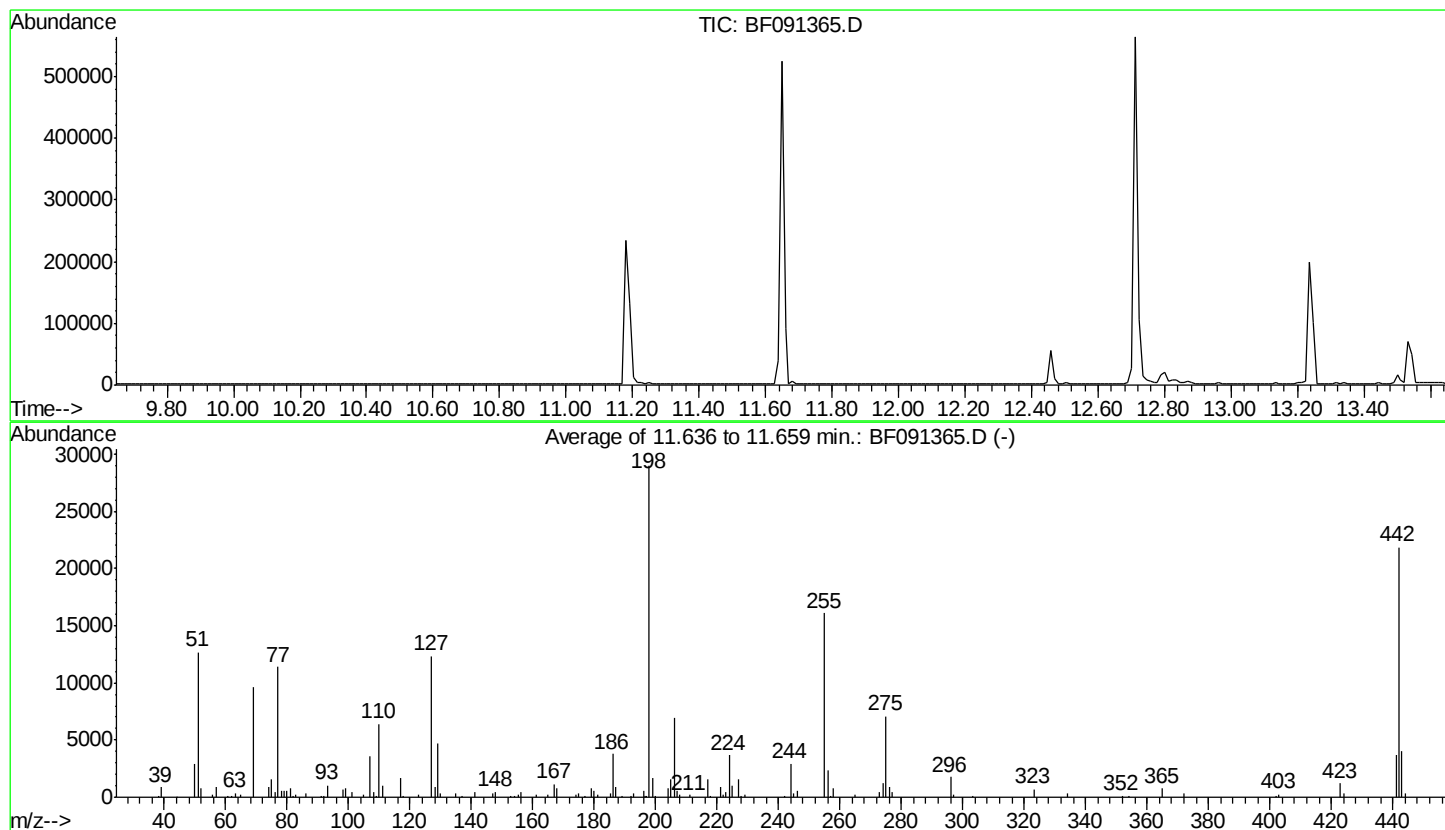

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	12655	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.1	9584	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.7	12365	PASS
197	198	0.00	2	0.5	142	PASS
198	198	100	100	100.0	28986	PASS
199	198	5	9	5.8	1671	PASS
275	198	10	60	24.5	7092	PASS
365	198	1	100	2.6	762	PASS
441	442	0.01	24	16.9	3695	PASS
442	198	50	100	75.3	21824	PASS
443	442	15	24	18.7	4083	PASS