


Data Path : Z:\HPCHEM1\BNA F\DATA\BF113017\
 Data File : BF101010.D
 Acq On : 30 Nov 2017 11:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF113017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 01 09:47:02 2017

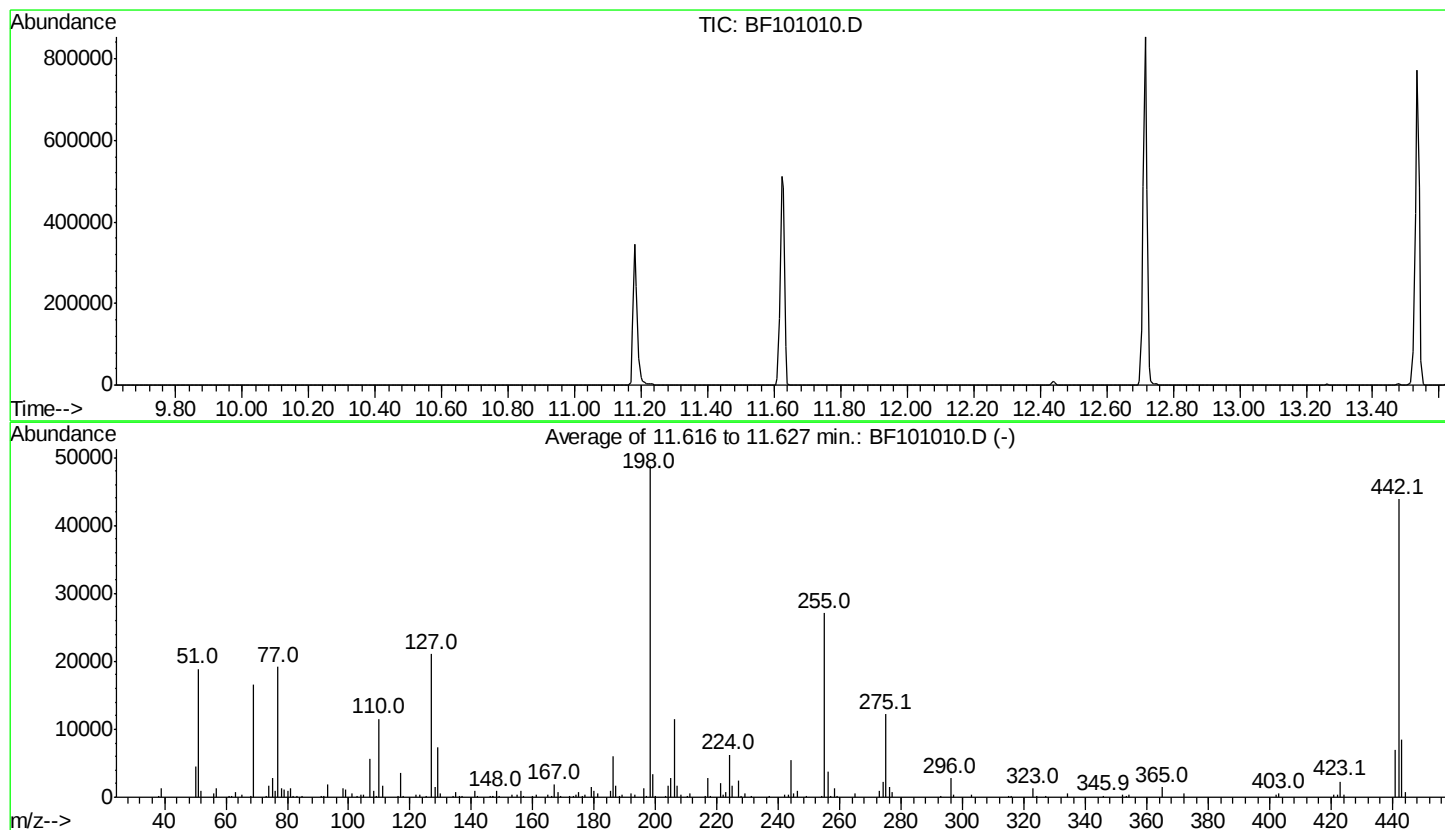

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	18905	PASS
68	69	0.00	2	1.3	209	PASS
69	198	0.00	100	33.9	16519	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	21086	PASS
197	198	0.00	2	0.6	280	PASS
198	198	100	100	100.0	48781	PASS
199	198	5	9	7.1	3463	PASS
275	198	10	60	24.9	12154	PASS
365	198	1	100	2.9	1434	PASS
441	443	0.01	100	82.7	7063	PASS
442	198	50	100	89.9	43830	PASS
443	442	15	24	19.5	8540	PASS