
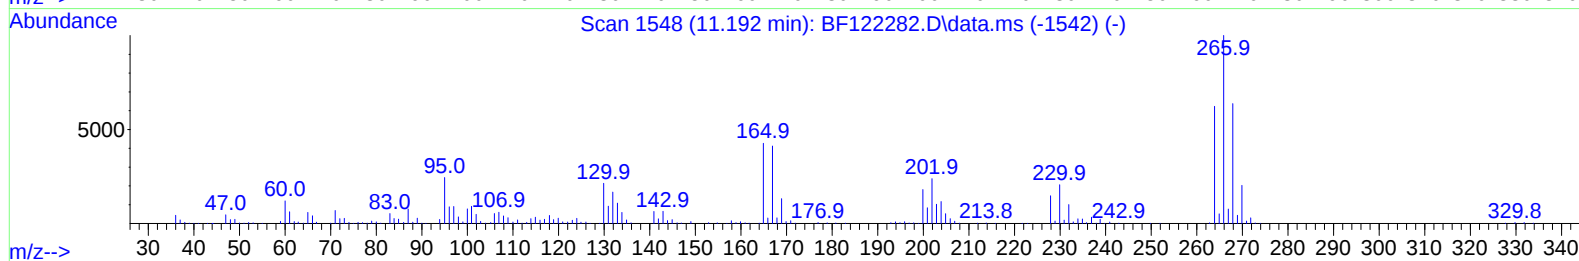
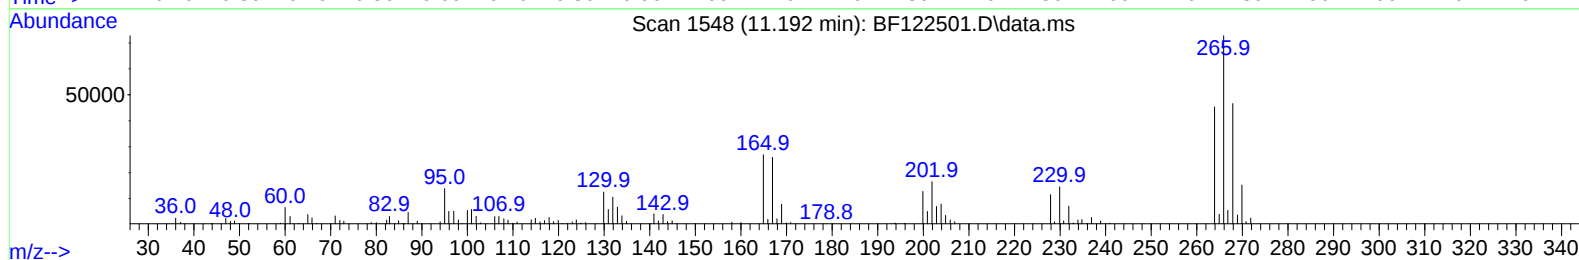


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113020\
Data File : BF122501.D
Acq On : 30 Nov 2020 11:15
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 01:13:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 14:38:56 2020
Response via : Initial Calibration

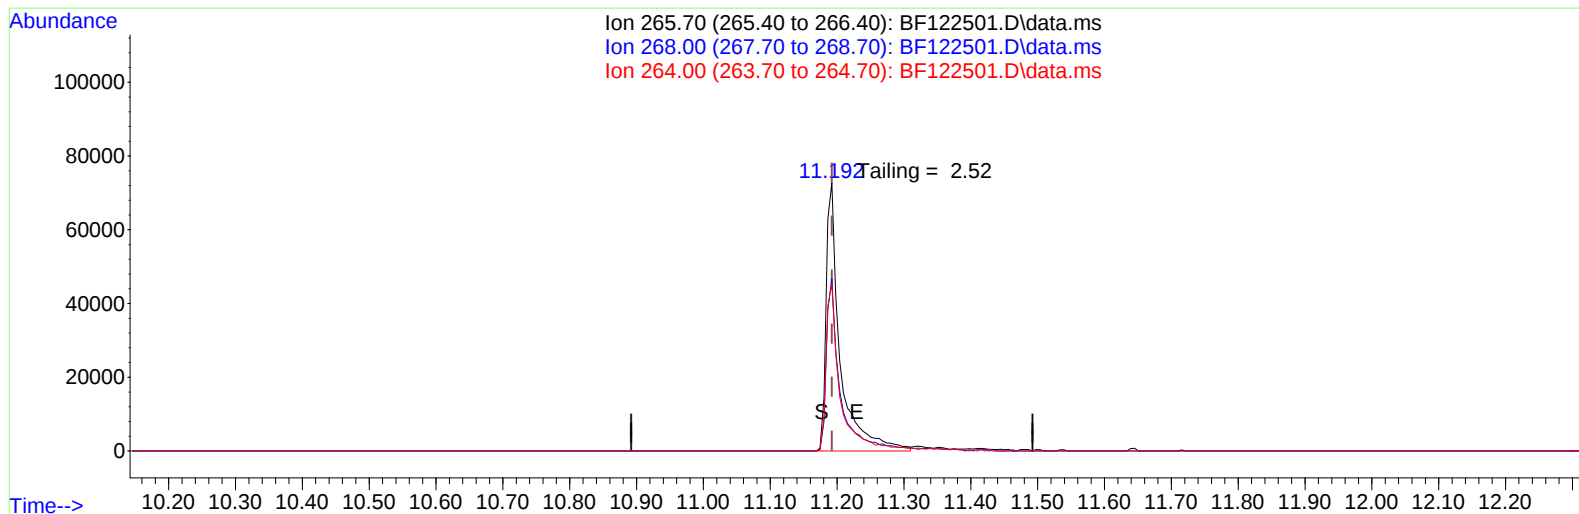

TIC: BF122501.D\data.ms

(70) Pentachlorophenol (C)




11.192min (-0.000) 31021.43 ng

response 107330

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	64.08
264.00	62.40	62.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113020\
Data File : BF122501.D
Acq On : 30 Nov 2020 11:15
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 01:13:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 14:38:56 2020
Response via : Initial Calibration

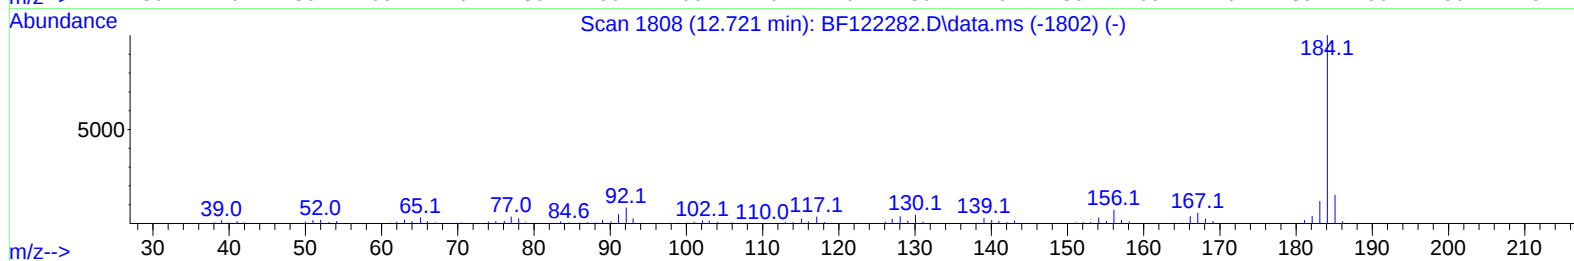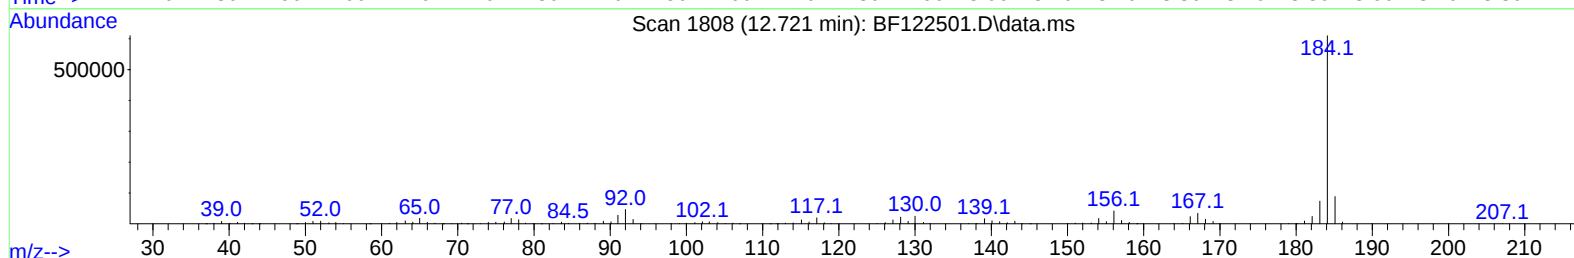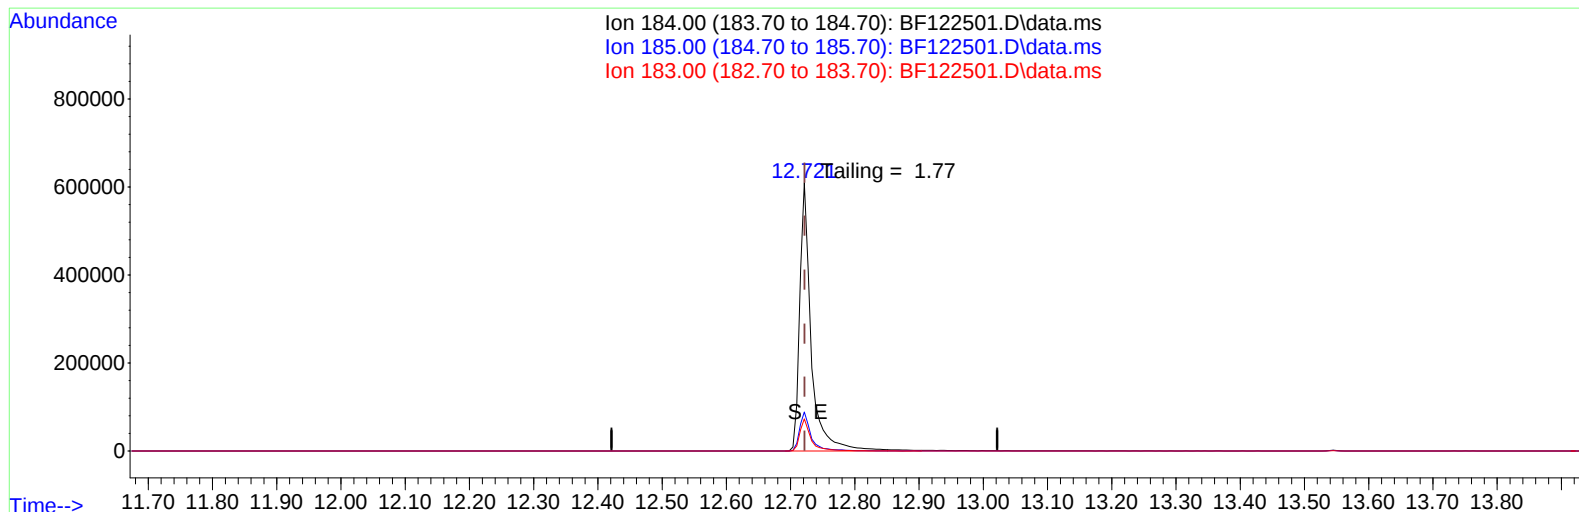

TIC: BF122501.D\data.ms

(77) Benzidine

12.721min (-0.000) 0.00 ng

response 766928

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.54
183.00	11.70	12.02
0.00	0.00	0.00