

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113020\
 Data File : BF122513.D
 Acq On : 30 Nov 2020 18:30
 Operator : JU/CG
 Sample : L4903-03 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-1-2-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.193	14	18	25	rVB5	22285	39425	1.77%	0.193%
2	5.051	502	504	510	rVB	31029	32059	1.44%	0.157%
3	5.469	571	575	588	rBV	1836323	1655917	74.54%	8.087%
4	6.481	743	747	764	rBV	1808550	1874505	84.38%	9.155%
5	6.857	807	811	814	rBV	1351267	1081961	48.71%	5.284%
6	7.416	902	906	917	rBV	1223678	1088401	49.00%	5.315%
7	8.139	1025	1029	1035	rBV	1699340	1423513	64.08%	6.952%
8	9.216	1208	1212	1224	rBV	2519589	2197296	98.92%	10.731%
9	9.610	1276	1279	1289	rVB	159917	153878	6.93%	0.752%
10	9.898	1324	1328	1343	rVB	2133339	1776769	79.98%	8.677%
11	10.686	1458	1462	1473	rBV	1311268	1414422	63.67%	6.908%
12	10.804	1480	1482	1486	rVB3	33467	44607	2.01%	0.218%
13	11.251	1554	1558	1561	rBV3	28073	35172	1.58%	0.172%
14	11.280	1561	1563	1568	rVB2	36367	35845	1.61%	0.175%
15	11.386	1577	1581	1587	rBV	1851103	1772496	79.79%	8.656%
16	11.910	1667	1670	1673	rBV3	75568	68142	3.07%	0.333%
17	12.363	1744	1747	1753	rBV	99473	109938	4.95%	0.537%
18	12.698	1802	1804	1807	rBV4	72925	64178	2.89%	0.313%
19	12.969	1846	1850	1854	rBV	2465274	2221393	100.00%	10.849%
20	14.027	2026	2030	2034	rBV	1665582	1560701	70.26%	7.622%
21	15.510	2278	2282	2293	rVB	1159340	1825391	82.17%	8.915%




Sum of corrected areas: 20476009

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113020\
Data File : BF122513.D
Acq On : 30 Nov 2020 18:30
Operator : JU/CG
Sample : L4903-03 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-1-2-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

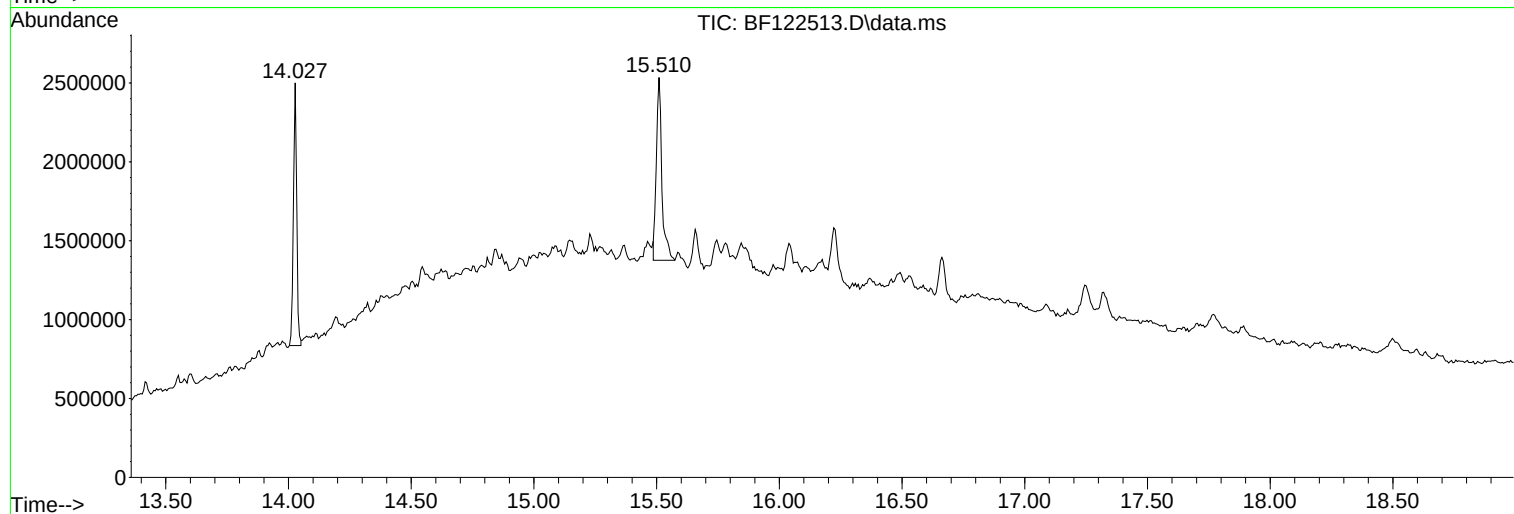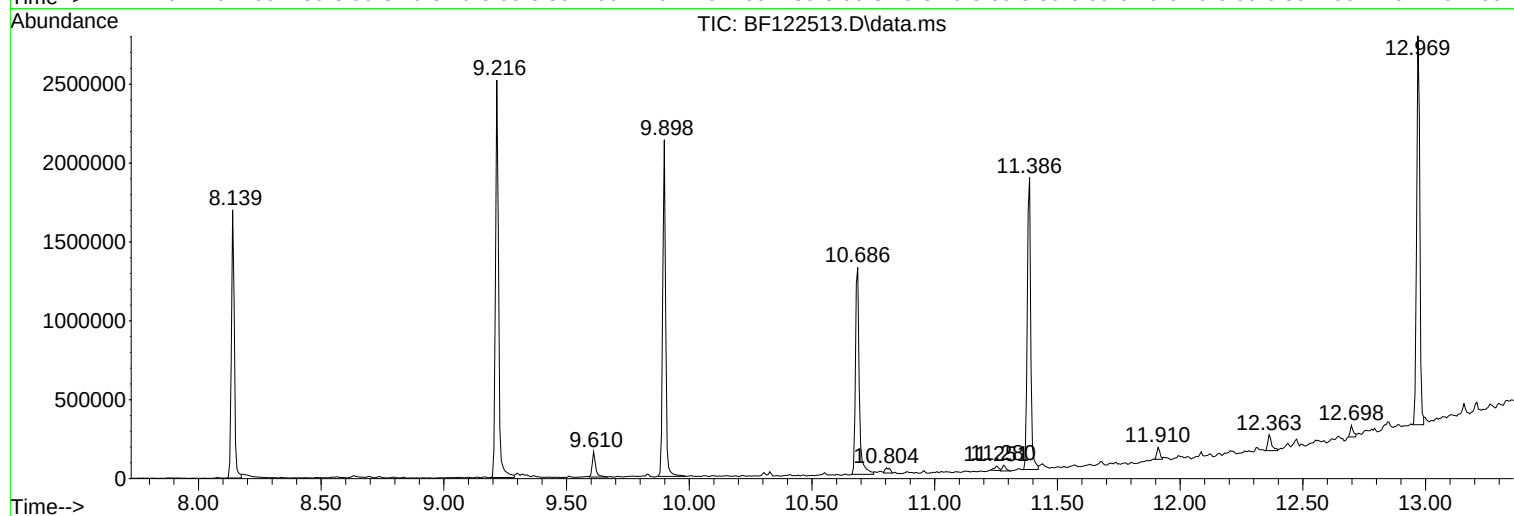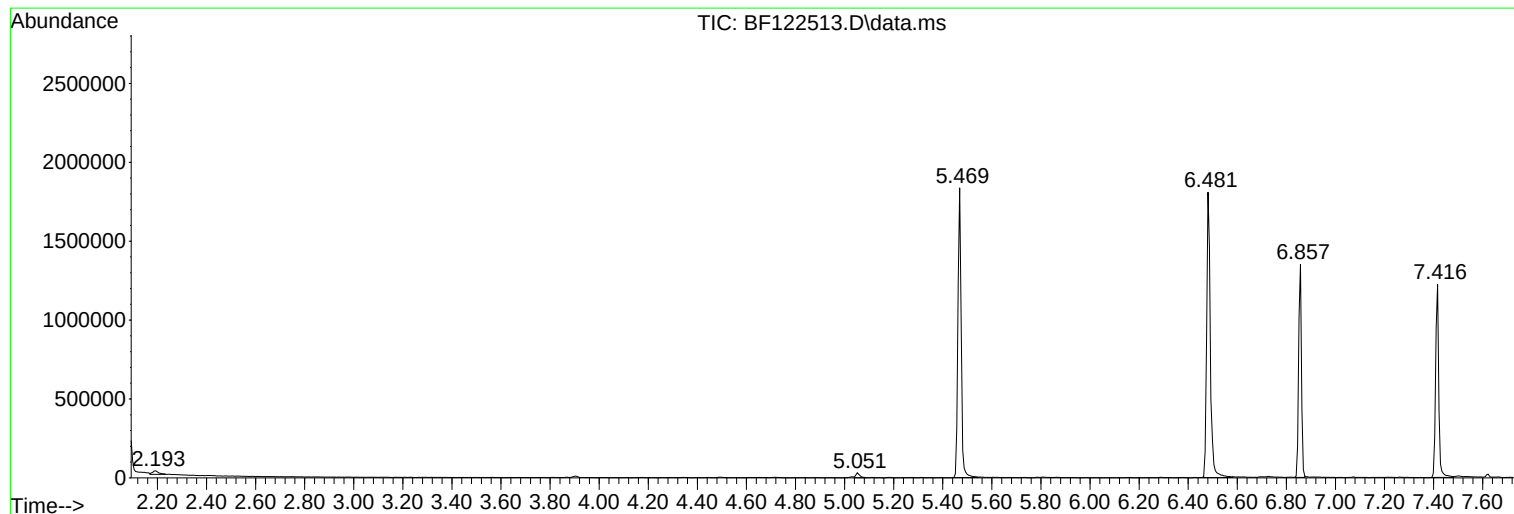

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113020\
Data File : BF122513.D
Acq On : 30 Nov 2020 18:30
Operator : JU/CG
Sample : L4903-03 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-1-2-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113020\
Data File : BF122513.D
Acq On : 30 Nov 2020 18:30
Operator : JU/CG
Sample : L4903-03 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-1-2-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------