
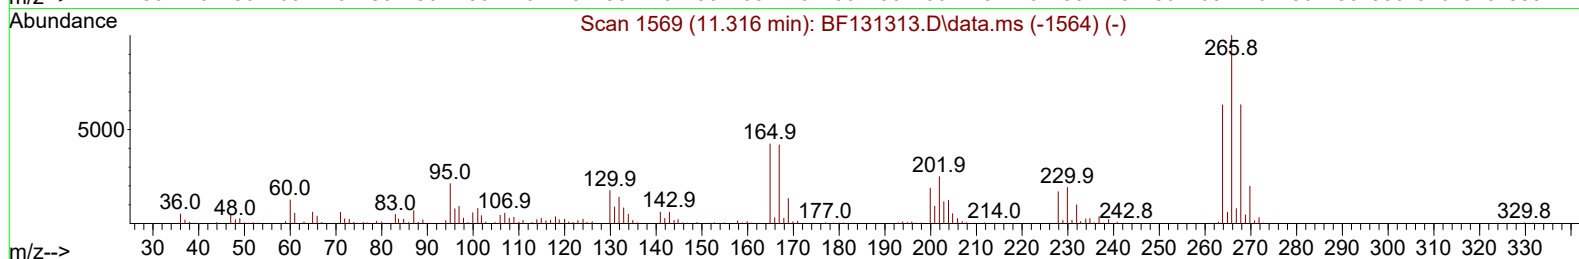
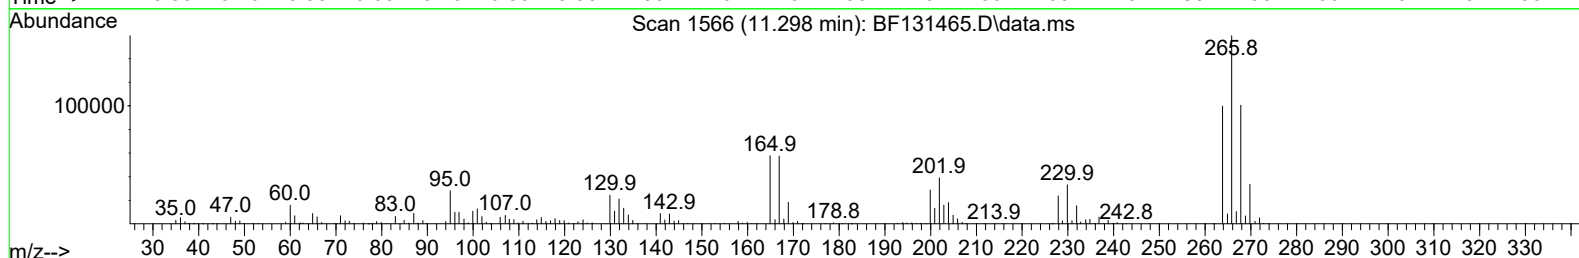


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113022\  
Data File : BF131465.D  
Acq On    : 30 Nov 2022  09:31  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 01 04:31:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 01 01:09:58 2022
Response via : Initial Calibration

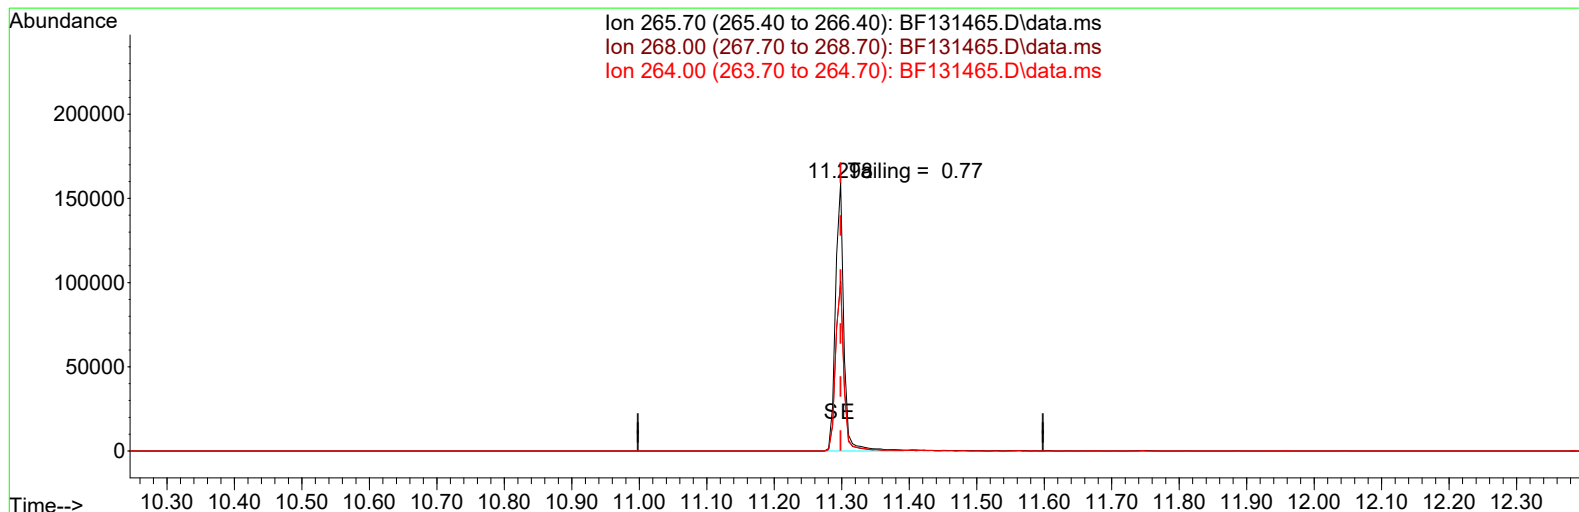

TIC: BF131465.D\data.ms

(70) Pentachlorophenol (C)




11.298min (+ 0.000) 31166.31 ng

response **137706**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	63.09
264.00	63.00	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF113022\
Data File : BF131465.D
Acq On : 30 Nov 2022 09:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 04:31:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 01 01:09:58 2022
Response via : Initial Calibration

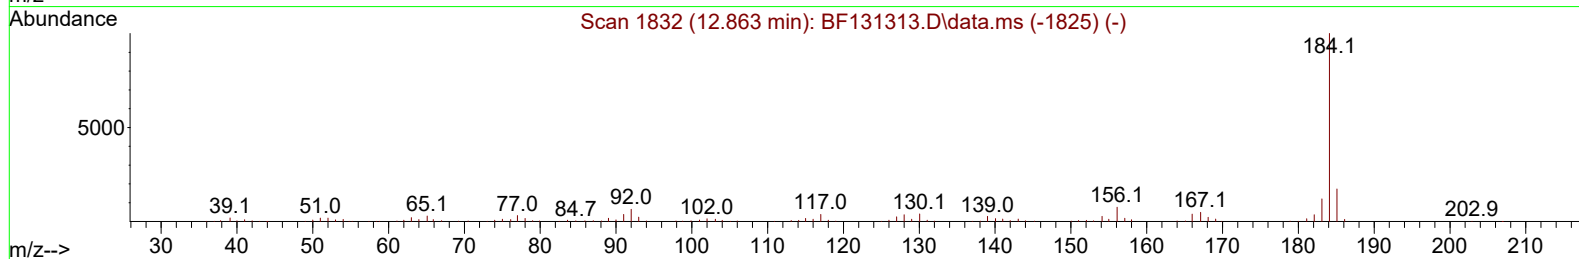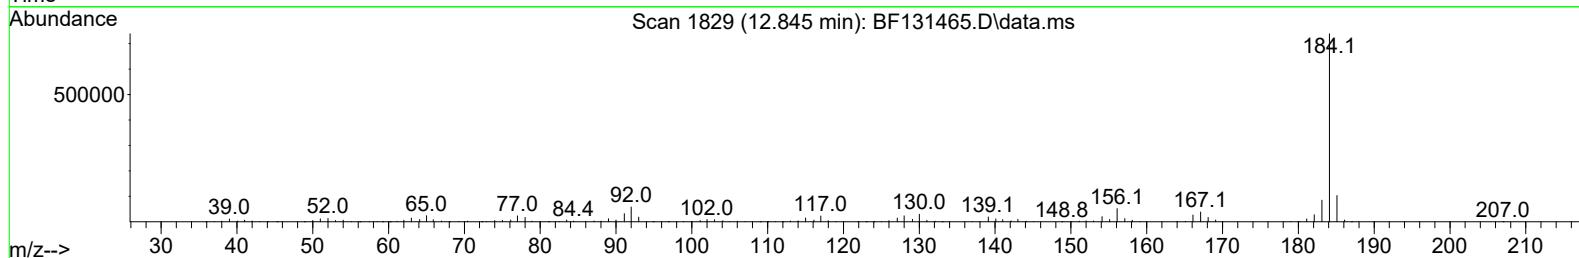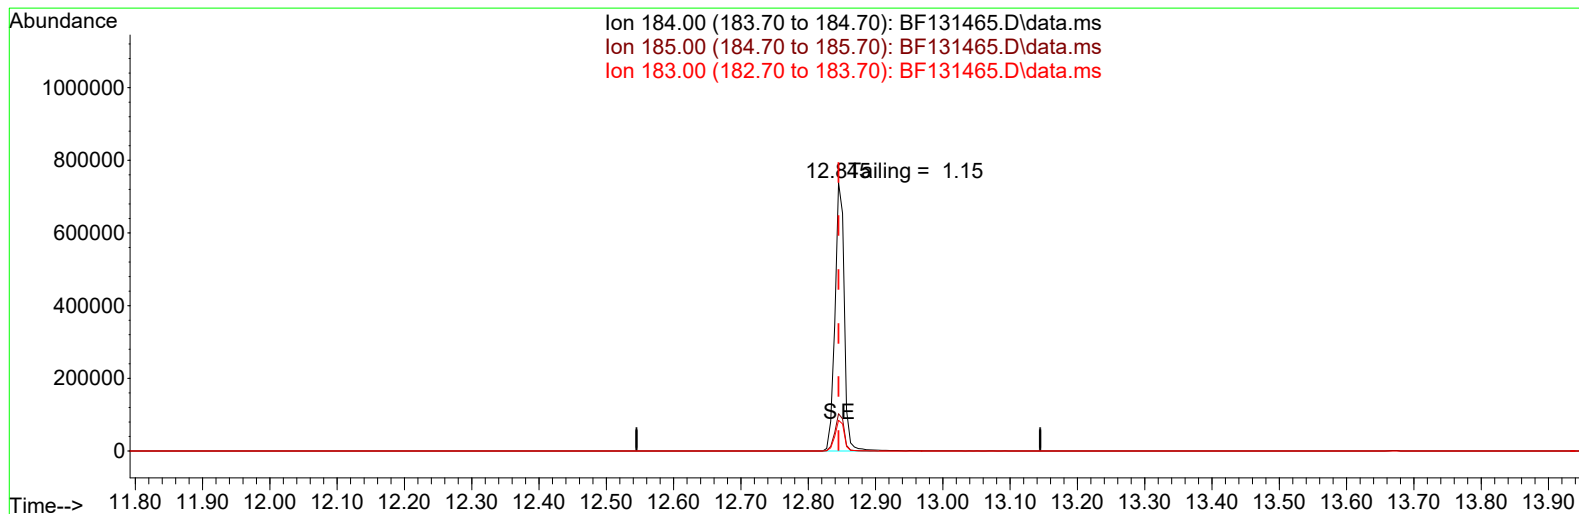

TIC: BF131465.D\data.ms

(77) Benzidine

12.845min (+ 0.000) 0.00 ng

response 709142

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	13.94
183.00	12.00	11.49
0.00	0.00	0.00